


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080521\
 Data File : BF124941.D
 Acq On : 5 Aug 2021 8:58
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 06 11:27:24 2021

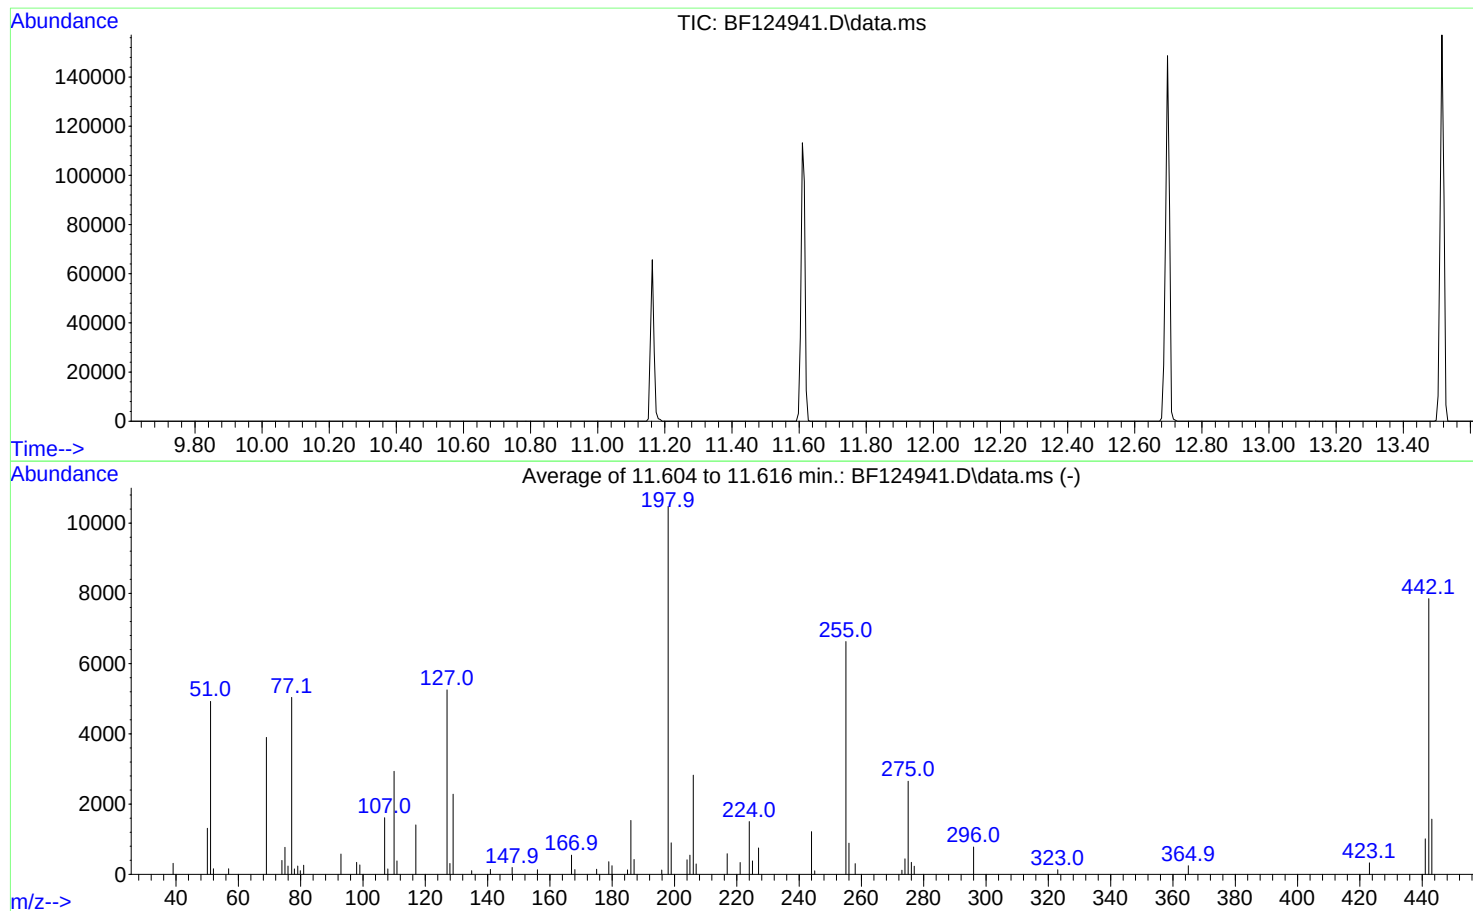




AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.0	4926	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.2	3900	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.2	5254	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	10473	PASS
199	198	5	9	8.6	896	PASS
275	198	10	60	25.3	2651	PASS
365	198	1	100	2.3	245	PASS
441	198	0.01	100	9.7	1013	PASS
442	442	50	100	100.0	7851	PASS
443	442	15	24	20.0	1574	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080521\
 Data File : BF124941.D
 Acq On : 5 Aug 2021 8:58
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 05 10:56:08 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 04 17:59:00 2021
 Response via : Initial Calibration

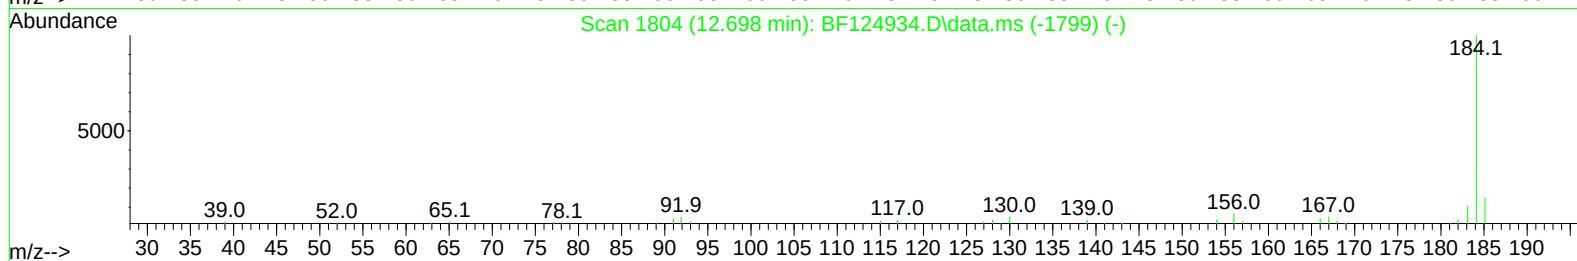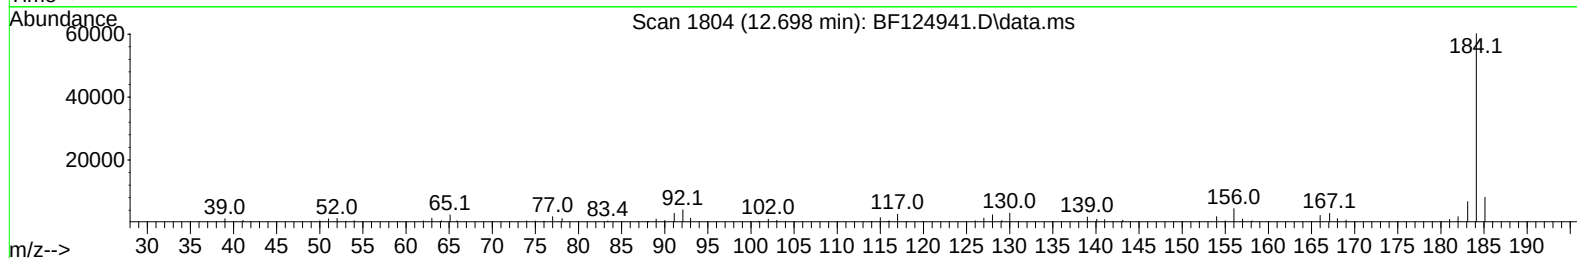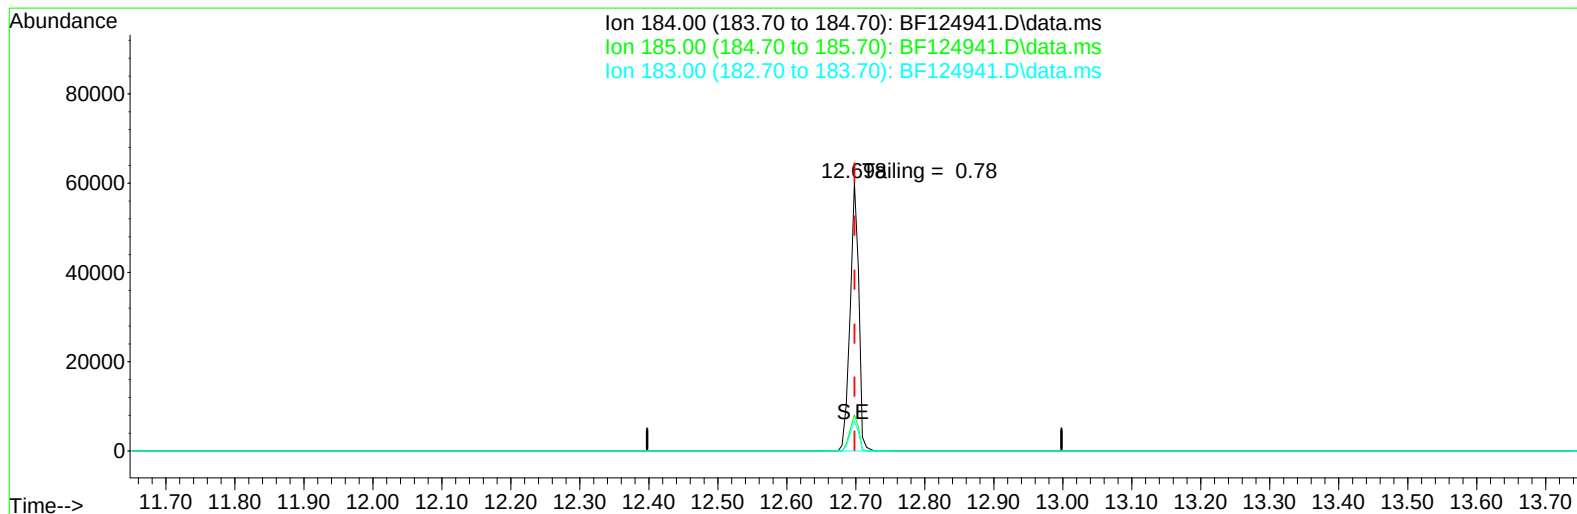

TIC: BF124941.D\data.ms

(77) Benzidine

12.698min (-0.000) 0.00 ng




response 52364

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.50
183.00	10.10	11.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080521\
Data File : BF124941.D
Acq On : 5 Aug 2021 8:58
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 05 10:56:08 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 04 17:59:00 2021
Response via : Initial Calibration

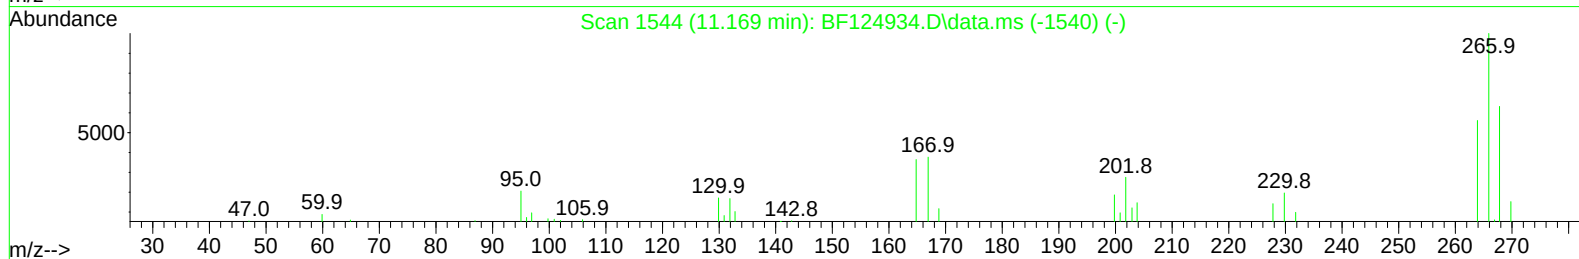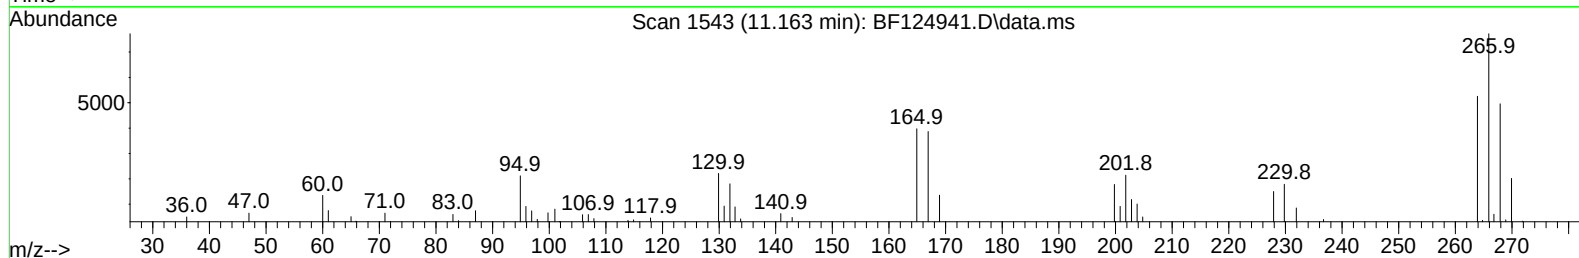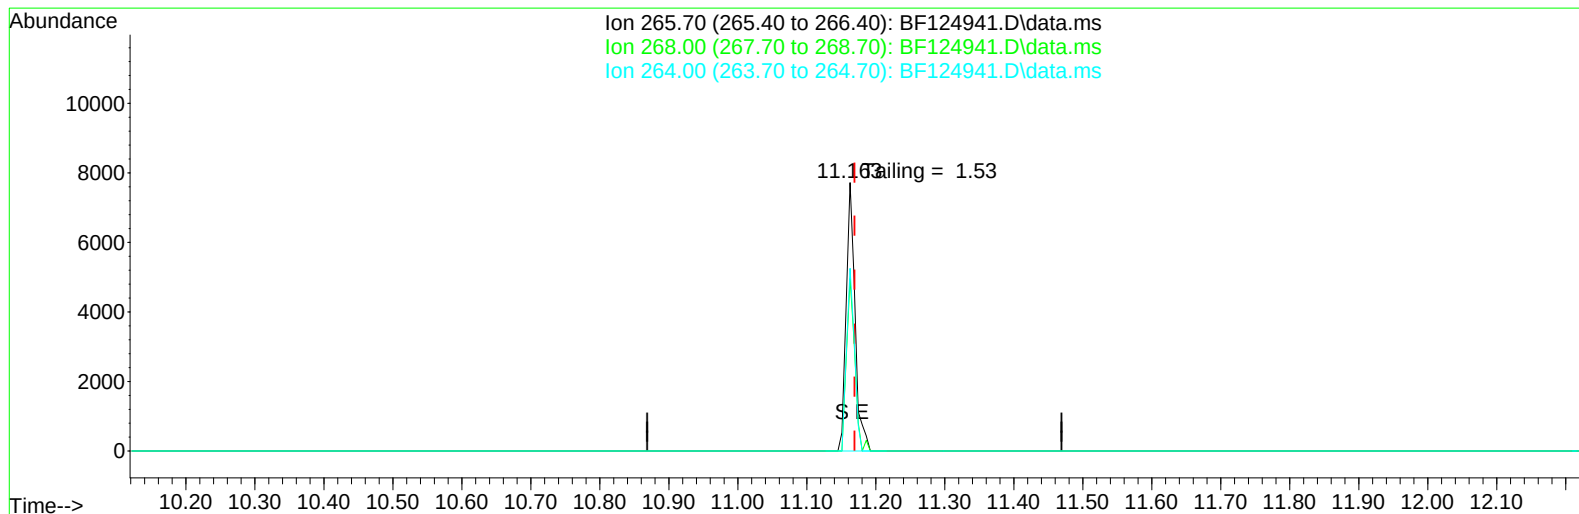

TIC: BF124941.D\data.ms

(70) Pentachlorophenol (C)

11.163min (-0.006) 0.00 ng

response 6882

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	64.20
264.00	69.90	68.01
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/5/2021	BNA_F	<u>BF124941.D</u>
Compound Name	Response	Retention Time
DDT	25293	13.51
DDD	0	13.3
DDE	0	12.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
0	25293	0.00

Instrument :
BNA_F
ClientSampleId :
DFTPP