
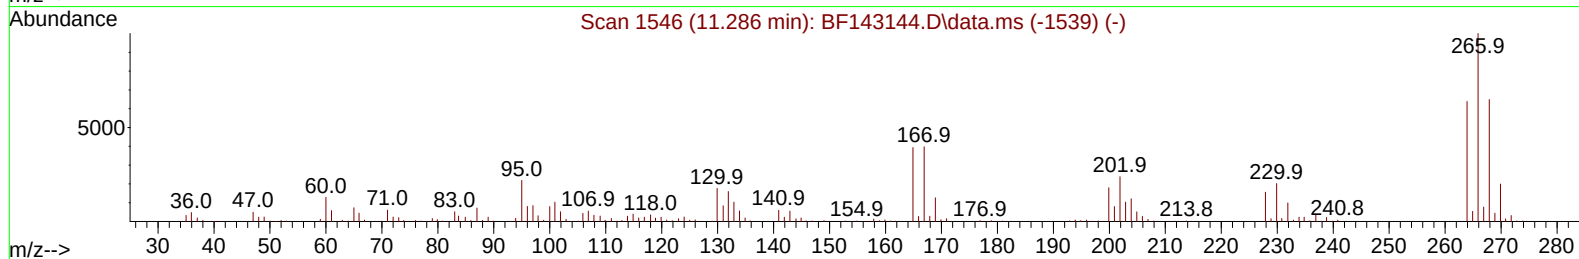
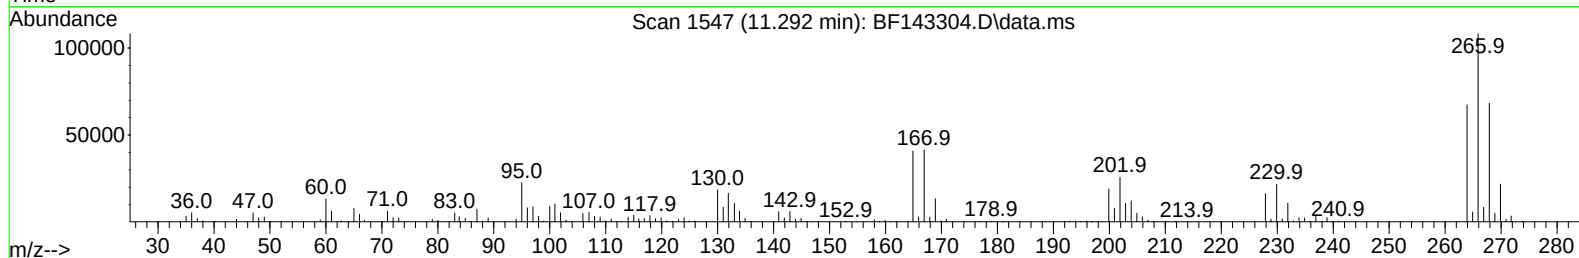


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143304.D
Acq On : 05 Aug 2025 09:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 05 10:59:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

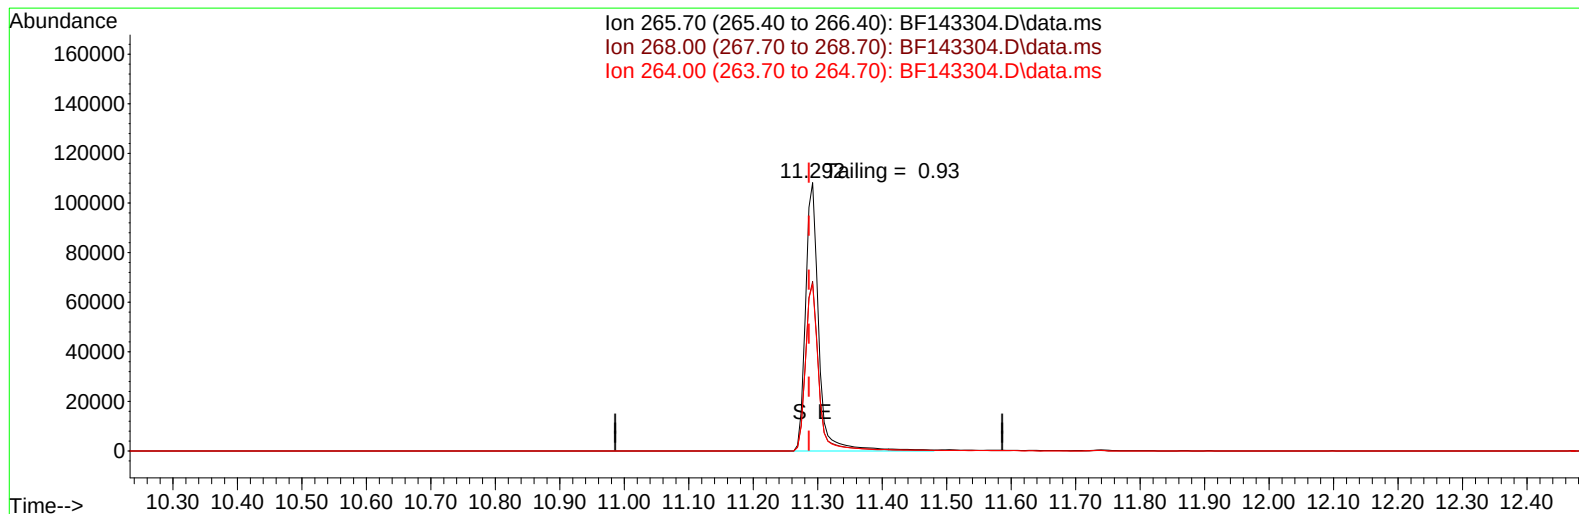

TIC: BF143304.D\data.ms

(70) Pentachlorophenol (C)




11.292min (+ 0.006) 26944.60 ng

response 154742

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.16
264.00	63.80	62.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143304.D
Acq On : 05 Aug 2025 09:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 05 10:59:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

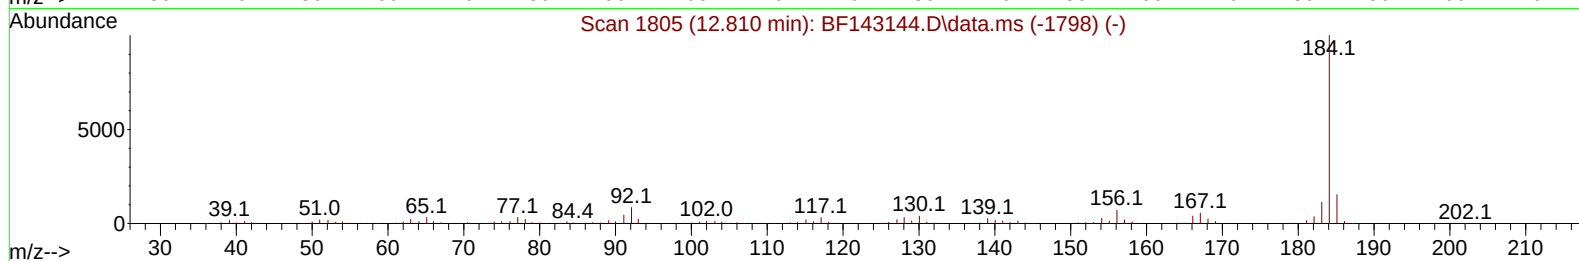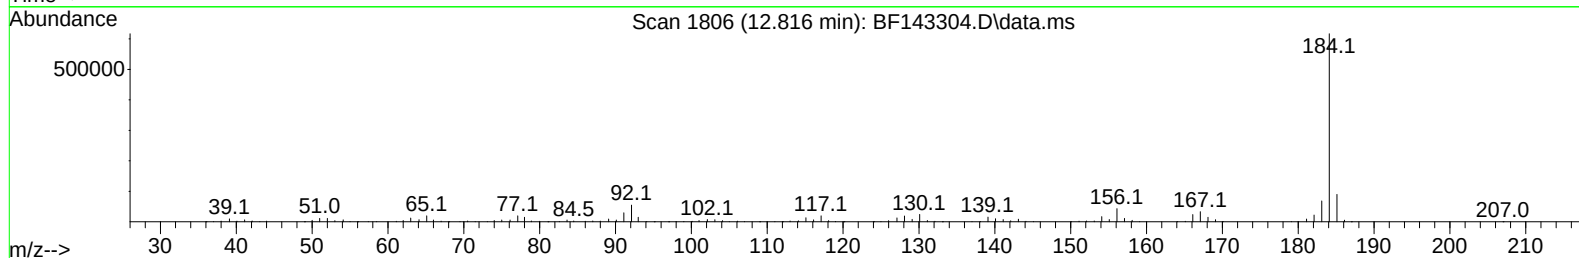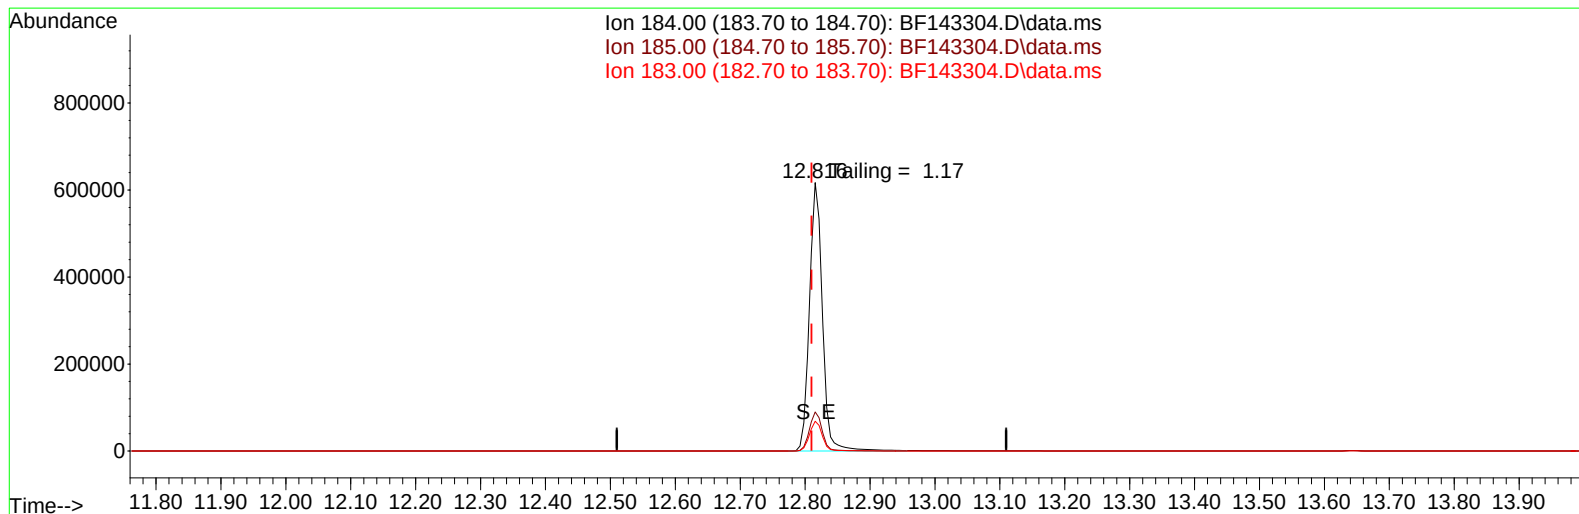

TIC: BF143304.D\data.ms

(77) Benzidine

12.816min (+ 0.006) 0.00 ng

response 856718

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.56
183.00	11.20	11.12
0.00	0.00	0.00