


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080615\
 Data File : BF080881.D
 Acq On : 6 Aug 2015 9:53
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 07 03:17:12 2015

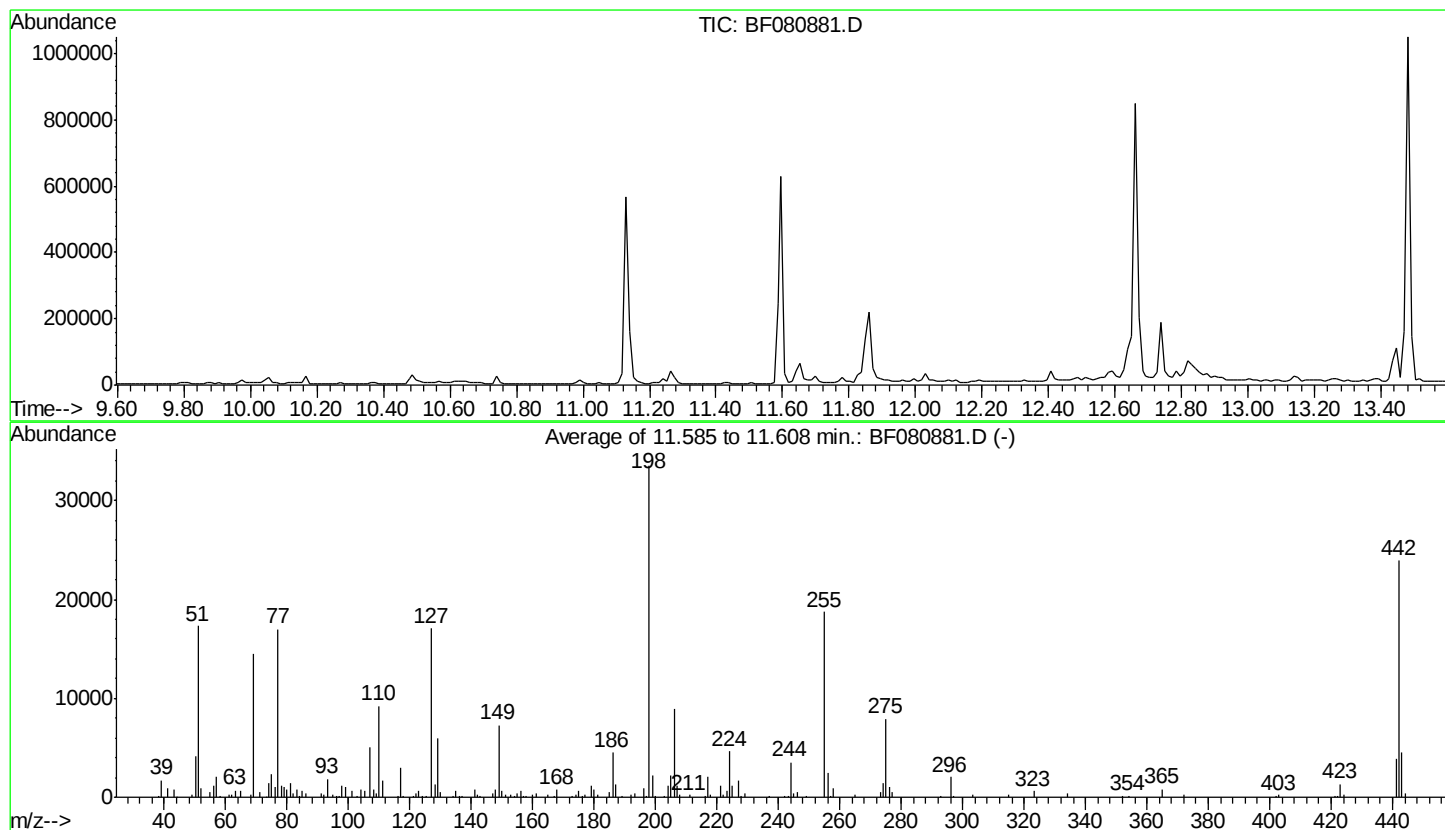

AutoFind: Scans 831, 832, 833; Background Corrected with Scan 828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.7	17349	PASS
68	69	0.00	2	1.7	248	PASS
69	198	0.00	100	43.2	14490	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.9	17082	PASS
197	198	0.00	2	0.5	162	PASS
198	198	100	100	100.0	33543	PASS
199	198	5	9	6.4	2157	PASS
275	198	10	60	23.7	7955	PASS
365	198	1	100	2.3	784	PASS
441	442	0.01	24	16.2	3878	PASS
442	198	50	100	71.3	23927	PASS
443	442	15	24	18.7	4478	PASS