

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF080620\  
 Data File : BF121216.D  
 Acq On : 6 Aug 2020 22:14  
 Operator : JU/CG  
 Sample : L3574-03 2X  
 Misc :  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 FK-GF-02-060-B

Quant Time: Aug 07 00:33:34 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Jul 29 14:55:43 2020  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|---------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 6.79  | 152  | 142268   | 20.00 | ng    | -0.01    |
| 21) Naphthalene-d8        | 8.07  | 136  | 539472   | 20.00 | ng    | -0.01    |
| 39) Acenaphthene-d10      | 9.83  | 164  | 277892   | 20.00 | ng    | 0.00     |
| 64) Phenanthrene-d10      | 11.32 | 188  | 504959   | 20.00 | ng    | 0.00     |
| 76) Chrysene-d12          | 13.96 | 240  | 342458   | 20.00 | ng    | 0.00     |
| 86) Perylene-d12          | 15.42 | 264  | 366300   | 20.00 | ng    | 0.01     |

## System Monitoring Compounds

|                          |       |     |        |       |    |       |
|--------------------------|-------|-----|--------|-------|----|-------|
| 5) 2-Fluorophenol        | 5.40  | 112 | 338441 | 39.00 | ng | -0.01 |
| 7) Phenol-d6             | 6.43  | 99  | 411525 | 36.71 | ng | -0.02 |
| 23) Nitrobenzene-d5      | 7.35  | 82  | 260227 | 27.91 | ng | -0.02 |
| 42) 2,4,6-Tribromophenol | 10.62 | 330 | 113009 | 37.15 | ng | -0.01 |
| 45) 2-Fluorobiphenyl     | 9.15  | 172 | 519084 | 27.89 | ng | -0.01 |
| 79) Terphenyl-d14        | 12.90 | 244 | 432748 | 27.47 | ng | 0.00  |

## Target Compounds


|                                |       |     |        |           |   | Qvalue |
|--------------------------------|-------|-----|--------|-----------|---|--------|
| 9) Benzaldehyde                | 6.43  | 77  | 360    | Below Cal | # | 1      |
| 19) n-Nitroso-di-n-propylamine | 7.35  | 70  | 34925  | 5.479 ng  | # | 78     |
| 25) Isophorone                 | 7.35  | 82  | 257402 | 13.834 ng | # | 62     |
| 50) Dimethylphthalate          | 9.55  | 163 | 67877  | 3.386 ng  |   | 99     |
| 51) 2,6-Dinitrotoluene         | 9.83  | 165 | 35989  | 8.356 ng  | # | 27     |
| 57) 2,4-Dinitrotoluene         | 9.83  | 165 | 36391  | 6.434 ng  | # | 29     |
| 65) 4,6-Dinitro-2-methylphenol | 10.62 | 198 | 108    | 3.877 ng  | # | 83     |
| 71) Phenanthrene               | 11.34 | 178 | 54490  | 2.098 ng  |   | 98     |
| 75) Fluoranthene               | 12.53 | 202 | 149645 | 5.199 ng  |   | 99     |
| 78) Pyrene                     | 12.76 | 202 | 143355 | 5.921 ng  |   | 98     |
| 81) Benzo(a)anthracene         | 13.95 | 228 | 82116  | 3.960 ng  |   | 95     |
| 83) Chrysene                   | 13.99 | 228 | 78922  | 3.621 ng  |   | 96     |
| 87) Indeno(1,2,3-cd)pyrene     | 16.84 | 276 | 51560  | 2.024 ng  |   | 96     |
| 88) Benzo(b)fluoranthene       | 14.99 | 252 | 160119 | 7.232 ng  | # | 92     |
| 89) Benzo(k)fluoranthene       | 14.99 | 252 | 160119 | 7.929 ng  | # | 93     |
| 90) Benzo(a)pyrene             | 15.35 | 252 | 87192  | 4.316 ng  |   | 97     |
| 92) Benzo(a,h,i)perylene       | 17.27 | 276 | 48446  | 2.361 ng  |   | 96     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF080620\  
Data File : BF121216.D  
Acq On : 6 Aug 2020 22:14  
Operator : JU/CG  
Sample : L3574-03 2X  
Misc :  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
FK-GF-02-060-B

Quant Time: Aug 07 00:33:34 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jul 29 14:55:43 2020  
Response via : Initial Calibration

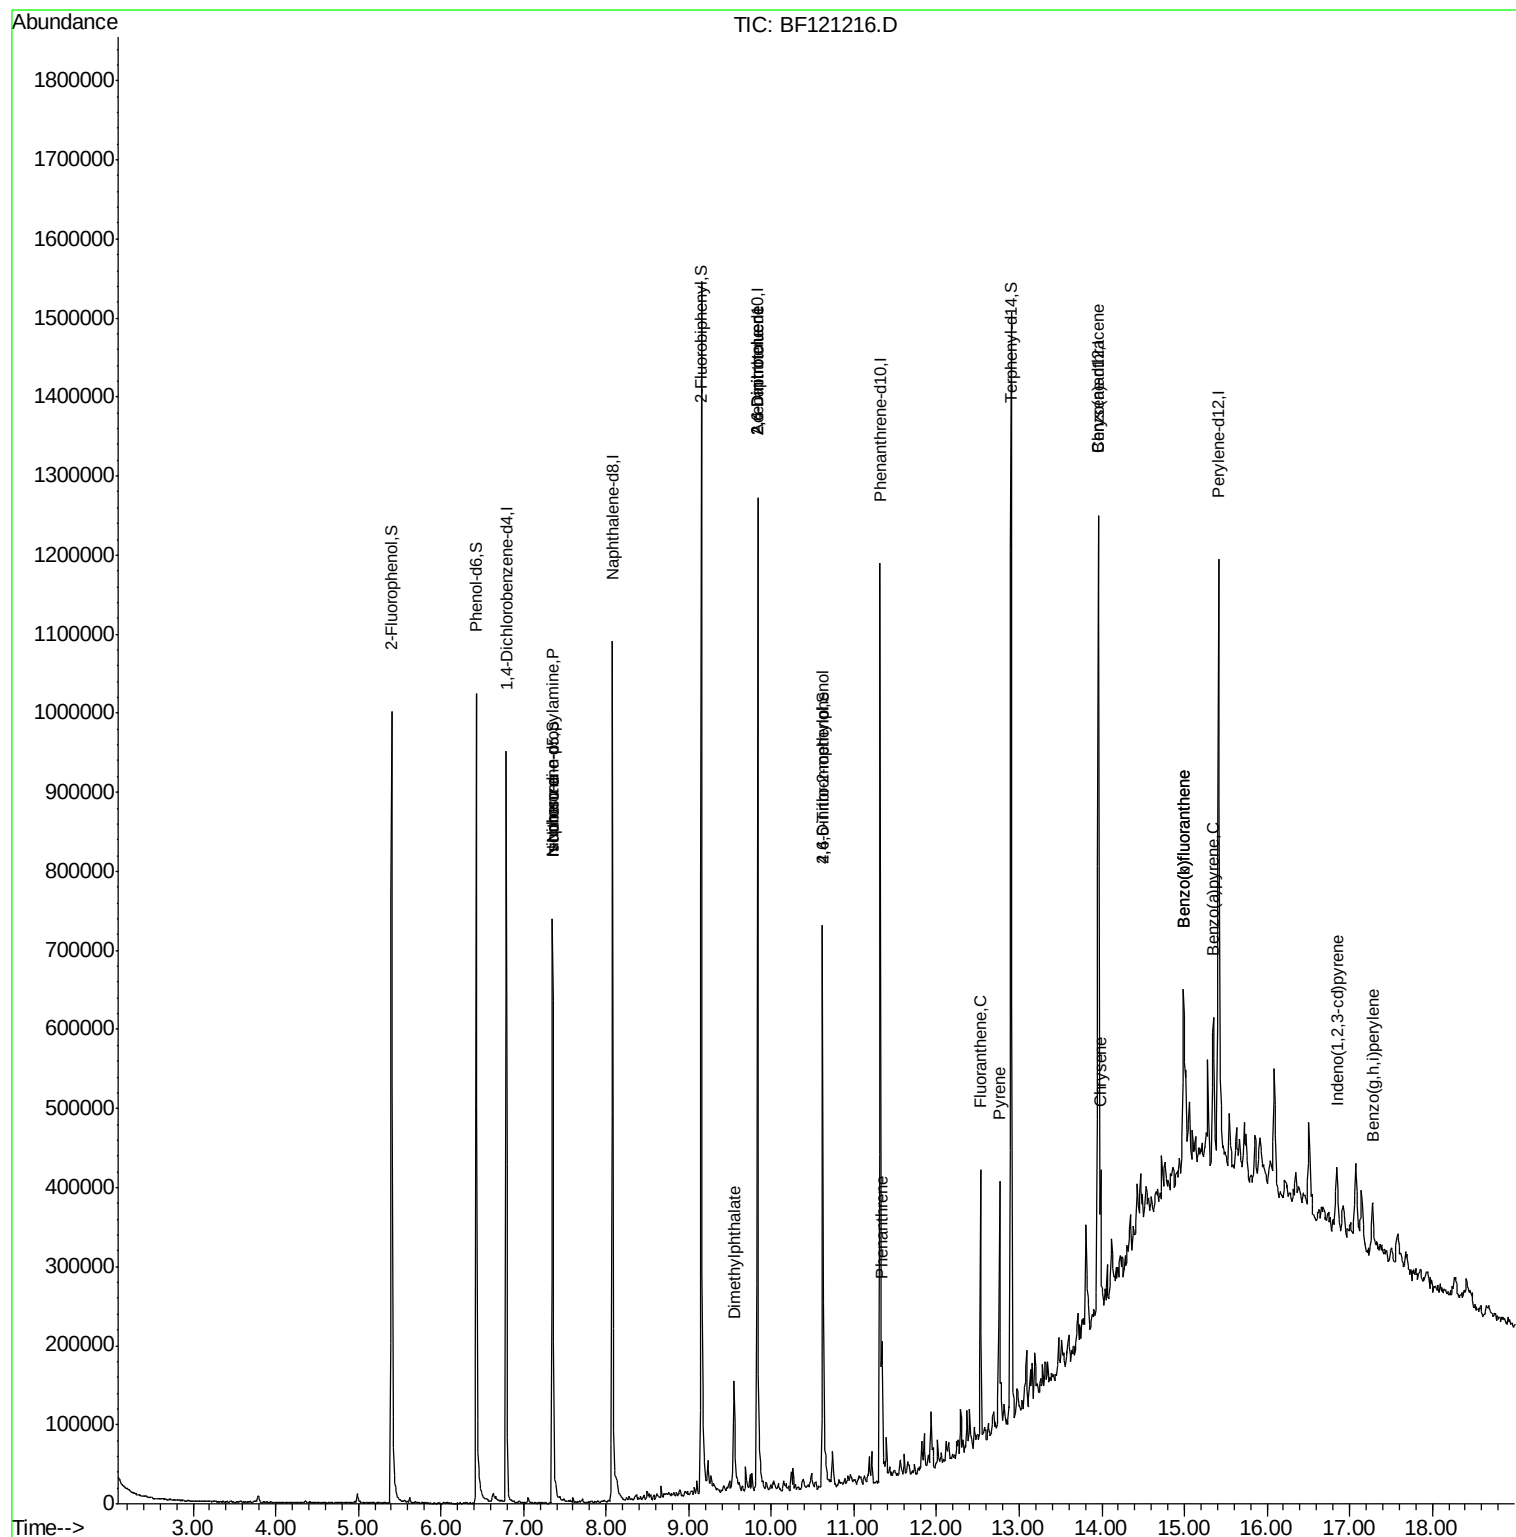

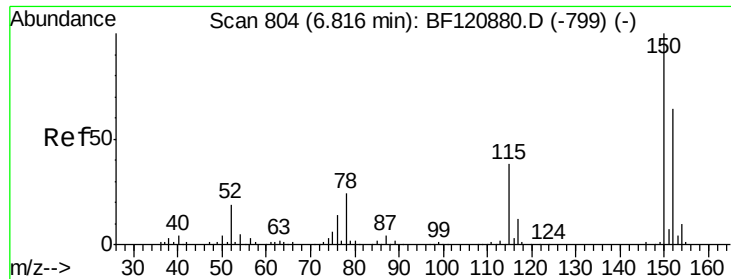


#1




1,4-Dichlorobenzene-d4  
Concen: 20.000 ng  
RT: 6.79 min Scan# 800  
Delta R.T. -0.01 min  
Lab File: BF121216.D  
Acq: 6 Aug 2020 22:14

Instrument :  
BNA\_F  
ClientSampleId :  
FK-GF-02-060-B

Tot Ion:152 Resp: 142268  
Ion Ratio Lower Upper  
152 100  
150 155.3 125.6 188.4  
115 56.1 46.2 69.2




Abundance Ion 152.00 (151.70 to 152.70): E  
Ion 150.00 (149.70 to 150.70): E  
Ion 115.00 (114.70 to 115.70): E

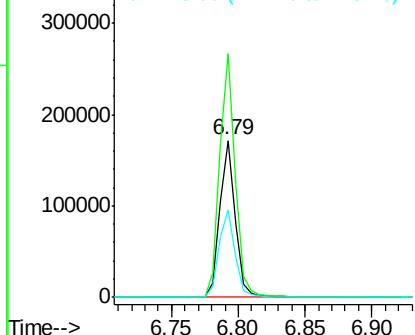



#5




2-Fluorophenol  
Concen: 38.999 ng  
RT: 5.40 min Scan# 564  
Delta R.T. -0.01 min  
Lab File: BF121216.D  
Acq: 6 Aug 2020 22:14

Tgt Ion:112 Resp: 338441  
Ion Ratio Lower Upper  
112 100  
64 54.5 43.9 65.9  
63 27.3 22.7 34.1



Abundance Ion 112.00 (111.70 to 112.70): E  
Ion 64.00 (63.70 to 64.70): BF1  
Ion 63.00 (62.70 to 63.70): BF1

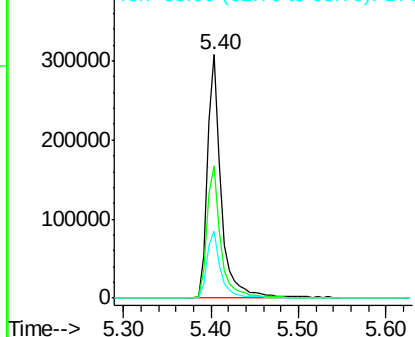

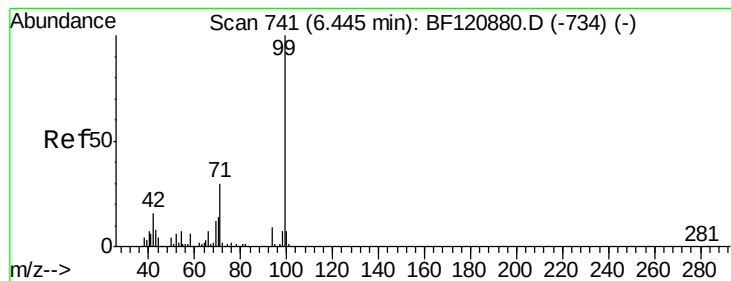

#7

Phenol-d6

Concen: 36.710 ng

RT: 6.43 min Scan# 738

Delta R.T. -0.02 min

Lab File: BF121216.D

Acq: 6 Aug 2020 22:14

Instrument :

BNA\_F

ClientSampleId :

FK-GF-02-060-B





Tot Ion: 99 Resp: 411525

Ion Ratio Lower Upper

99 100

42 16.3 13.5 20.3

71 29.6 25.0 37.4

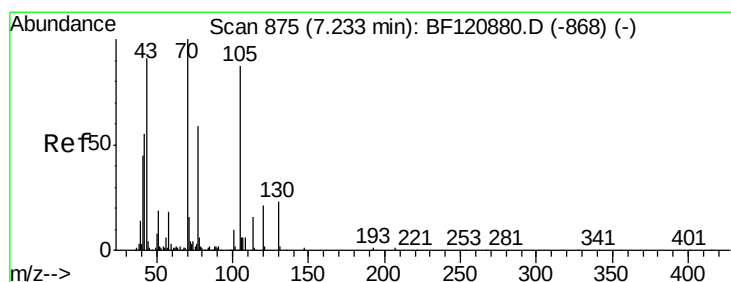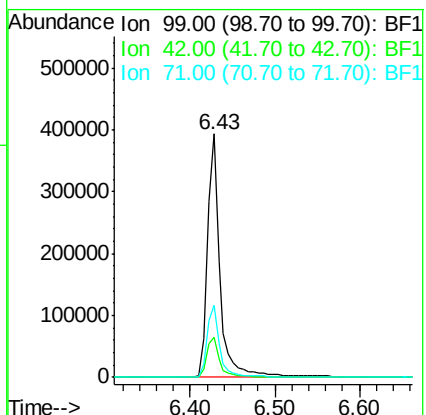

#19

n-Nitroso-di-n-propylamine

Concen: 5.479 ng

RT: 7.35 min Scan# 895

Delta R.T. 0.12 min

Lab File: BF121216.D

Acq: 6 Aug 2020 22:14

Tgt Ion: 70 Resp: 34925


Ion Ratio Lower Upper


70 100

42 46.5 43.3 64.9

101 0.0 8.4 12.6#

130 2.0 18.7 28.1#

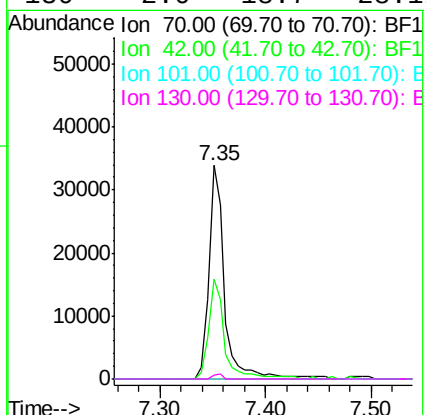

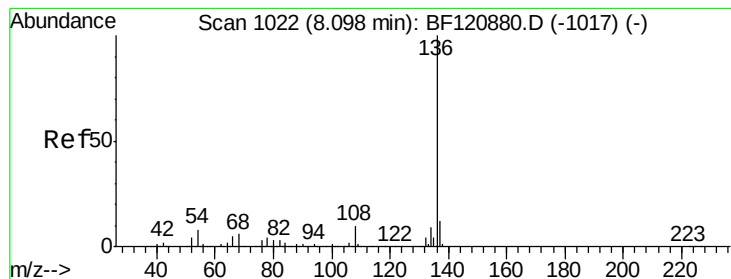

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.07 min Scan# 1018

Delta R.T. -0.01 min

Lab File: BF121216.D

Acq: 6 Aug 2020 22:14

Instrument :

BNA\_F

ClientSampleId :

FK-GF-02-060-B

Tot Ion:136 Resp: 539472



Ion Ratio Lower Upper

136 100

137 11.2 9.0 13.4

54 7.8 6.1 9.1

68 6.0 5.0 7.6



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

8.07


600000

400000

200000

0

Time-->

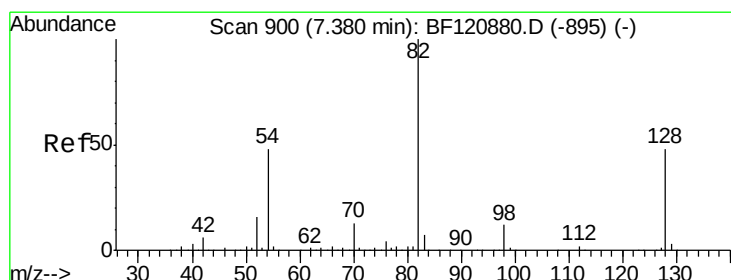

#23

Nitrobenzene-d5

Concen: 27.912 ng

RT: 7.35 min Scan# 895

Delta R.T. -0.02 min

Lab File: BF121216.D

Acq: 6 Aug 2020 22:14



Tgt Ion: 82 Resp: 260227

Ion Ratio Lower Upper

82 100

128 44.4 39.2 58.8

54 50.3 37.8 56.8



Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

7.35


300000

200000

100000

0





Time-->

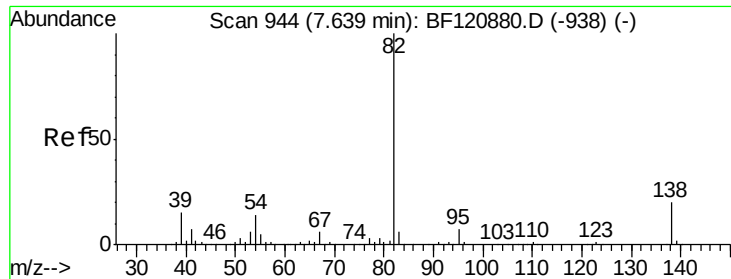

#25  
Isophorone  
Concen: 13.834 ng  
RT: 7.35 min Scan# 895  
Delta R.T. -0.28 min  
Lab File: BF121216.D  
Acq: 6 Aug 2020 22:14




Instrument :  
BNA\_F  
ClientSampleId :  
FK-GF-02-060-B


Tot Ion: 82 Resp: 257402  
Ion Ratio Lower Upper  
82 100  
95 0.0 5.5 8.3#  
138 0.0 16.2 24.2#

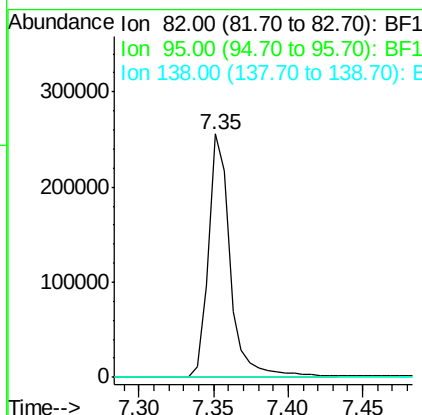

#39  
Acenaphthene-d10  
Concen: 20.000 ng  
RT: 9.83 min Scan# 1317  
Delta R.T. -0.01 min  
Lab File: BF121216.D  
Acq: 6 Aug 2020 22:14

Tgt Ion:164 Resp: 277892  
Ion Ratio Lower Upper  
164 100  
162 101.5 82.2 123.2  
160 45.6 37.2 55.8

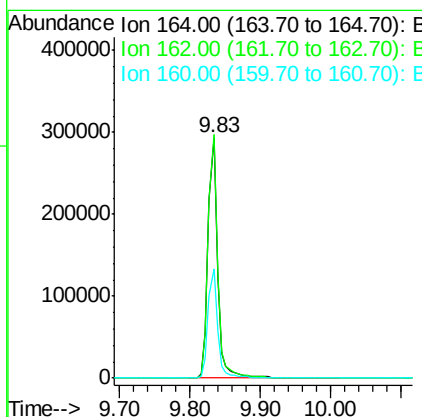

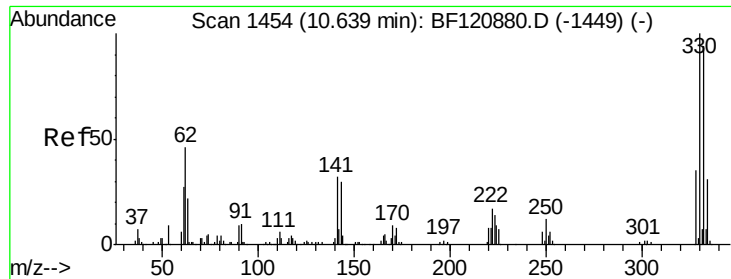

#42

2,4,6-Tribromophenol

Concen: 37.152 ng

RT: 10.62 min Scan# 1451

Delta R.T. -0.01 min

Lab File: BF121216.D

Acq: 6 Aug 2020 22:14

Instrument :

BNA\_F

ClientSampleId :

FK-GF-02-060-B


Tot Ion:330 Resp: 113009

Ion Ratio Lower Upper

330 100

332 95.7 76.1 114.1




141 33.0 24.1 36.1



Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

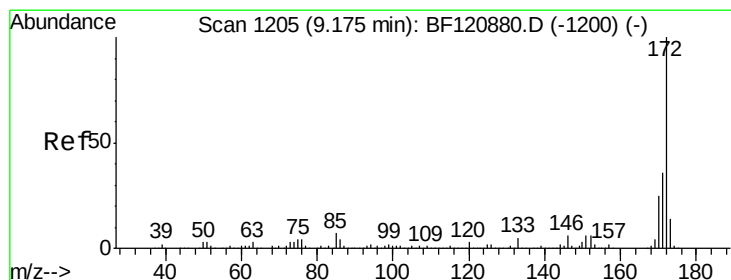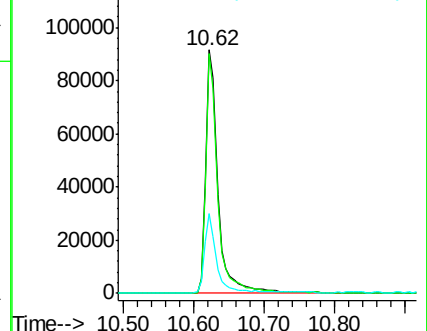

#45

2-Fluorobiphenyl

Concen: 27.889 ng

RT: 9.15 min Scan# 1201

Delta R.T. -0.01 min

Lab File: BF121216.D

Acq: 6 Aug 2020 22:14


Tgt Ion:172 Resp: 519084

Ion Ratio Lower Upper

172 100

171 34.8 29.0 43.4



170 23.8 19.6 29.4




Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

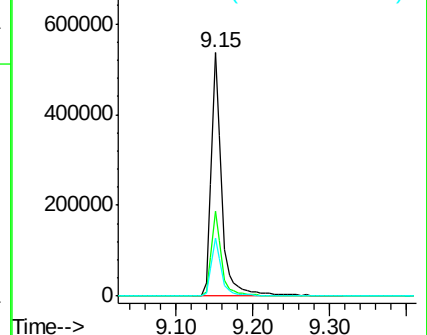



#50

Dimethylphthalate

Concen: 3.386 ng

RT: 9.55 min Scan# 1269

Delta R.T. -0.02 min

Lab File: BF121216.D

Acq: 6 Aug 2020 22:14

Instrument :

BNA\_F

ClientSampleId :

FK-GF-02-060-B


Tot Ion:163 Resp: 67877

Ion Ratio Lower Upper

163 100

194 4.2 3.0 4.4




164 10.0 8.4 12.6



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

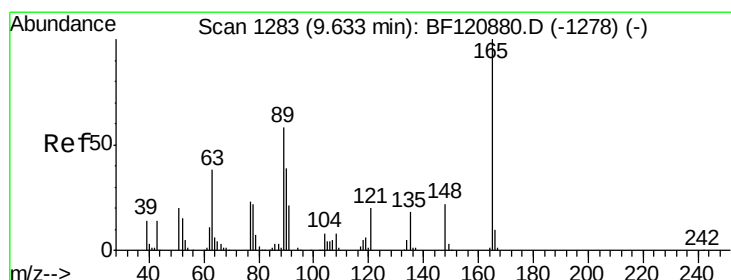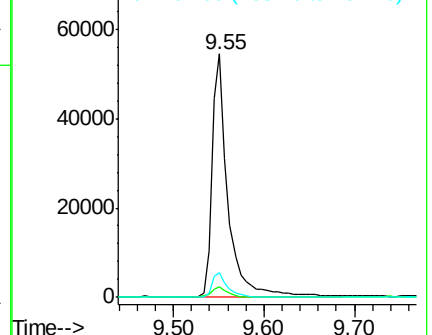

#51

2,6-Dinitrotoluene

Concen: 8.356 ng

RT: 9.83 min Scan# 1317

Delta R.T. 0.21 min

Lab File: BF121216.D

Acq: 6 Aug 2020 22:14


Tgt Ion:165 Resp: 35989

Ion Ratio Lower Upper

165 100

63 1.0 41.1 61.7#



89 1.1 43.5 65.3#




Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

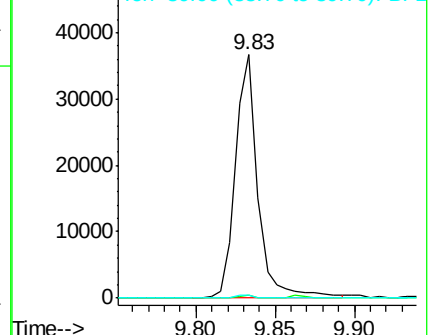




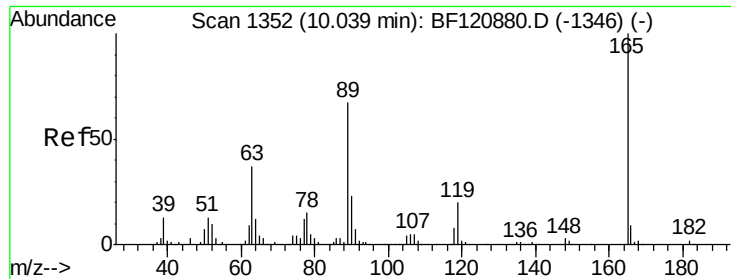

#57  
 2,4-Dinitrotoluene  
 Concen: 6.434 ng  
 RT: 9.83 min Scan# 1317  
 Delta R.T. -0.20 min  
 Lab File: BF121216.D  
 Acq: 6 Aug 2020 22:14

Instrument :  
 BNA\_F  
 ClientSampleId :  
 FK-GF-02-060-B

| Tot Ion:165 | Resp: | 36391       |
|-------------|-------|-------------|
| Ion         | Ratio | Lower Upper |
| 165         | 100   |             |
| 63          | 1.0   | 29.8 44.8#  |
| 89          | 1.1   | 50.3 75.5#  |
| 182         | 0.0   | 2.1 3.1#    |






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1


Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E

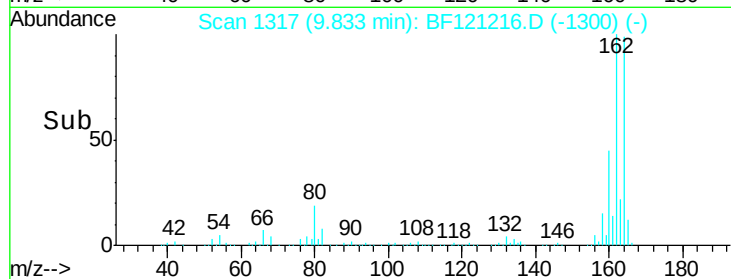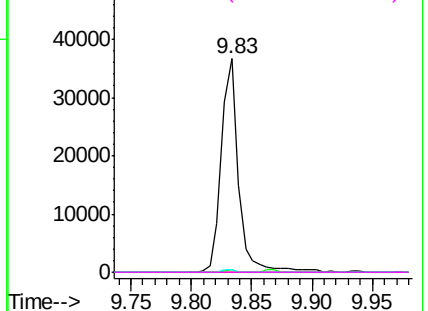

#64  
 Phenanthrene-d10  
 Concen: 20.000 ng  
 RT: 11.32 min Scan# 1569  
 Delta R.T. -0.01 min  
 Lab File: BF121216.D  
 Acq: 6 Aug 2020 22:14



| Tgt Ion:188 | Resp: | 504959      |
|-------------|-------|-------------|
| Ion         | Ratio | Lower Upper |
| 188         | 100   |             |
| 94          | 10.1  | 8.0 12.0    |
| 80          | 10.5  | 8.3 12.5    |




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

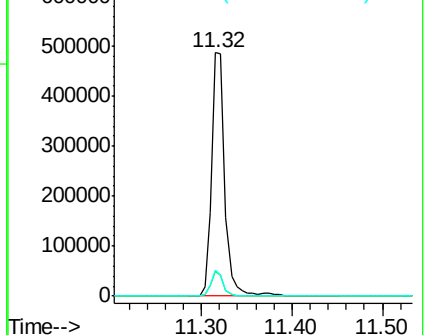


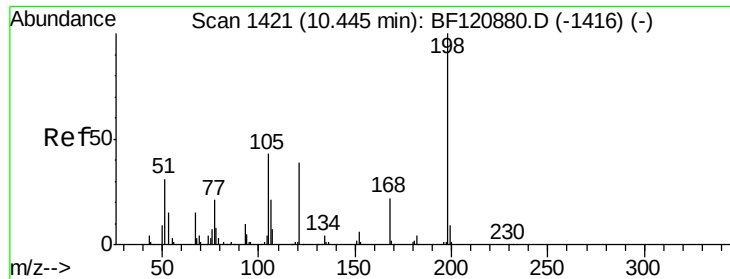




#65  
 4,6-Dinitro-2-methylphenol  
 Concen: 3.877 ng  
 RT: 10.62 min Scan# 1451  
 Delta R.T. 0.18 min  
 Lab File: BF121216.D  
 Acq: 6 Aug 2020 22:14

Instrument :  
 BNA\_F  
 ClientSampleId :  
 FK-GF-02-060-B

Tot Ion:198 Resp: 108  
 Ion Ratio Lower Upper  
 198 100  
 51 43.1 23.4 63.4  
 105 65.3 23.7 63.7#

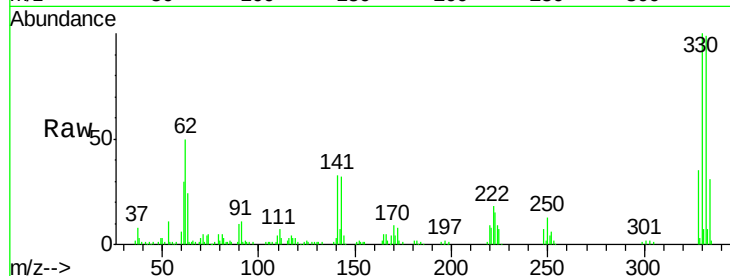


Abundance Ion 198.00 (197.70 to 198.70): E  
 Ion 51.00 (50.70 to 51.70): BF1  
 Ion 105.00 (104.70 to 105.70): E

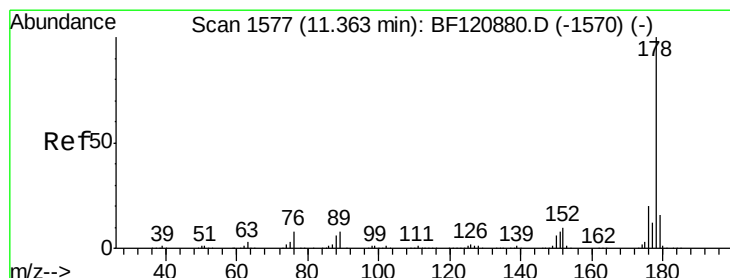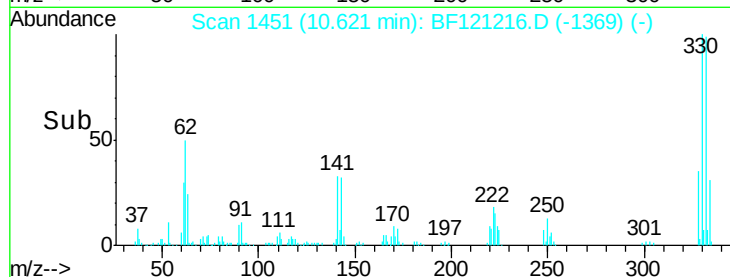
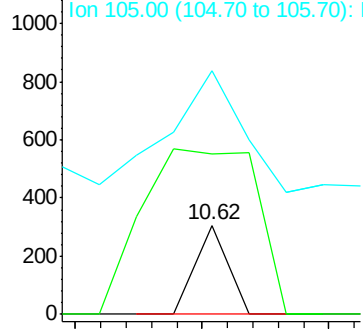



#71  
 Phenanthrene  
 Concen: 2.098 ng  
 RT: 11.34 min Scan# 1573  
 Delta R.T. -0.01 min  
 Lab File: BF121216.D  
 Acq: 6 Aug 2020 22:14

Tgt Ion:178 Resp: 54490  
 Ion Ratio Lower Upper  
 178 100  
 176 18.6 16.2 24.2  
 179 16.1 12.6 19.0

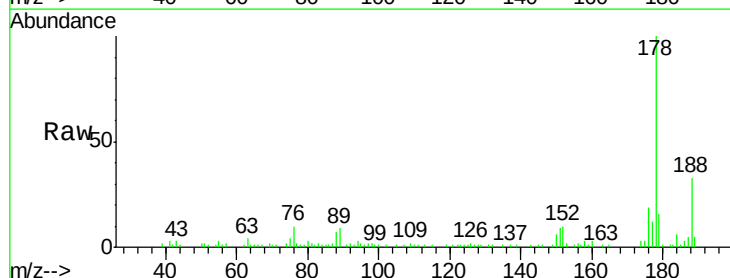

Abundance Ion 178.00 (177.70 to 178.70): E  
 Ion 176.00 (175.70 to 176.70): E  
 Ion 179.00 (178.70 to 179.70): E

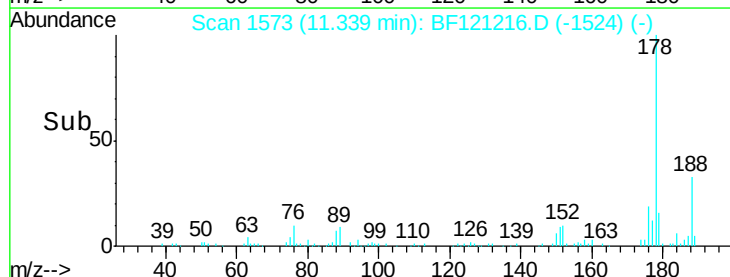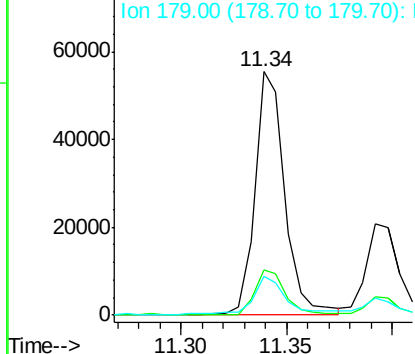

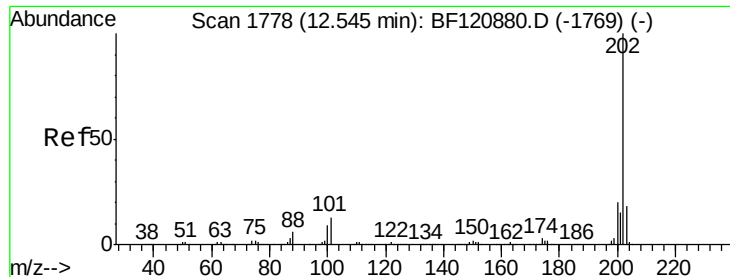

#75

Fluoranthene

Concen: 5.199 ng

RT: 12.53 min Scan# 1776

Delta R.T. -0.01 min

Lab File: BF121216.D

Acq: 6 Aug 2020 22:14

Instrument :

BNA\_F

ClientSampleId :

FK-GF-02-060-B


Tot Ion:202 Resp: 149645

Ion Ratio Lower Upper

202 100

101 10.9 0.0 30.5




203 17.4 0.0 37.7

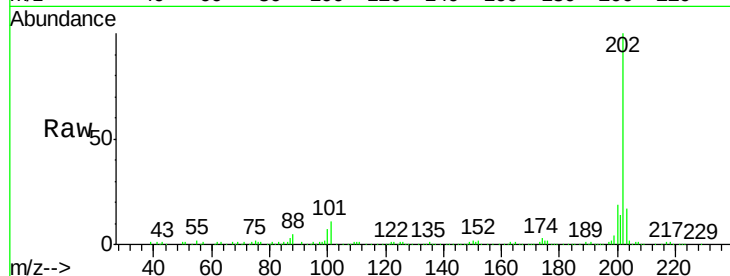

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

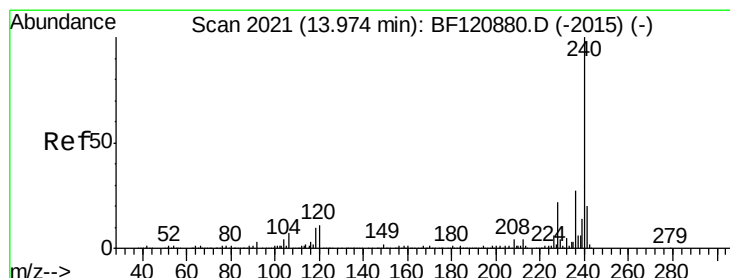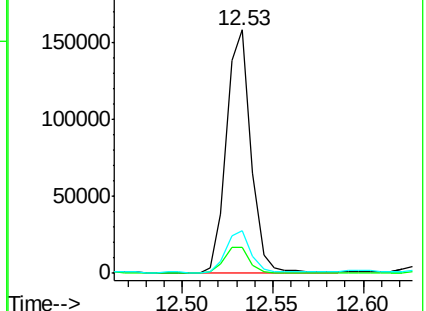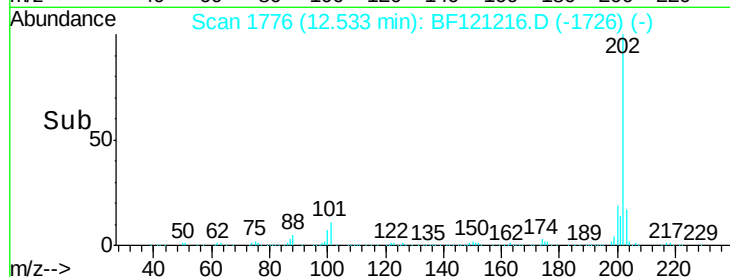

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.96 min Scan# 2018

Delta R.T. -0.01 min

Lab File: BF121216.D

Acq: 6 Aug 2020 22:14


Tgt Ion:240 Resp: 342458

Ion Ratio Lower Upper

240 100

120 12.4 9.3 13.9



236 26.5 21.1 31.7

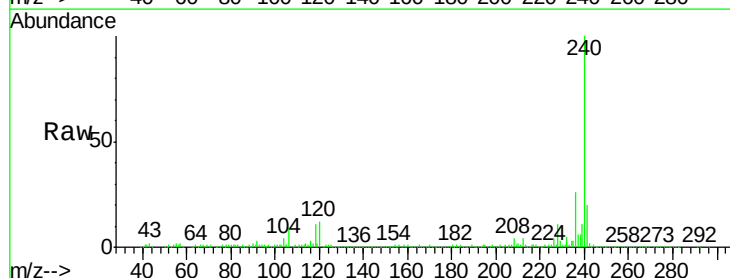


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



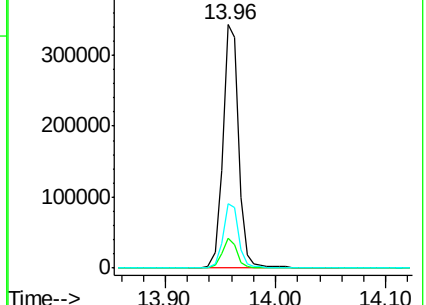
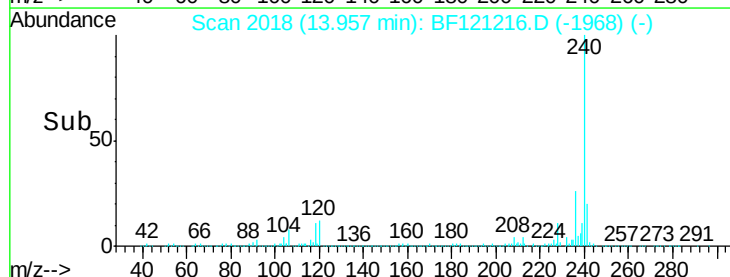


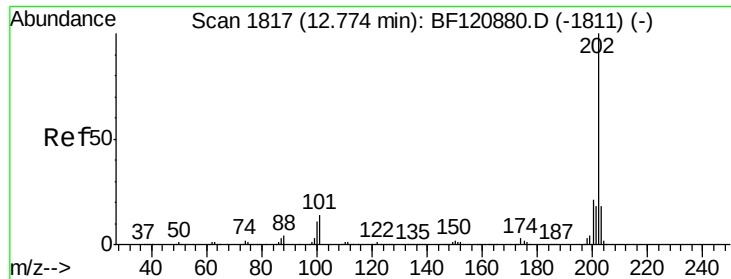

#78  
Pvrene  
Concen: 5.921 ng  
RT: 12.76 min Scan# 1815  
Delta R.T. -0.00 min  
Lab File: BF121216.D  
Acq: 6 Aug 2020 22:14




Instrument :  
BNA\_F  
ClientSampleId :  
FK-GF-02-060-B


| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 202     | 100   |       |       |
| 200     | 20.5  | 17.0  | 25.6  |
| 203     | 17.3  | 14.6  | 21.8  |

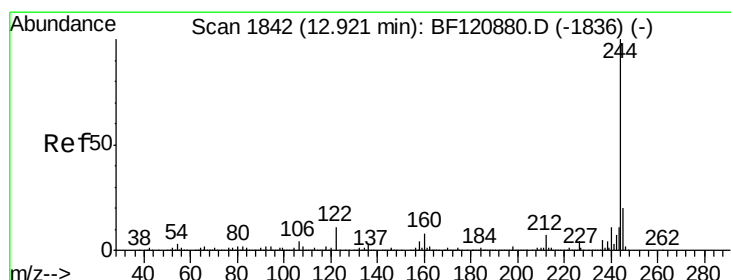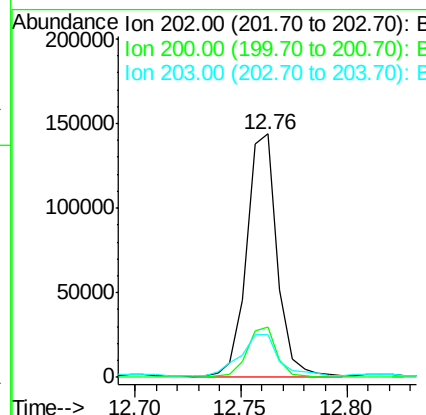

#79  
Terphenyl-d14  
Concen: 27.469 ng  
RT: 12.90 min Scan# 1839  
Delta R.T. -0.01 min  
Lab File: BF121216.D  
Acq: 6 Aug 2020 22:14

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 244     | 100   |       |       |
| 212     | 6.7   | 5.7   | 8.5   |
| 122     | 10.4  | 8.3   | 12.5  |

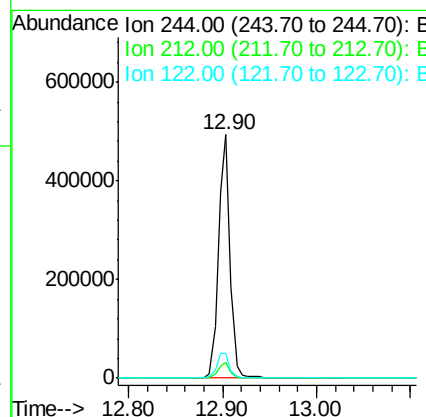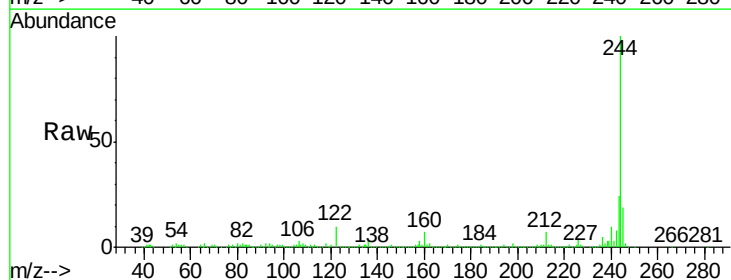







#81  
Benzo(a)anthracene  
Concen: 3.960 ng  
RT: 13.95 min Scan# 2017  
Delta R.T. -0.00 min  
Lab File: BF121216.D  
Acq: 6 Aug 2020 22:14

Instrument :  
BNA\_F  
ClientSampleId :  
FK-GF-02-060-B

Tot Ion:228 Resp: 82116  
Ion Ratio Lower Upper  
228 100  
226 30.8 22.6 34.0  
229 22.7 16.1 24.1




Abundance Ion 228.00 (227.70 to 228.70): E  
Ion 226.00 (225.70 to 226.70): E  
Ion 229.00 (228.70 to 229.70): E


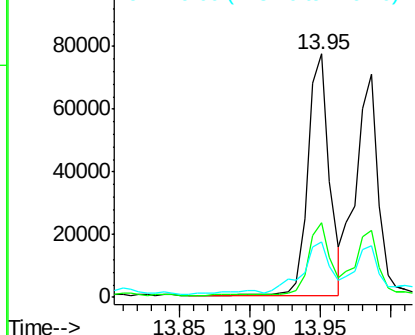



#83  
Chrysene  
Concen: 3.621 ng  
RT: 13.99 min Scan# 2023  
Delta R.T. -0.01 min  
Lab File: BF121216.D  
Acq: 6 Aug 2020 22:14

Tgt Ion:228 Resp: 78922  
Ion Ratio Lower Upper  
228 100  
226 30.3 25.4 38.0  
229 23.2 16.2 24.4



Abundance Ion 228.00 (227.70 to 228.70): E  
Ion 226.00 (225.70 to 226.70): E  
Ion 229.00 (228.70 to 229.70): E




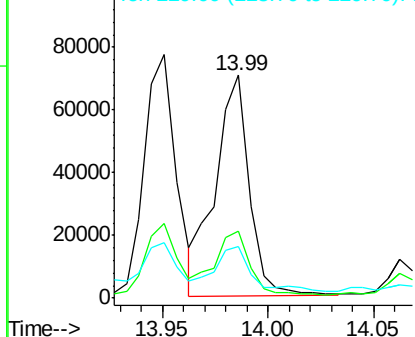


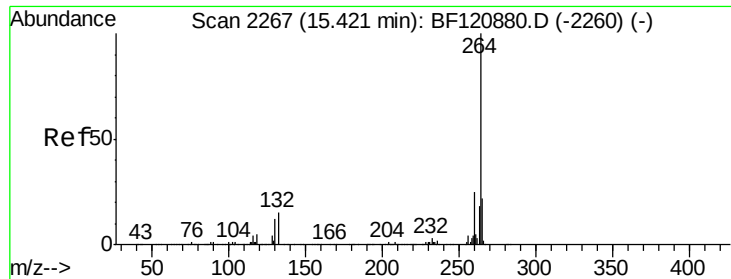

#86  
Pervlene-d12  
Concen: 20.000 ng  
RT: 15.42 min Scan# 2266  
Delta R.T. 0.01 min  
Lab File: BF121216.D  
Acq: 6 Aug 2020 22:14




Instrument :  
BNA\_F  
ClientSampleId :  
FK-GF-02-060-B


| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 264     | 100   |       |       |
| 260     | 25.1  | 19.9  | 29.9  |
| 265     | 21.7  | 17.8  | 26.8  |

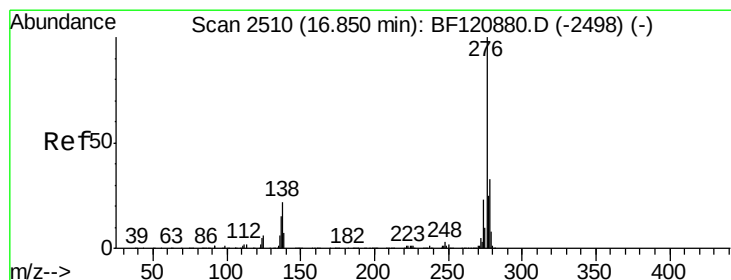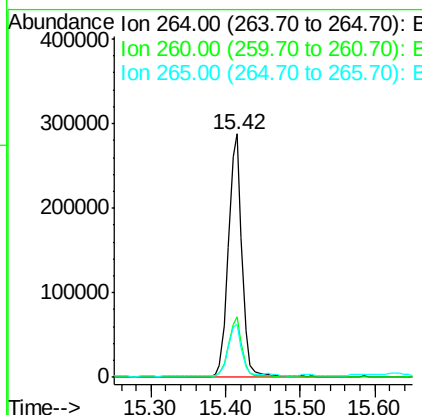

#87  
Indeno(1,2,3-cd)pyrene  
Concen: 2.024 ng  
RT: 16.84 min Scan# 2509  
Delta R.T. 0.01 min  
Lab File: BF121216.D  
Acq: 6 Aug 2020 22:14

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 276     | 100   |       |       |
| 138     | 21.0  | 19.3  | 28.9  |
| 277     | 25.7  | 20.1  | 30.1  |

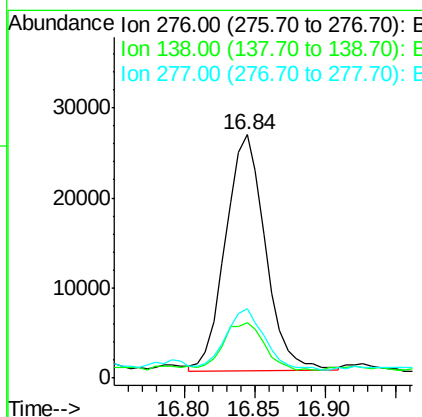



#88

Benzo(b)fluoranthene

Concen: 7.232 ng

RT: 14.99 min Scan# 2194

Delta R.T. -0.00 min

Lab File: BF121216.D

Acq: 6 Aug 2020 22:14





Instrument :

BNA\_F

ClientSampleId :

FK-GF-02-060-B

|          |       |       |        |
|----------|-------|-------|--------|
| Tot Ion: | 252   | Resp: | 160119 |
| Ion      | Ratio | Lower | Upper  |
| 252      | 100   |       |        |
| 253      | 25.3  | 17.9  | 26.9   |
| 125      | 14.4  | 8.1   | 12.1#  |

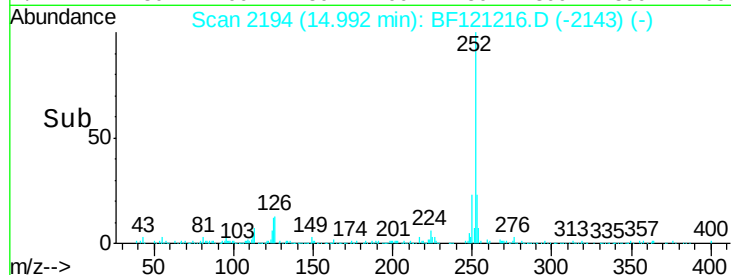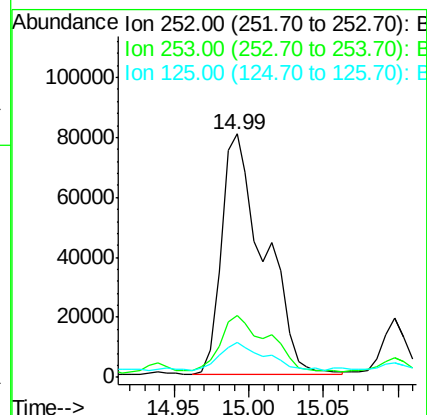

#89

Benzo(k)fluoranthene

Concen: 7.929 ng




RT: 14.99 min Scan# 2194


Delta R.T. -0.03 min

Lab File: BF121216.D

Acq: 6 Aug 2020 22:14

|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 252   | Resp: | 160119 |
| Ion      | Ratio | Lower | Upper  |
| 252      | 100   |       |        |
| 253      | 25.3  | 18.1  | 27.1   |
| 125      | 14.4  | 8.0   | 12.0#  |



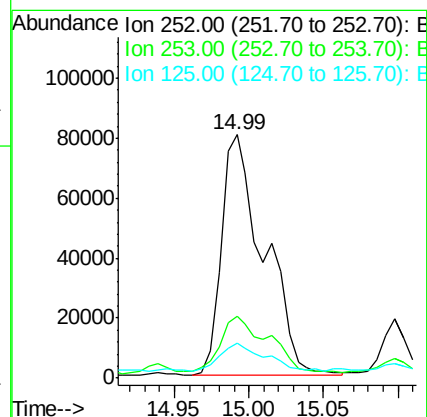





#90  
Benzo(a)pyrene  
Concen: 4.316 ng  
RT: 15.35 min Scan# 2255  
Delta R.T. 0.01 min  
Lab File: BF121216.D  
Acq: 6 Aug 2020 22:14

Instrument :  
BNA\_F  
ClientSampleId :  
FK-GF-02-060-B

Tot Ion:252 Resp: 87192  
Ion Ratio Lower Upper  
252 100  
253 24.2 18.0 27.0  
125 13.1 9.5 14.3

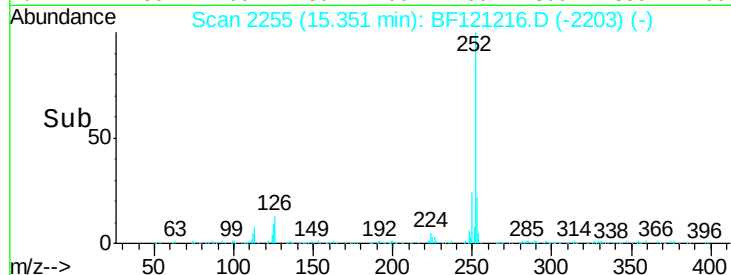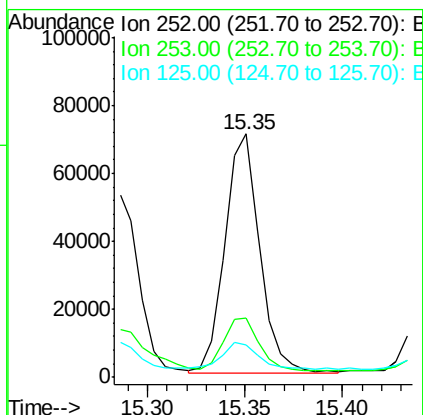

#92  
Benzo(g,h,i)perylene  
Concen: 2.361 ng  
RT: 17.27 min Scan# 2582  
Delta R.T. 0.01 min  
Lab File: BF121216.D  
Acq: 6 Aug 2020 22:14

Tgt Ion:276 Resp: 48446  
Ion Ratio Lower Upper  
276 100  
277 24.5 19.4 29.0  
138 25.0 17.2 25.8

