
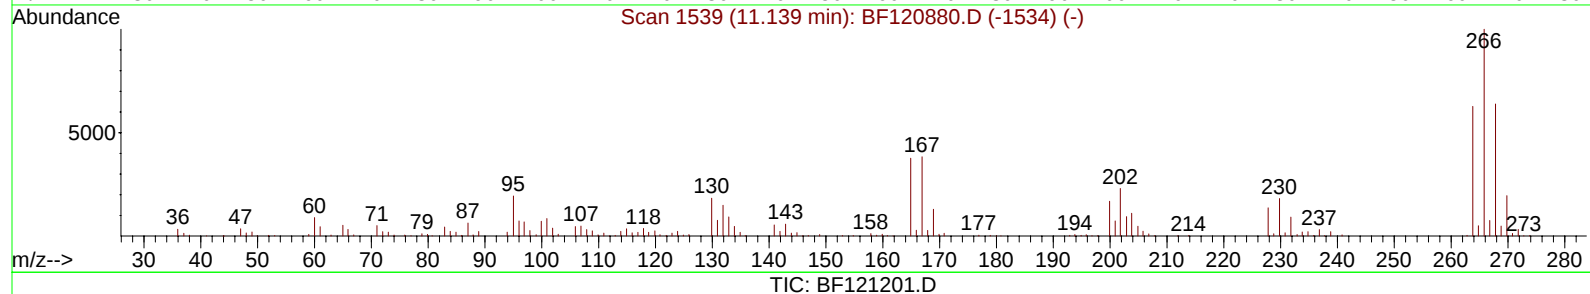
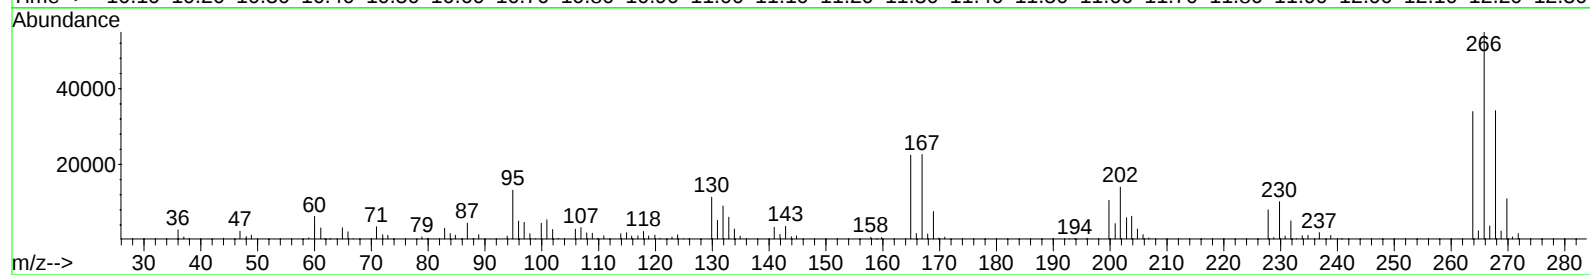


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF080620\
Data File : BF121201.D
Acq On : 6 Aug 2020 14:33
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 18:14:21 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 29 14:55:43 2020
Response via : Initial Calibration

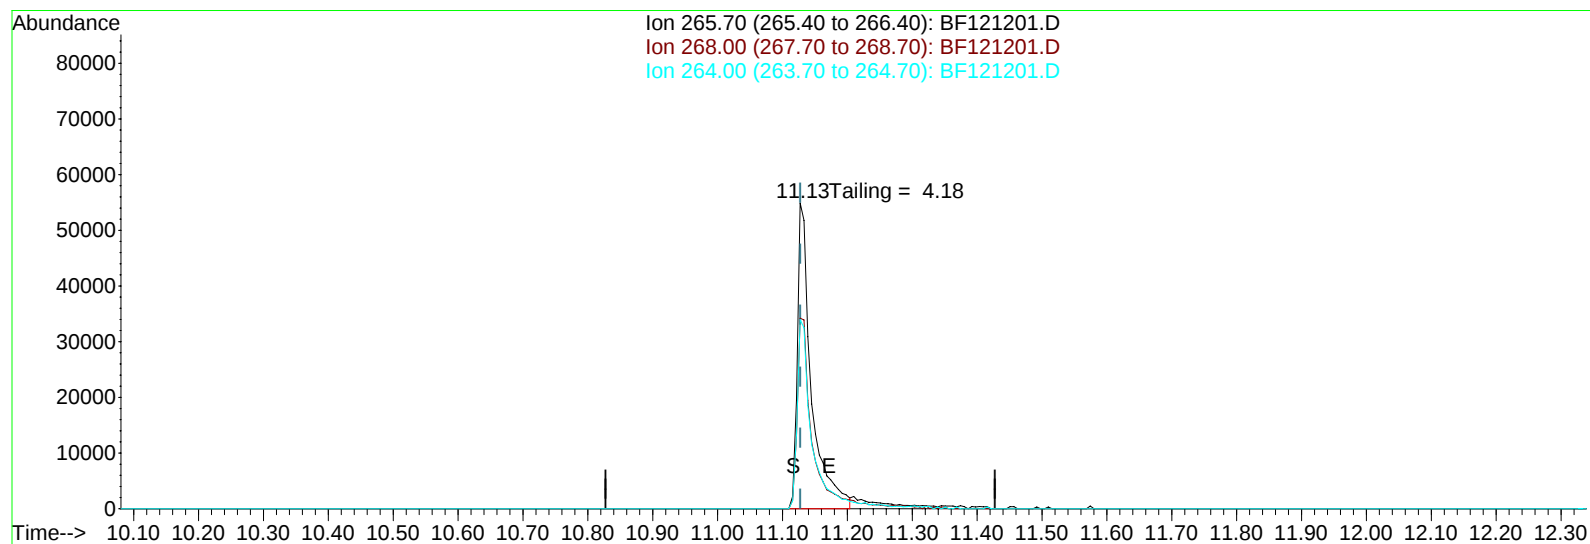

(70) Pentachlorophenol (C)




11.127min (-0.000) 30071.43ng

response 90381

Ion	Exp%	Act%
265.70	100	100
268.00	62.10	62.31
264.00	63.00	61.84
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF080620\
Data File : BF121201.D
Acq On : 6 Aug 2020 14:33
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 18:14:21 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 29 14:55:43 2020
Response via : Initial Calibration

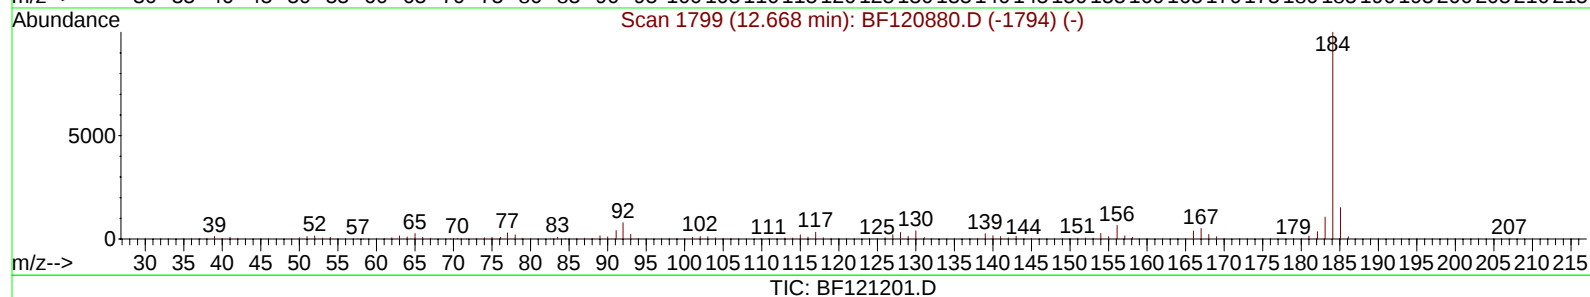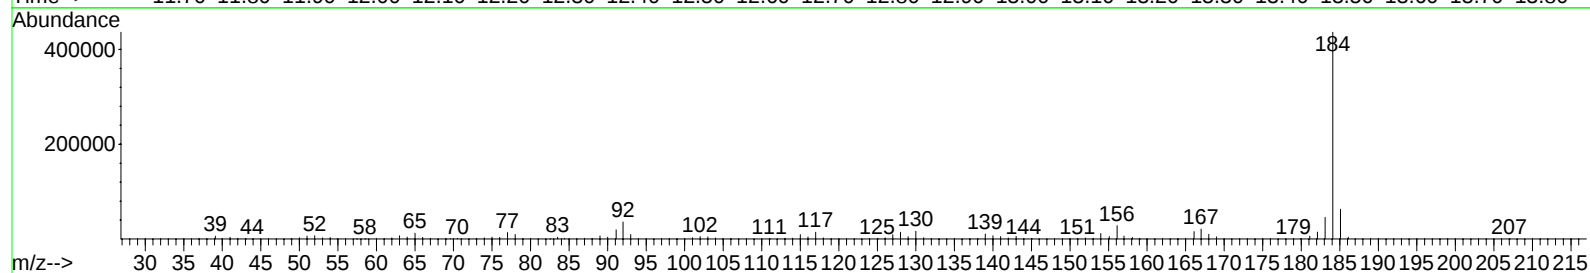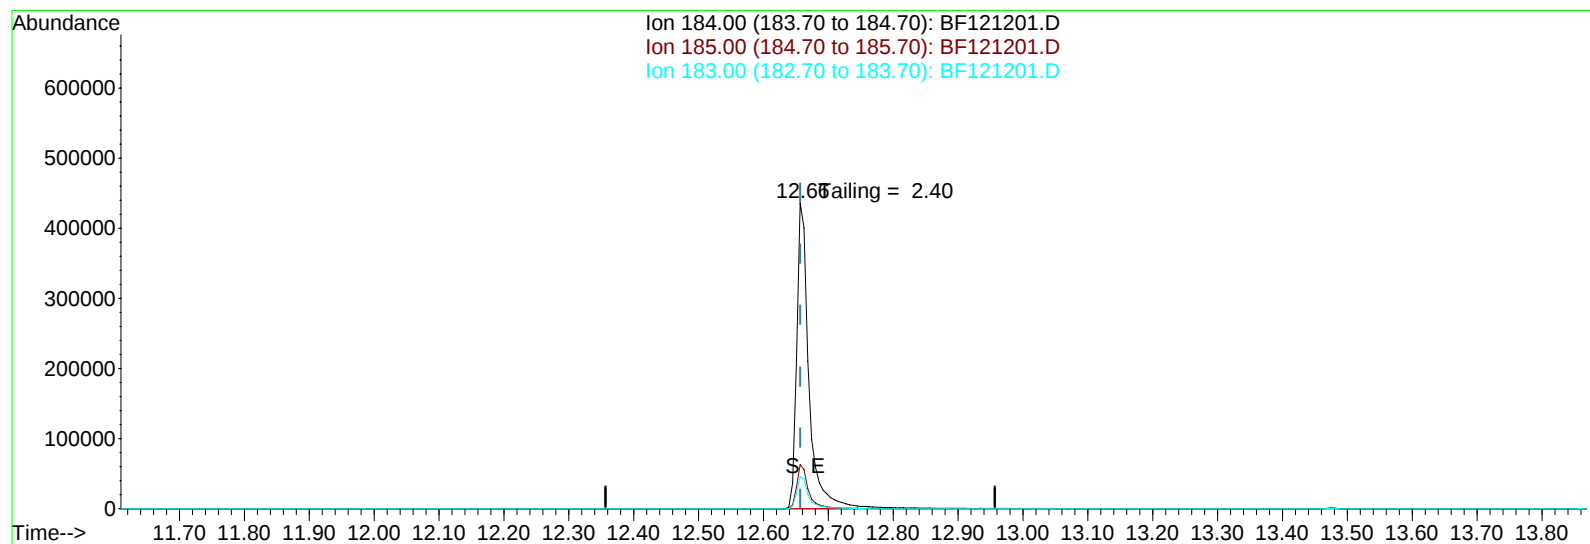

(77) Benzidine

12.657min (-0.000) 0.00ng

response 579213

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	14.43
183.00	11.20	10.54
0.00	0.00	0.00