

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080620\
Data File : BF121204.D
Acq On : 6 Aug 2020 16:06
Operator : JU/CG
Sample : PB130763BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130763BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.028	494	500	512	rBV	52020	80606	1.75%	0.286%
2	5.422	562	567	570	rBV	3343573	3624910	78.85%	12.855%
3	6.434	734	739	742	rBV	3014756	3576947	77.81%	12.685%
4	6.792	796	800	813	rVB	1017051	811741	17.66%	2.879%
5	7.357	891	896	899	rBV	2324989	2607981	56.73%	9.248%
6	8.075	1013	1018	1033	rBV	1110948	1046029	22.75%	3.709%
7	9.157	1196	1202	1217	rBV	3811790	4596943	100.00%	16.302%
8	9.827	1312	1316	1334	rBV	1100780	1180796	25.69%	4.187%
9	10.621	1446	1451	1480	rBV	2290610	2866318	62.35%	10.165%
10	11.316	1565	1569	1585	rBV	1147774	1199644	26.10%	4.254%
11	12.910	1834	1840	1843	rBV	3889601	4525060	98.44%	16.047%
12	13.957	2014	2018	2028	rBV	1032299	1056503	22.98%	3.747%
13	15.409	2259	2265	2283	rBV	650291	1025608	22.31%	3.637%


Sum of corrected areas: 28199086

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF080620\
Data File : BF121204.D
Acq On : 6 Aug 2020 16:06
Operator : JU/CG
Sample : PB130763BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130763BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

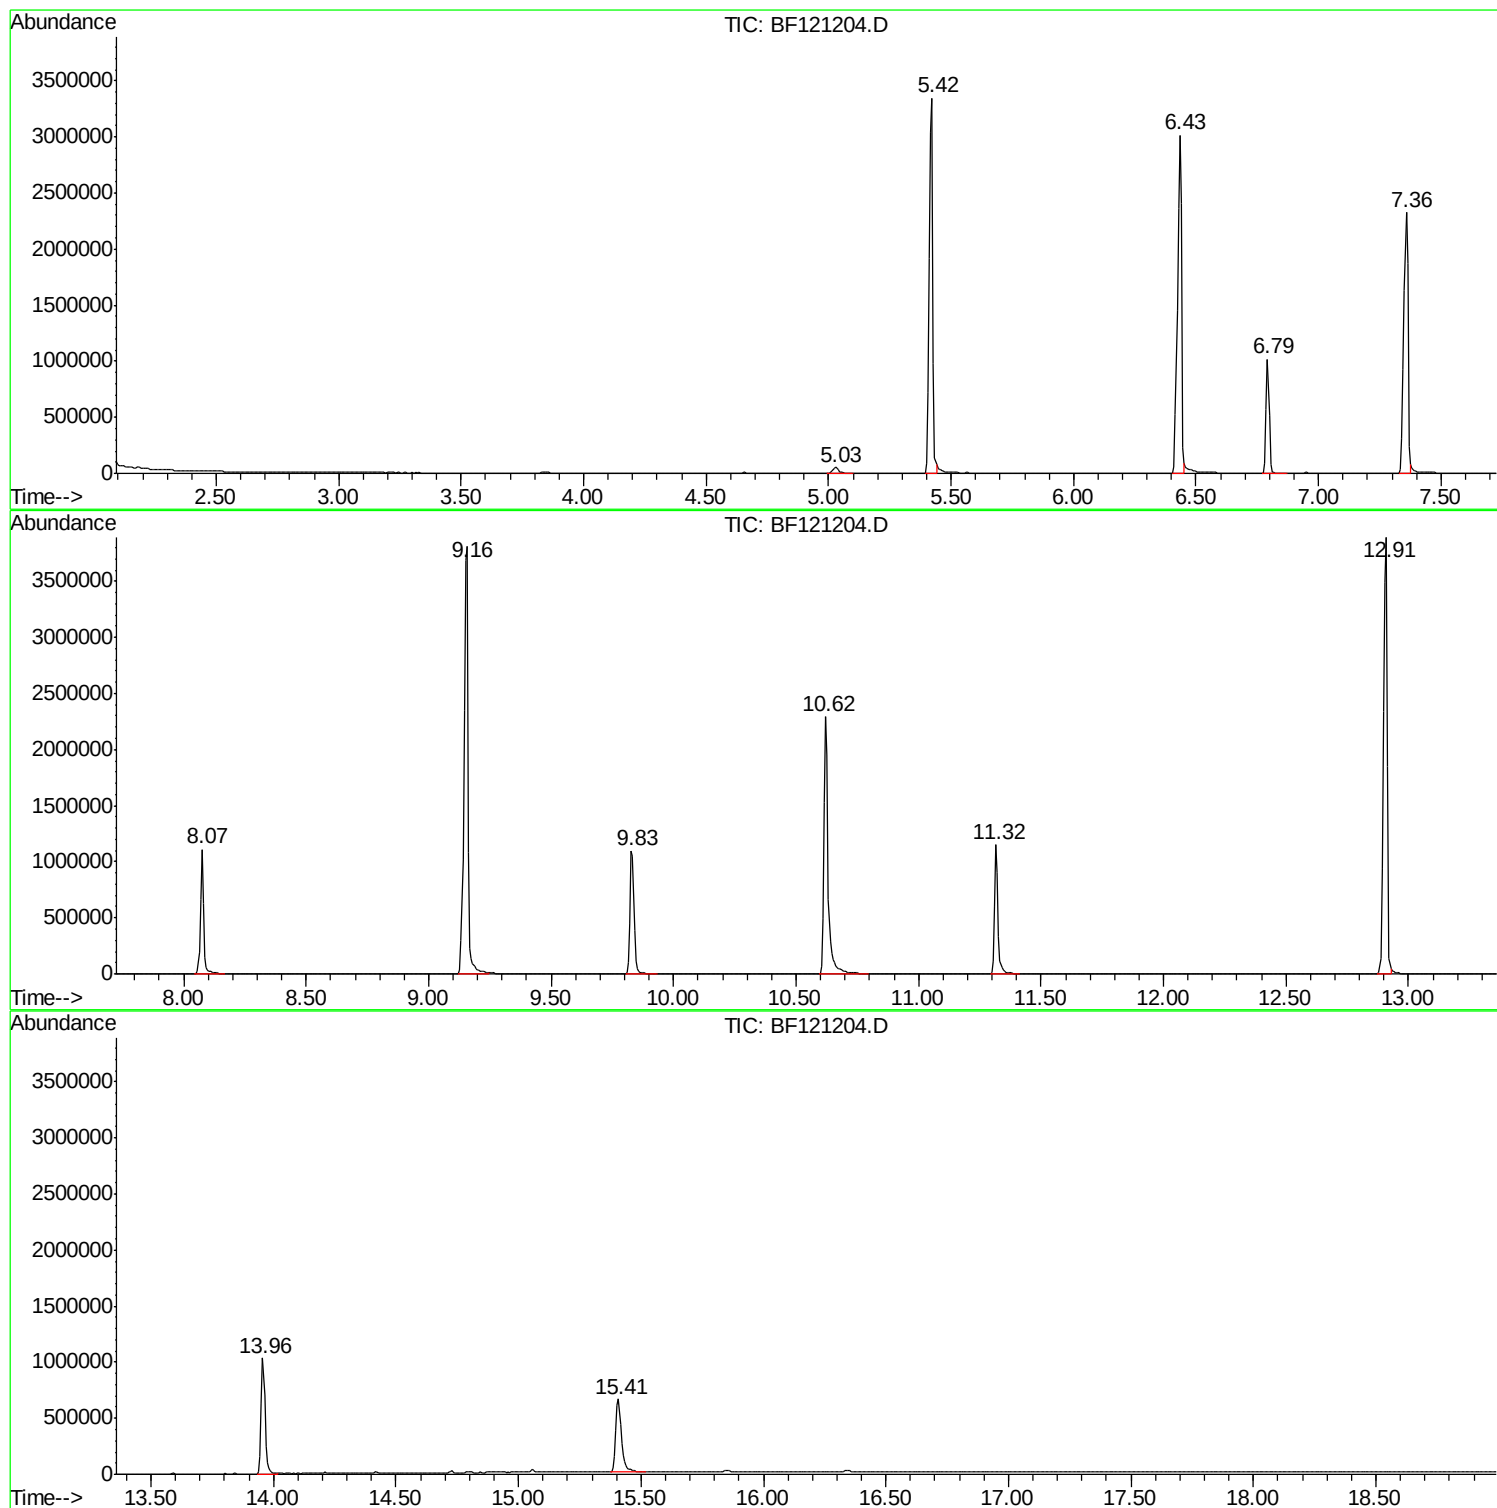

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080620\
Data File : BF121204.D
Acq On : 6 Aug 2020 16:06
Operator : JU/CG
Sample : PB130763BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130763BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080620\
Data File : BF121204.D
Acq On : 6 Aug 2020 16:06
Operator : JU/CG
Sample : PB130763BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130763BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc