


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080620\
 Data File : BF121193.D
 Acq On : 6 Aug 2020 8:40
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 29 14:55:43 2020

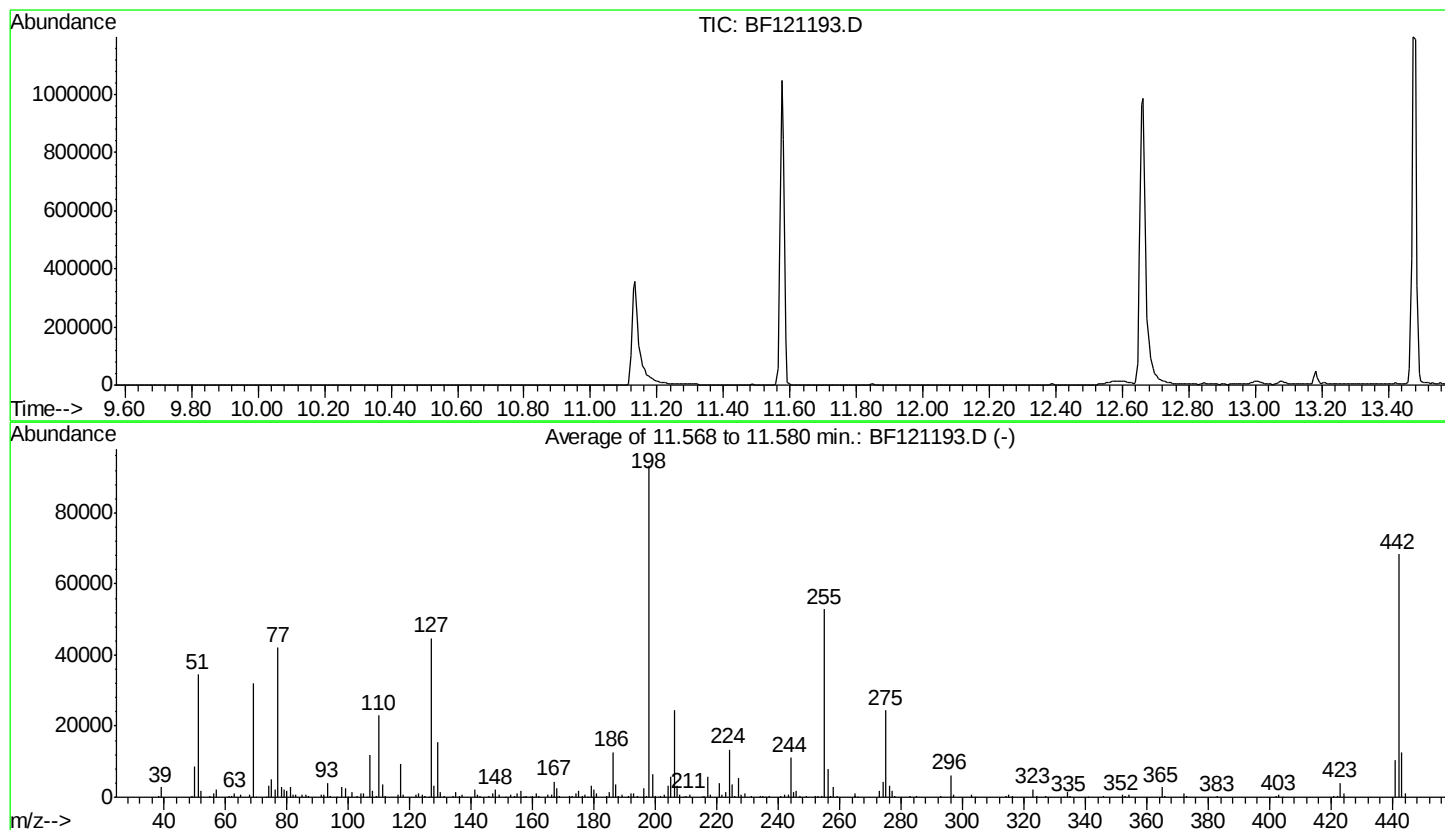

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	34562	PASS
68	69	0.00	2	1.9	596	PASS
69	198	0.00	100	34.4	32064	PASS
70	69	0.00	2	0.4	115	PASS
127	198	10	80	48.1	44829	PASS
197	198	0.00	2	0.6	527	PASS
198	198	100	100	100.0	93282	PASS
199	198	5	9	7.0	6516	PASS
275	198	10	60	26.2	24437	PASS
365	198	1	100	3.1	2860	PASS
441	198	0.01	100	11.4	10633	PASS
442	198	50	100	73.3	68341	PASS
443	442	15	24	18.6	12701	PASS