


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080620\
 Data File : BF121201.D
 Acq On : 6 Aug 2020 14:33
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 29 14:55:43 2020

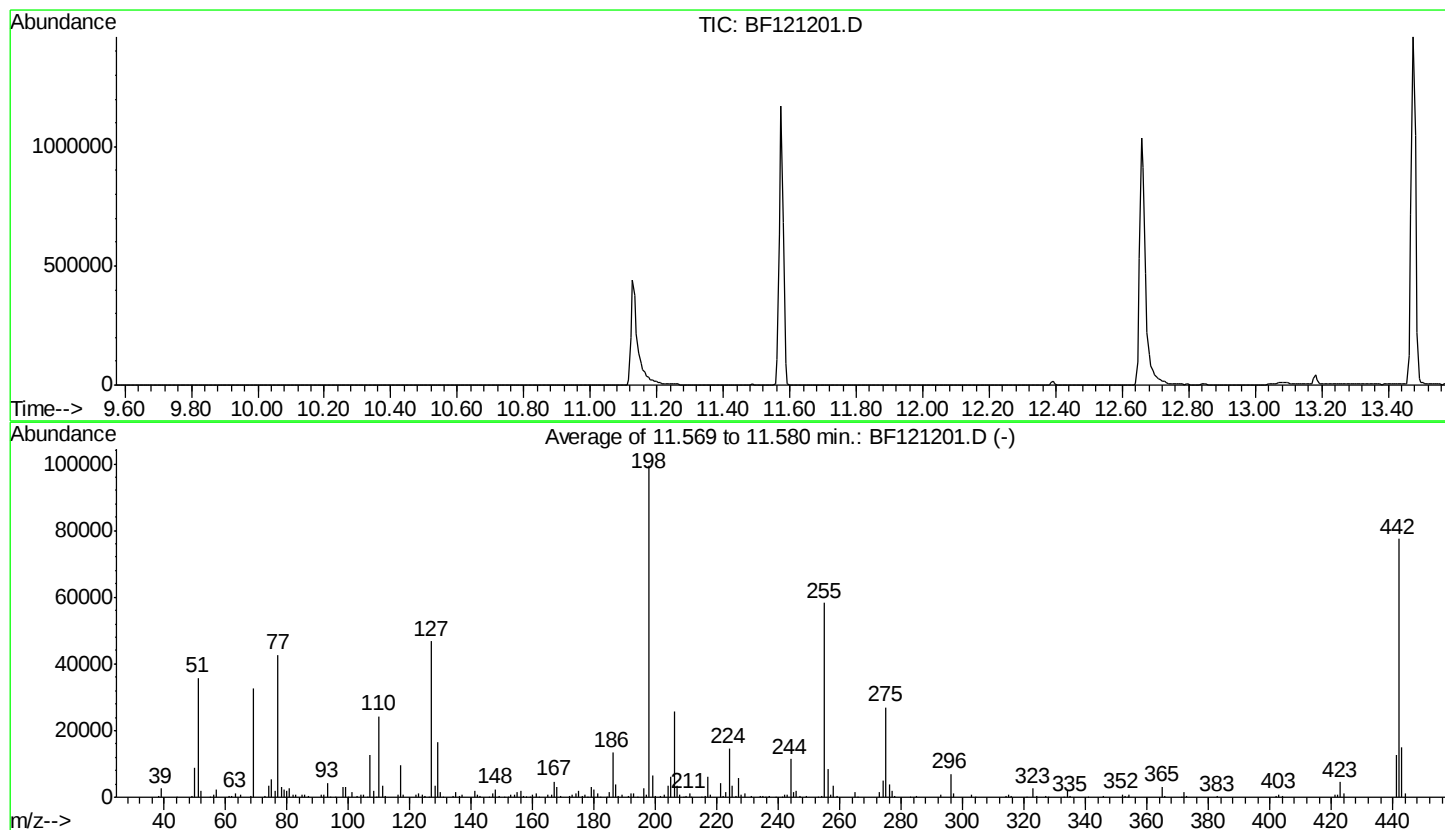

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	35781	PASS
68	69	0.00	2	1.7	560	PASS
69	198	0.00	100	32.8	32640	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.0	46754	PASS
197	198	0.00	2	0.7	706	PASS
198	198	100	100	100.0	99445	PASS
199	198	5	9	6.7	6672	PASS
275	198	10	60	27.2	27069	PASS
365	198	1	100	3.3	3262	PASS
441	198	0.01	100	12.6	12579	PASS
442	198	50	100	78.0	77536	PASS
443	442	15	24	19.1	14800	PASS