
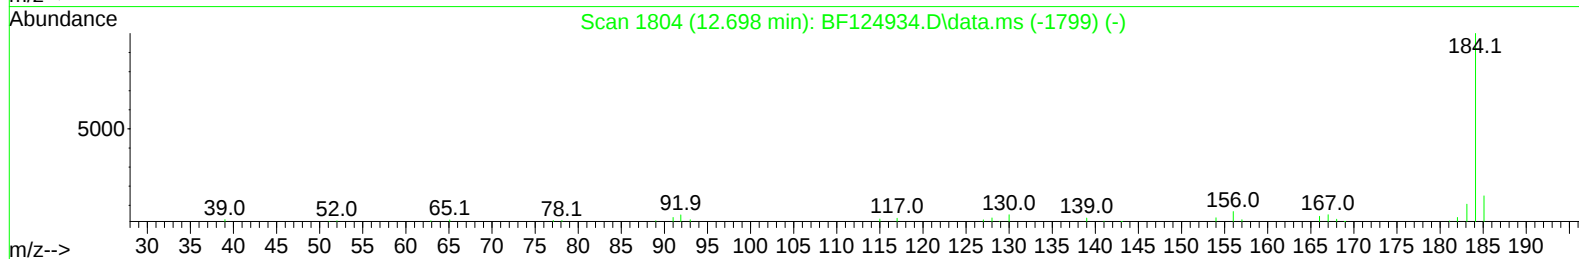
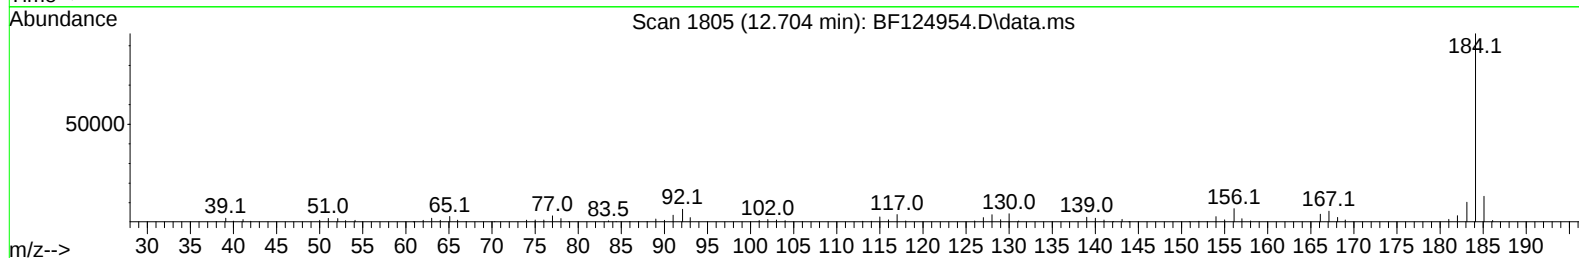


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080621\
Data File : BF124954.D
Acq On : 6 Aug 2021 7:27
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 11:18:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 04 17:59:00 2021
Response via : Initial Calibration

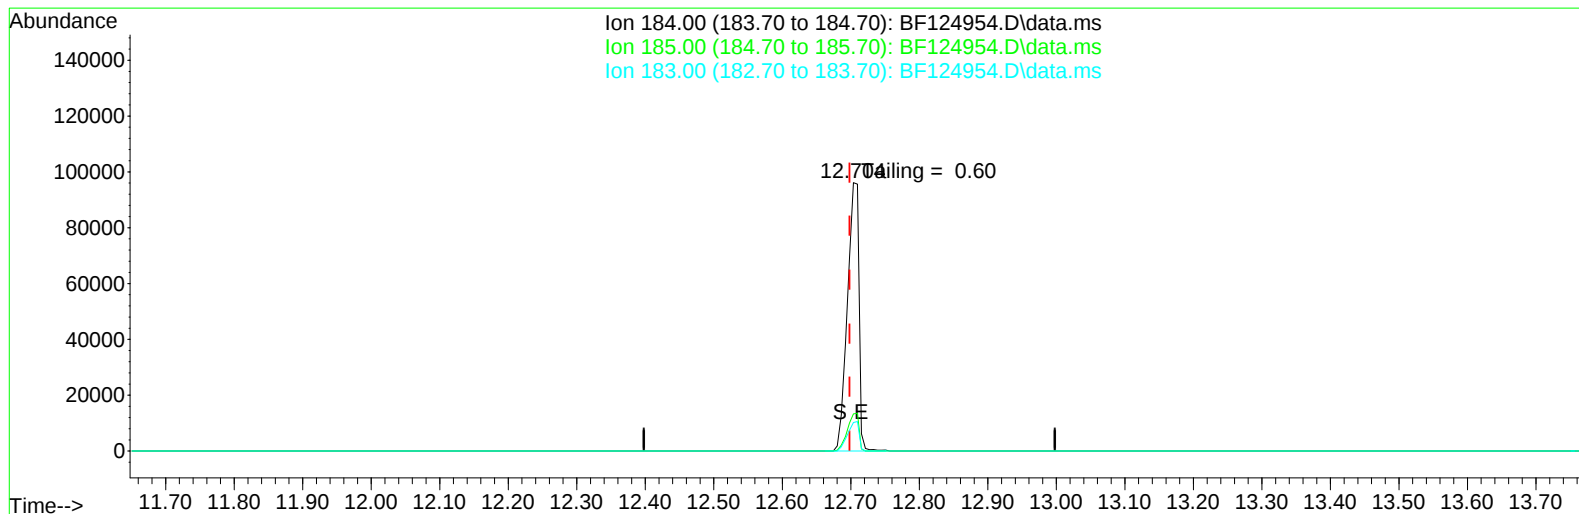

TIC: BF124954.D\data.ms

(77) Benzidine




12.704min (+ 0.006) 0.00 ng

response 113834

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.84
183.00	10.10	10.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080621\
Data File : BF124954.D
Acq On : 6 Aug 2021 7:27
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 11:18:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 04 17:59:00 2021
Response via : Initial Calibration

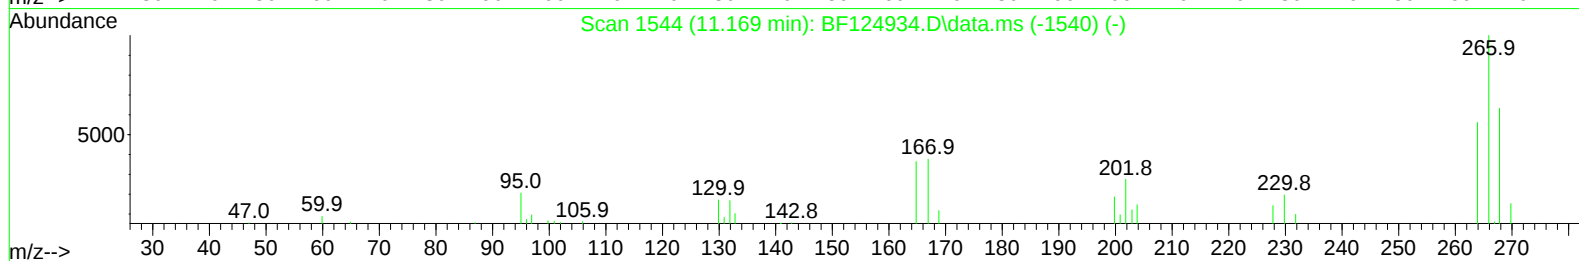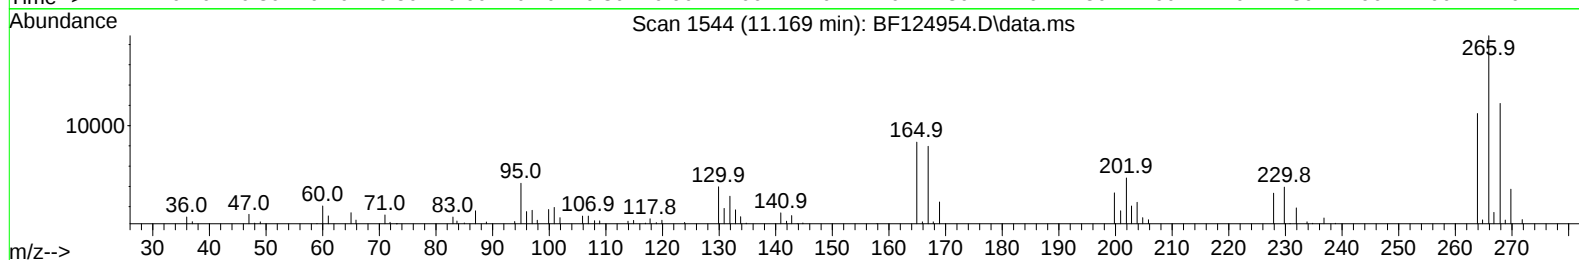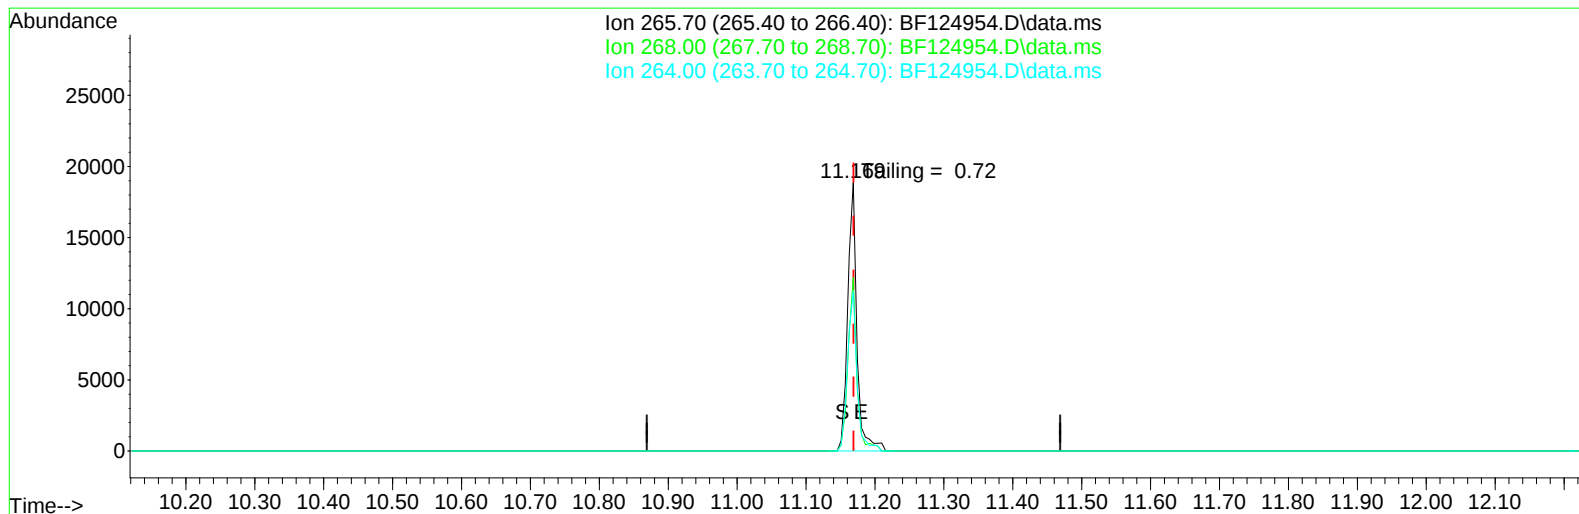

TIC: BF124954.D\data.ms

(70) Pentachlorophenol (C)

11.169min (-0.000) 0.00 ng

response 17493

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	64.61
264.00	69.90	59.31
0.00	0.00	0.00