

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080621\
 Data File : BF124956.D
 Acq On : 6 Aug 2021 10:19
 Operator : JU/CG
 Sample : PB138117BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB138117BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124956.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.457	569	573	576	rBV	214187	217305	70.56%	12.732%
2	6.457	738	743	746	rBV	193069	228312	74.13%	13.377%
3	6.828	803	806	809	rBB	57668	44174	14.34%	2.588%
4	7.392	897	902	905	rBB	141901	146154	47.46%	8.563%
5	8.110	1019	1024	1027	rBB	67777	59886	19.45%	3.509%
6	9.186	1201	1207	1210	rBB	304063	279624	90.79%	16.383%
7	9.863	1318	1322	1325	rBB	88082	71485	23.21%	4.188%
8	10.657	1451	1457	1460	rBV	171109	162229	52.68%	9.505%
9	11.351	1571	1575	1578	rBV	92290	72168	23.43%	4.228%
10	12.939	1840	1845	1848	rBV	352092	307974	100.00%	18.044%
11	13.851	1996	2000	2003	rVB	4231	4820	1.57%	0.282%
12	13.986	2020	2023	2026	rBB	74072	59116	19.20%	3.464%
13	15.445	2266	2271	2275	rBB	48222	53554	17.39%	3.138%




Sum of corrected areas: 1706801

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080621\
Data File : BF124956.D
Acq On : 6 Aug 2021 10:19
Operator : JU/CG
Sample : PB138117BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138117BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

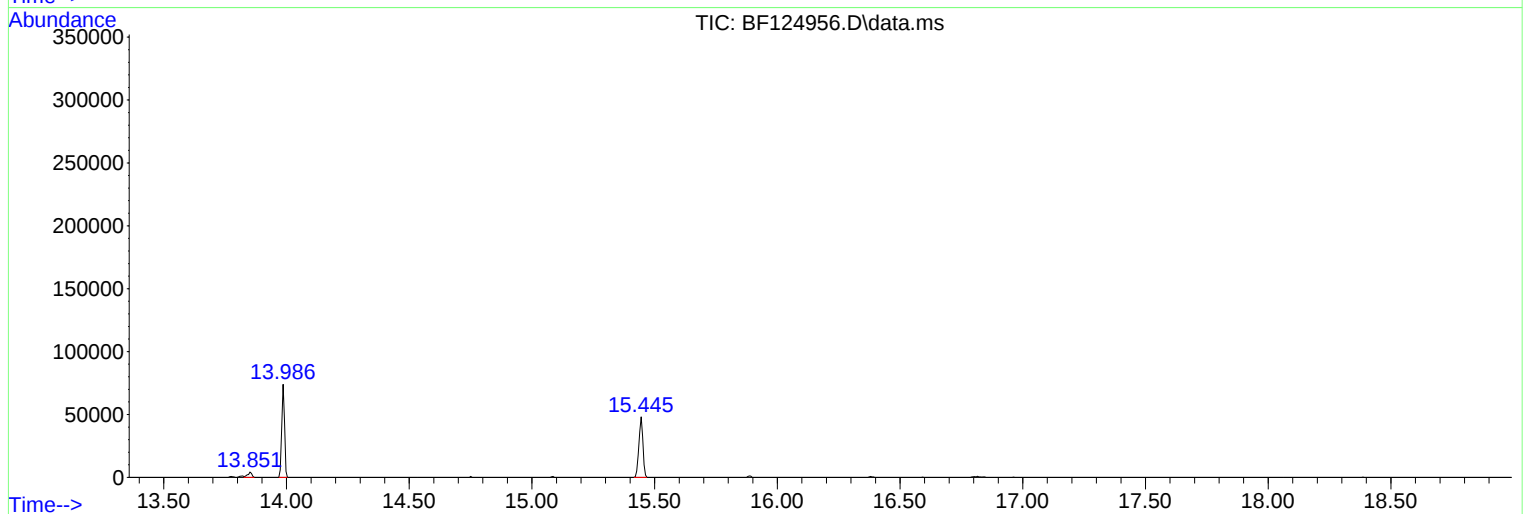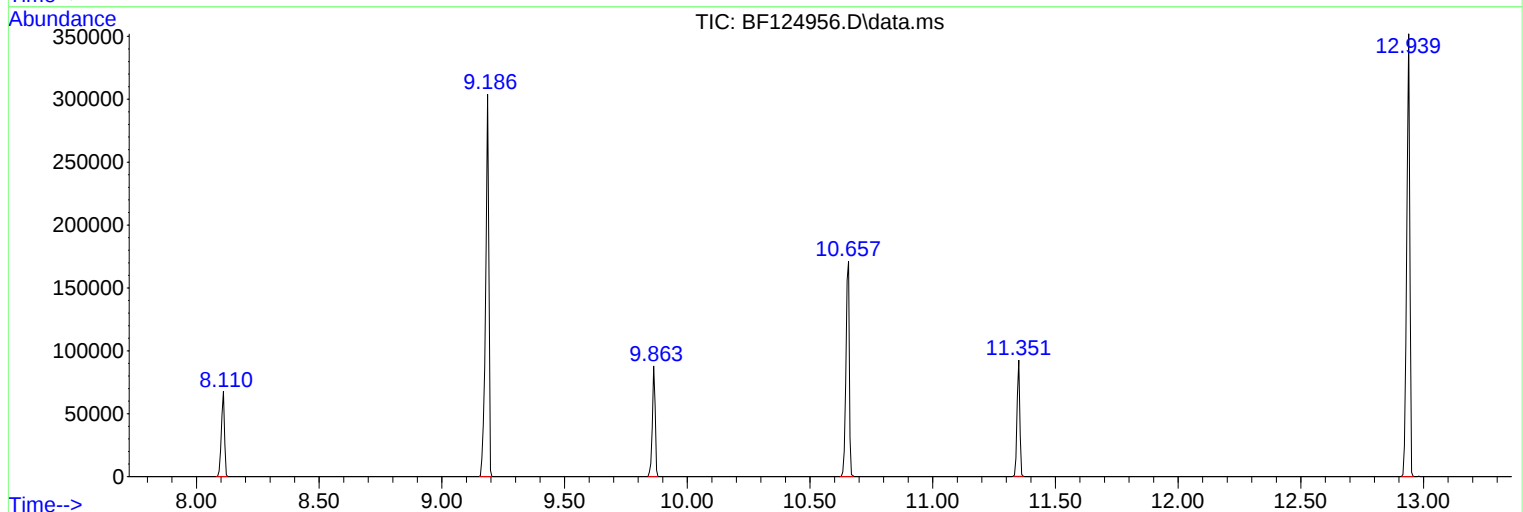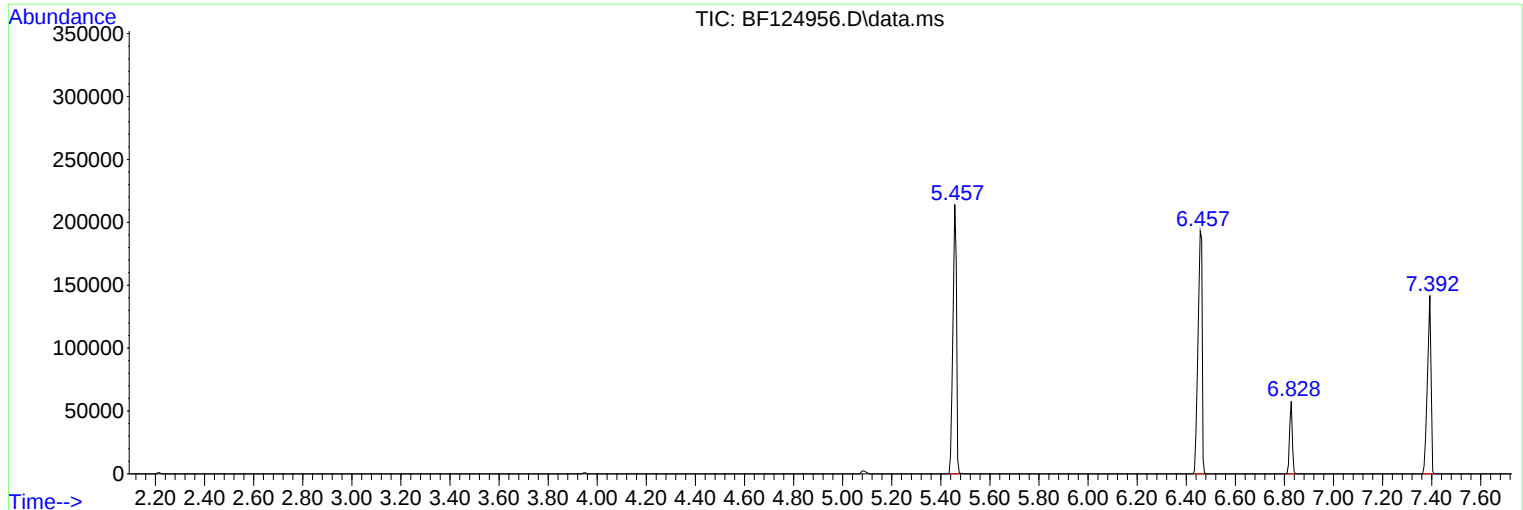

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080621\
Data File : BF124956.D
Acq On : 6 Aug 2021 10:19
Operator : JU/CG
Sample : PB138117BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138117BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080621\
Data File : BF124956.D
Acq On : 6 Aug 2021 10:19
Operator : JU/CG
Sample : PB138117BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138117BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------