


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF080621\  
 Data File : BF124954.D  
 Acq On : 6 Aug 2021 7:27  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF080421.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Aug 09 11:03:44 2021

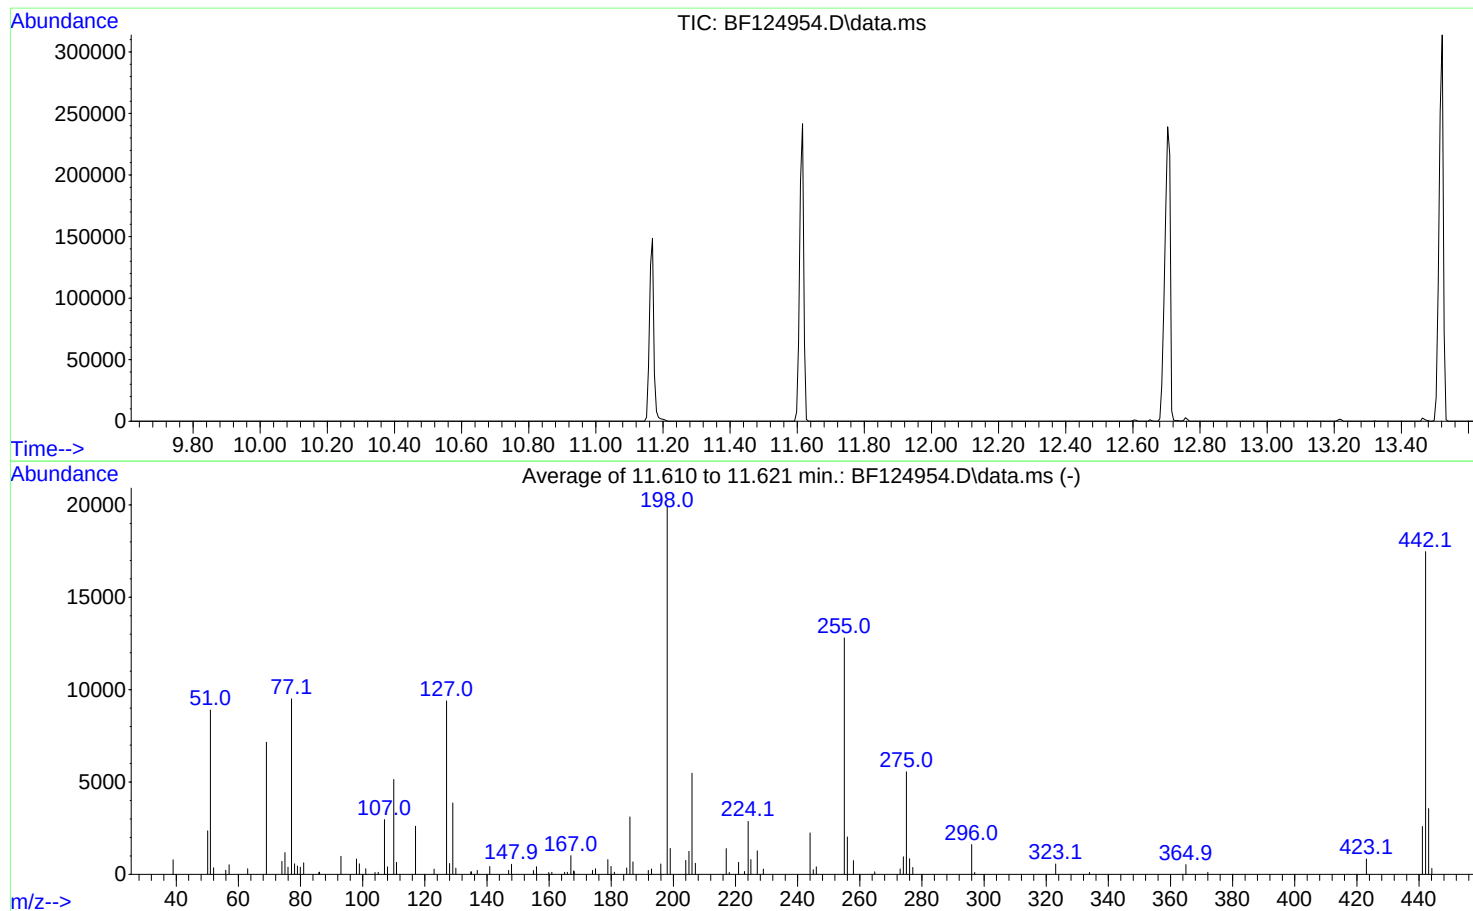




AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 44.7         | 8896       | PASS                |
| 68             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 69             | 198             | 0.00            | 100             | 35.9         | 7154       | PASS                |
| 70             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 127            | 198             | 10              | 80              | 47.1         | 9386       | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 19915      | PASS                |
| 199            | 198             | 5               | 9               | 7.1          | 1407       | PASS                |
| 275            | 198             | 10              | 60              | 27.9         | 5554       | PASS                |
| 365            | 198             | 1               | 100             | 2.7          | 528        | PASS                |
| 441            | 198             | 0.01            | 100             | 13.0         | 2587       | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 17474      | PASS                |
| 443            | 442             | 15              | 24              | 20.4         | 3560       | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF080621\  
 Data File : BF124954.D  
 Acq On : 6 Aug 2021 7:27  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Quant Time: Aug 06 11:18:17 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF080421.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Aug 04 17:59:00 2021  
 Response via : Initial Calibration

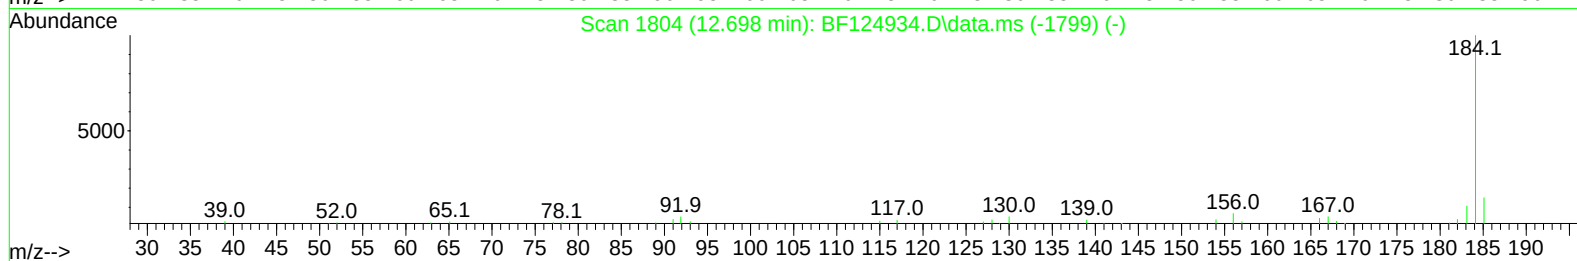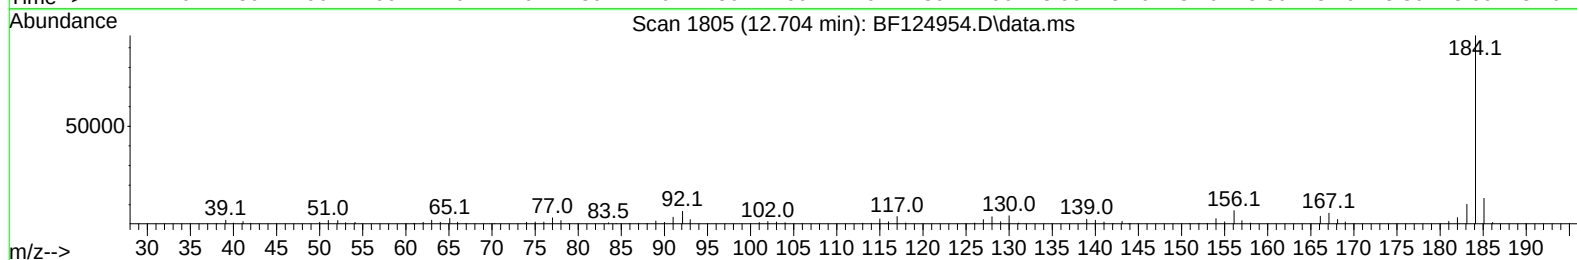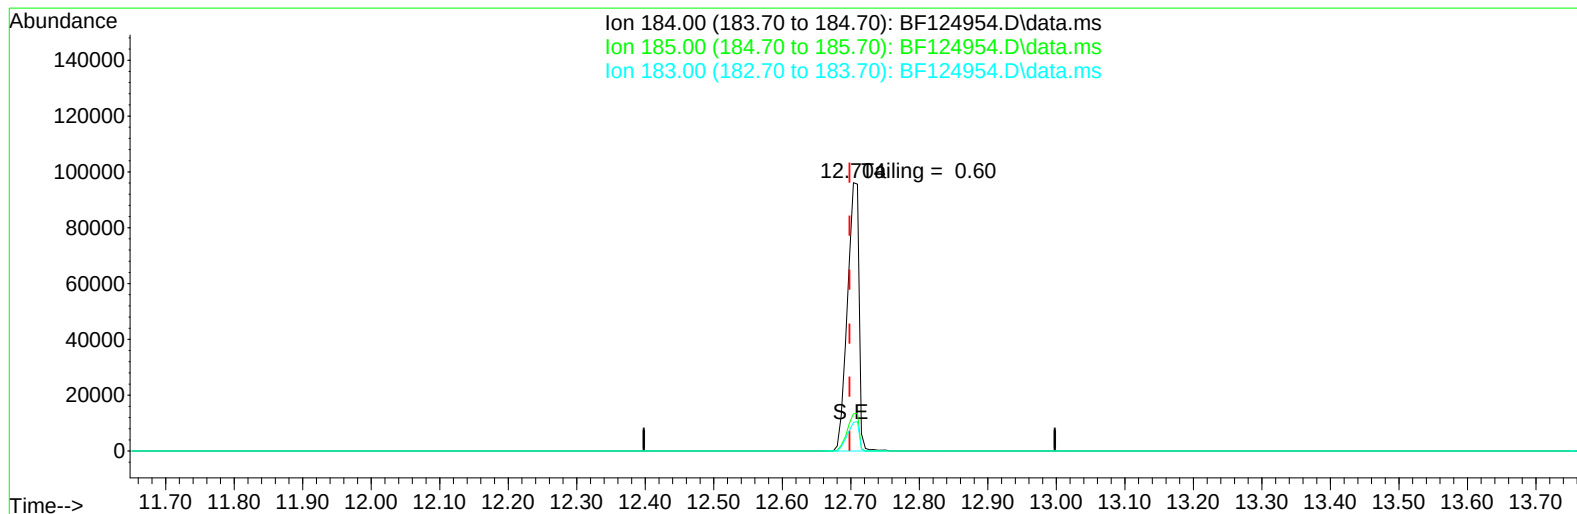

TIC: BF124954.D\data.ms

**(77) Benzidine**

12.704min (+ 0.006) 0.00 ng




response 113834

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.50  | 13.84  |
| 183.00 | 10.10  | 10.64  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF080621\  
Data File : BF124954.D  
Acq On : 6 Aug 2021 7:27  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Aug 06 11:18:17 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF080421.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 04 17:59:00 2021  
Response via : Initial Calibration

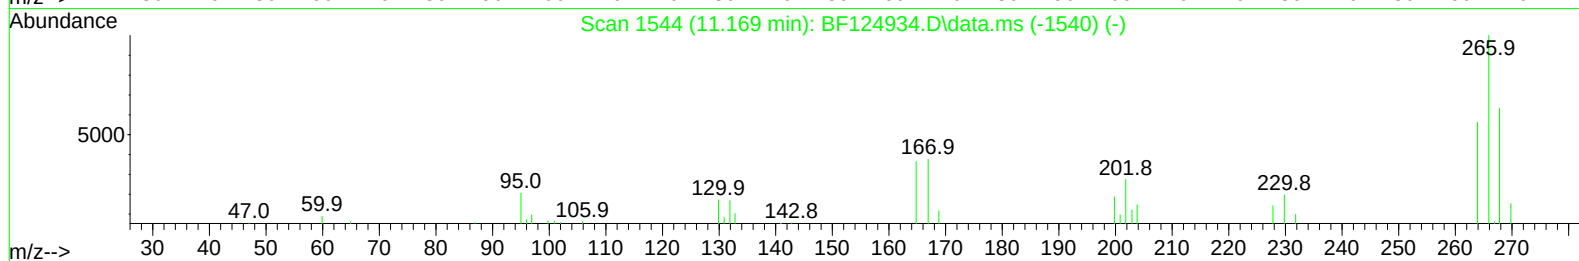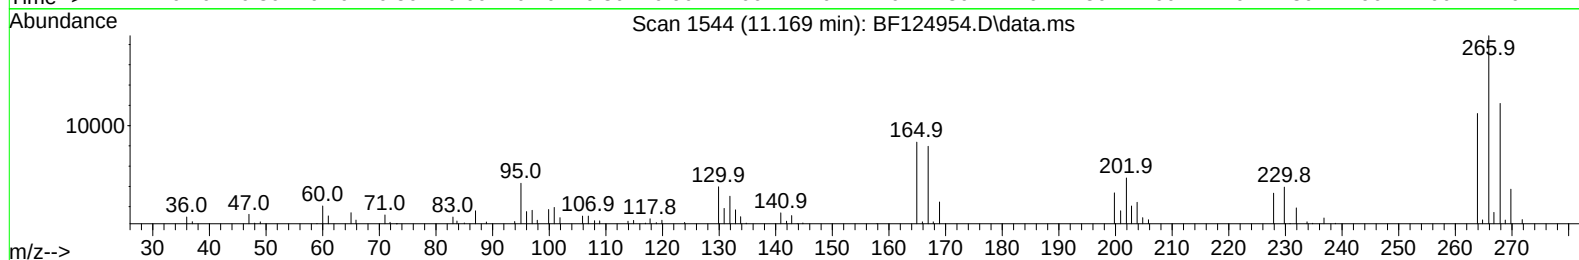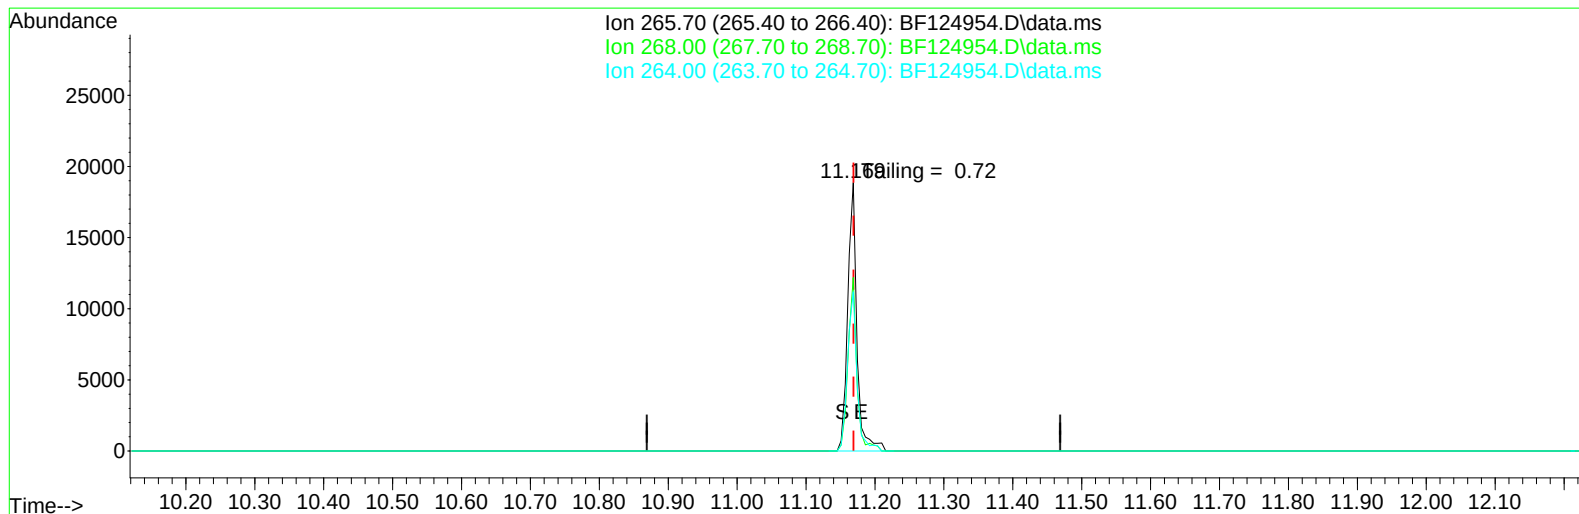

TIC: BF124954.D\data.ms

**(70) Pentachlorophenol (C)**

11.169min (-0.000) 0.00 ng

response 17493

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.10  | 64.61  |
| 264.00 | 69.90  | 59.31  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 8/6/2021      | BNA_F            | <u>BF124954.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 53194            | 13.52              |
| DDD           | 539              | 13.21              |
| DDE           | 0                | 12.71              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 539           | 53733            | 1.00               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP