
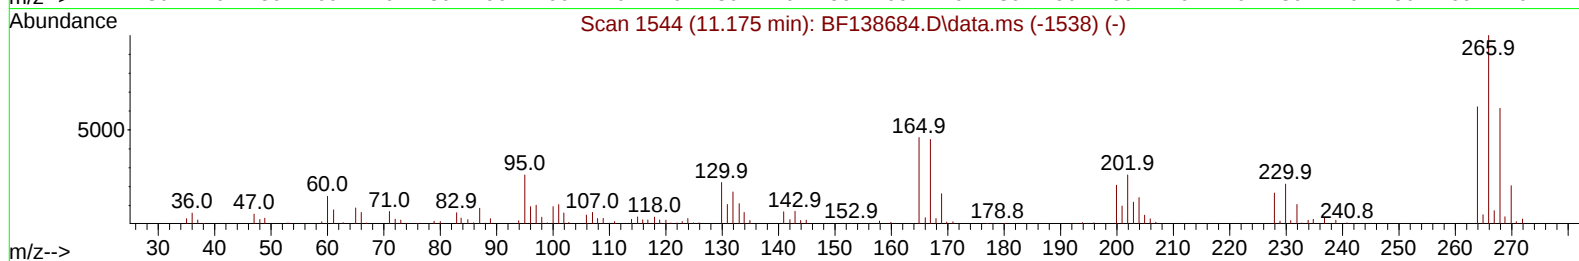
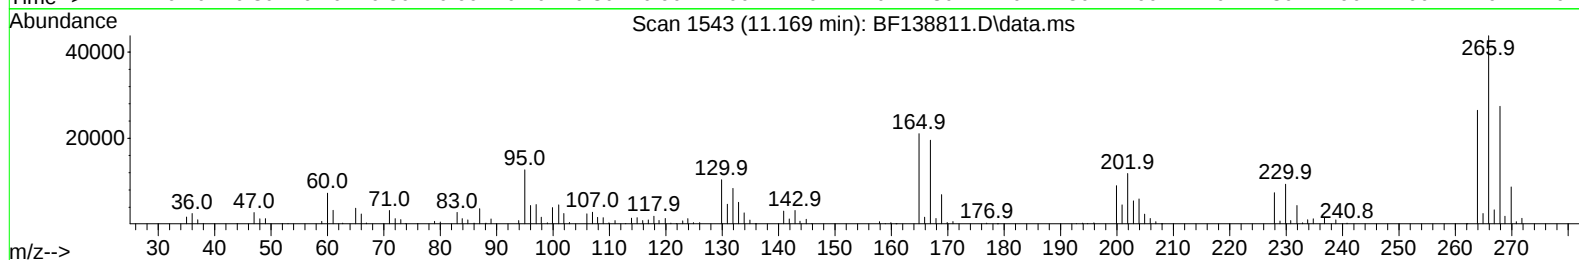


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080624\
Data File : BF138811.D
Acq On : 06 Aug 2024 17:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 17:56:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

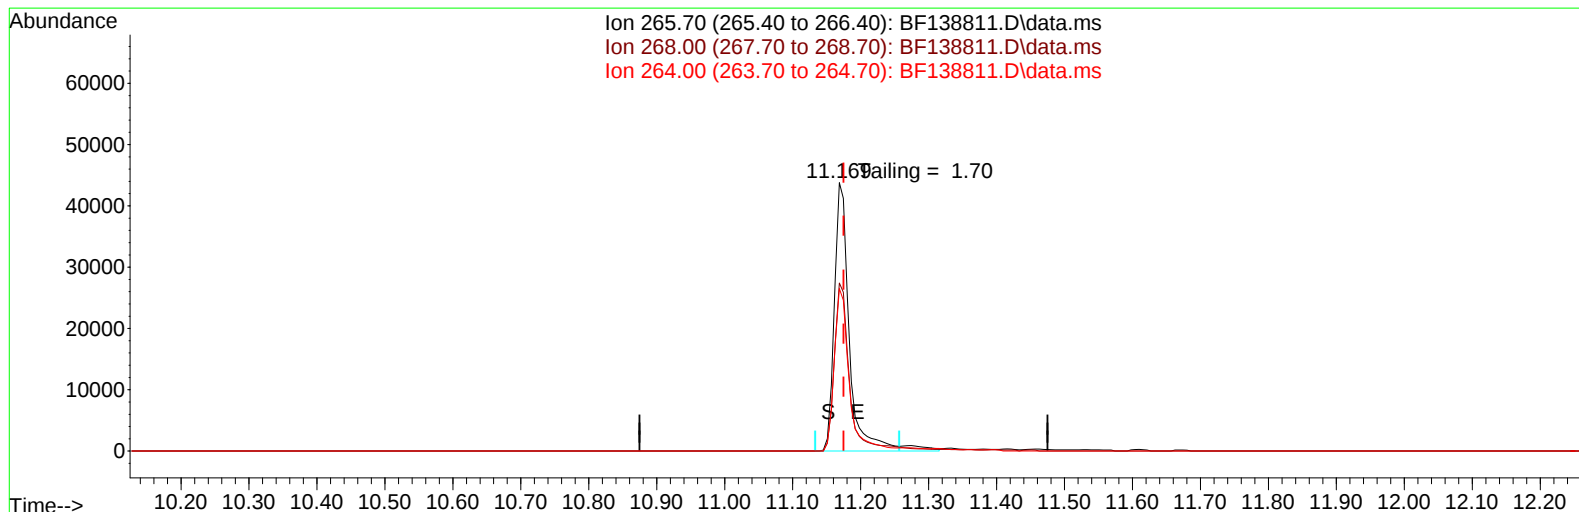

TIC: BF138811.D\data.ms

(70) Pentachlorophenol (C)




11.169min (-0.006) 51517.64 ng

response 66454

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	62.64
264.00	62.20	60.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080624\
Data File : BF138811.D
Acq On : 06 Aug 2024 17:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 17:56:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

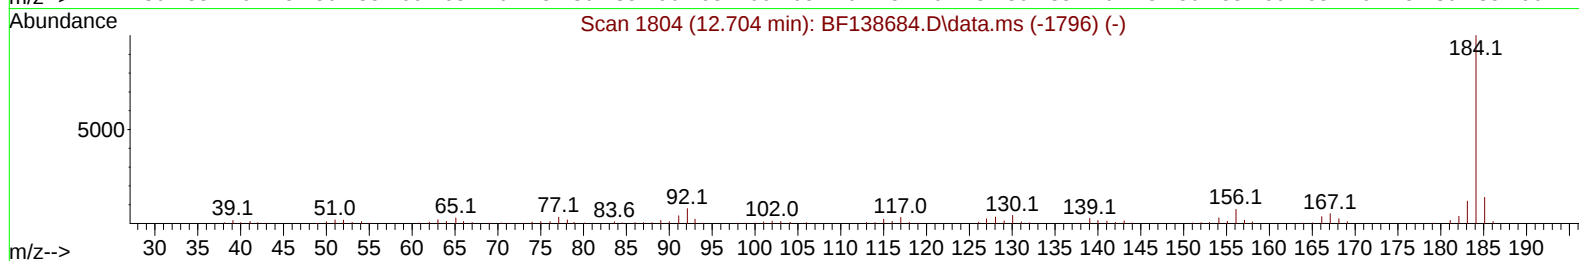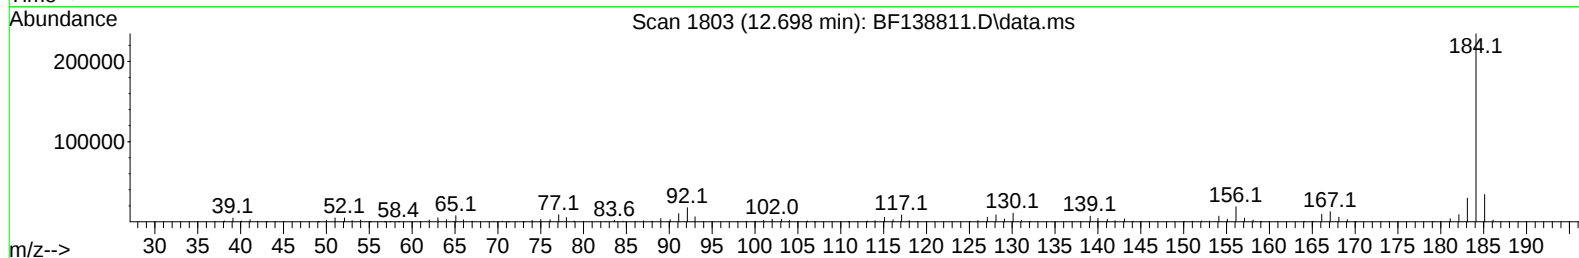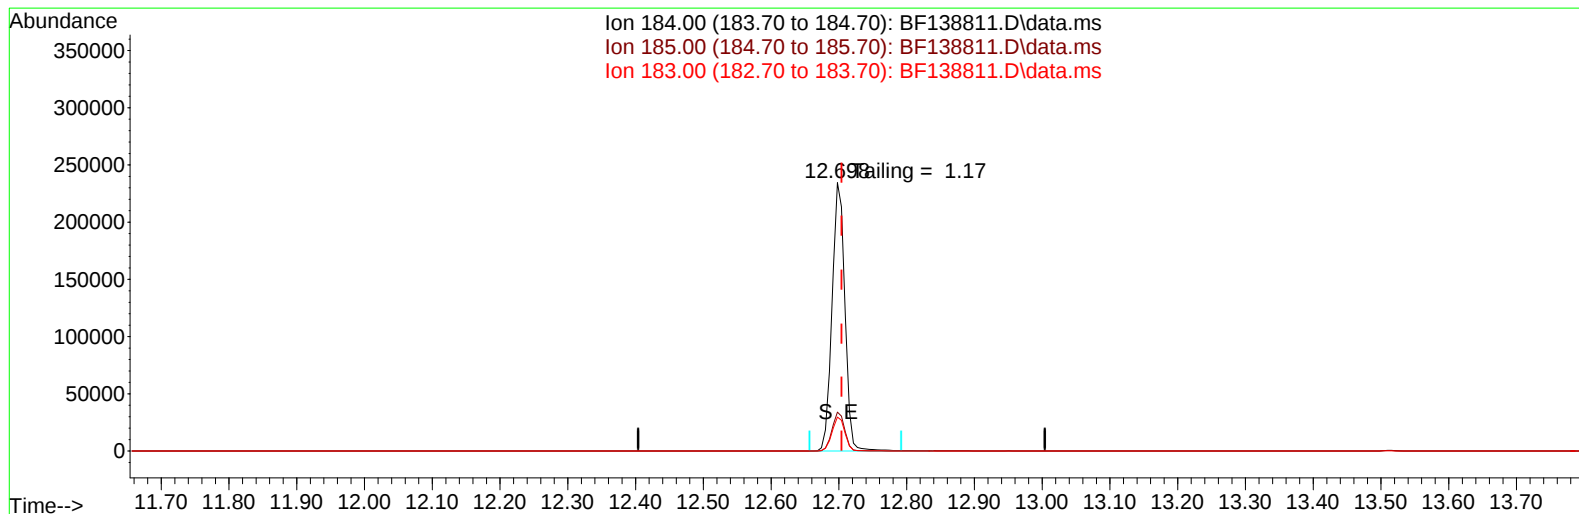

TIC: BF138811.D\data.ms

(77) Benzidine

12.698min (-0.006) 0.00 ng

response 307954

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.50
183.00	12.00	12.65
0.00	0.00	0.00