

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080624\
 Data File : BF138826.D
 Acq On : 07 Aug 2024 01:34
 Operator : RC/JU
 Sample : P3441-01RE
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BU-02-08012024RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138826.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.122	3	5	19	rVB	492015	628053	62.46%	8.086%
2	3.387	215	220	232	rBV	4944	16383	1.63%	0.211%
3	5.063	500	505	520	rVB	36807	56248	5.59%	0.724%
4	5.469	569	574	589	rBV	667670	869518	86.48%	11.195%
5	6.481	741	746	761	rBV	678110	888790	88.39%	11.443%
6	6.839	802	807	812	rBV	226911	274421	27.29%	3.533%
7	7.404	897	903	914	rBV	450561	580849	57.77%	7.479%
8	7.657	941	946	953	rBV	15394	21119	2.10%	0.272%
9	8.122	1019	1025	1031	rBV	271074	356548	35.46%	4.591%
10	8.439	1074	1079	1090	rVB	18788	32567	3.24%	0.419%
11	9.192	1201	1207	1212	rBV	825919	1005481	100.00%	12.946%
12	9.869	1318	1322	1332	rVB	280824	359090	35.71%	4.623%
13	9.963	1333	1338	1346	rVB2	14655	23559	2.34%	0.303%
14	10.663	1452	1457	1470	rBV	328334	430534	42.82%	5.543%
15	11.357	1570	1575	1586	rBV	238482	318710	31.70%	4.103%
16	11.880	1657	1664	1672	rBV5	18152	33529	3.33%	0.432%
17	11.968	1676	1679	1686	rVB	5883	11272	1.12%	0.145%
18	12.568	1777	1781	1786	rBV	37975	47724	4.75%	0.614%
19	12.798	1814	1820	1826	rBV	42116	58667	5.83%	0.755%
20	12.939	1838	1844	1849	rBV	566441	711936	70.81%	9.166%
21	13.233	1890	1894	1900	rBV2	5737	10642	1.06%	0.137%
22	13.321	1905	1909	1912	rBV	8481	13148	1.31%	0.169%
23	13.633	1957	1962	1968	rVB3	5448	11040	1.10%	0.142%
24	13.851	1993	1999	2007	rVB3	27971	57405	5.71%	0.739%
25	13.915	2007	2010	2014	rVV	9687	13467	1.34%	0.173%
26	13.998	2018	2024	2033	rVB2	199675	323743	32.20%	4.168%
27	14.492	2103	2108	2114	rVB6	15441	33547	3.34%	0.432%
28	14.827	2162	2165	2170	rVB	10694	13335	1.33%	0.172%
29	15.033	2196	2200	2205	rBV	23944	45575	4.53%	0.587%
30	15.086	2205	2209	2214	rVB	27055	42487	4.23%	0.547%
31	15.157	2216	2221	2230	rVB8	11669	33246	3.31%	0.428%
32	15.333	2247	2251	2256	rVB	16487	24066	2.39%	0.310%
33	15.392	2257	2261	2266	rVV	19578	33554	3.34%	0.432%
34	15.456	2267	2272	2285	rVB	136267	223336	22.21%	2.876%
35	15.886	2341	2345	2350	rVB	15863	23548	2.34%	0.303%
36	17.203	2565	2569	2581	rVB9	16455	41959	4.17%	0.540%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080624\
Data File : BF138826.D
Acq On : 07 Aug 2024 01:34
Operator : RC/JU
Sample : P3441-01RE
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-02-08012024RE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	17.533	2614	2625	2636	rBV9	17347	67628	6.73%	0.871%
38	18.486	2780	2787	2793	rVB8	11694	30064	2.99%	0.387%




Sum of corrected areas: 7766788

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080624\
Data File : BF138826.D
Acq On : 07 Aug 2024 01:34
Operator : RC/JU
Sample : P3441-01RE
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-02-08012024RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

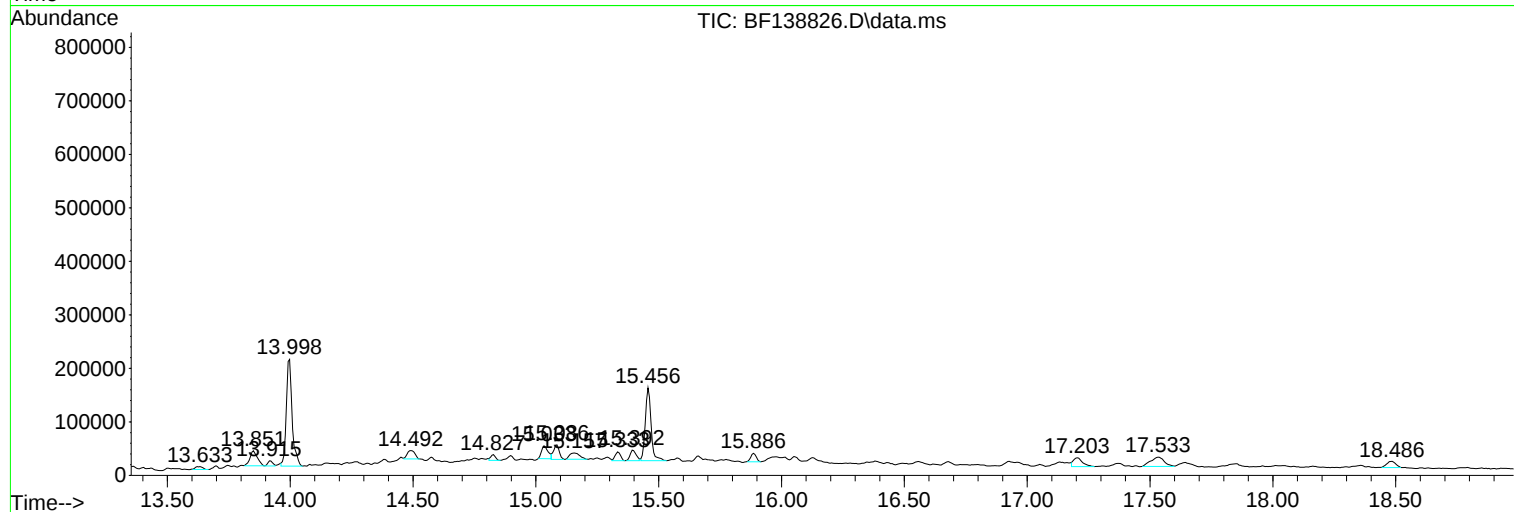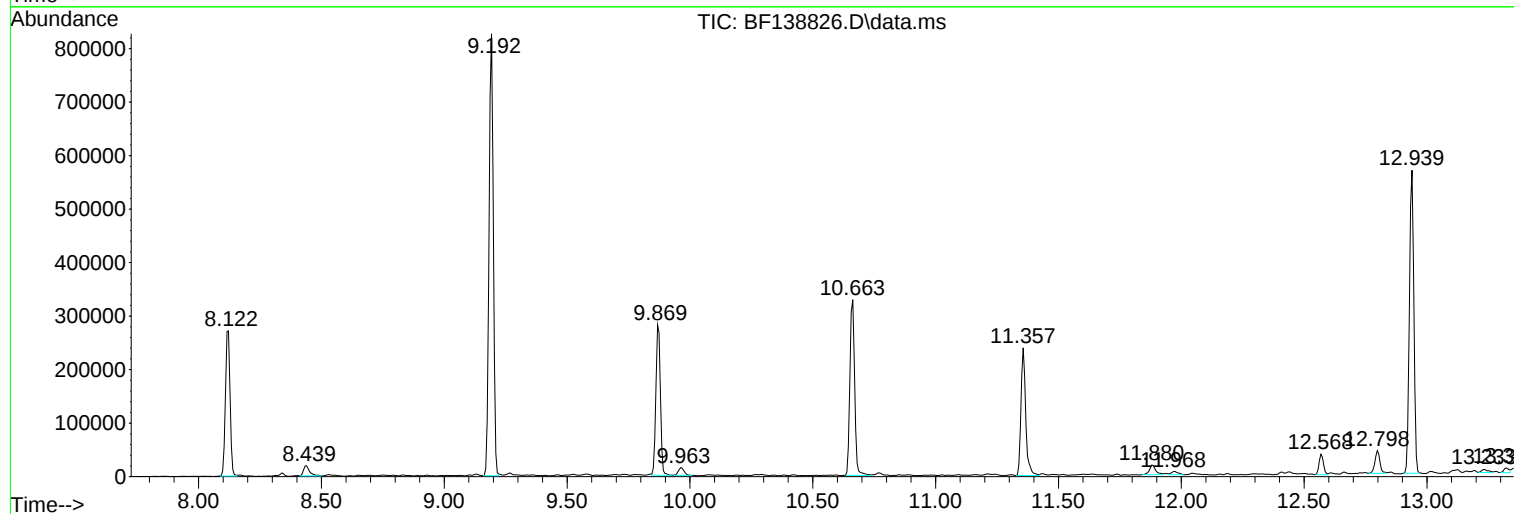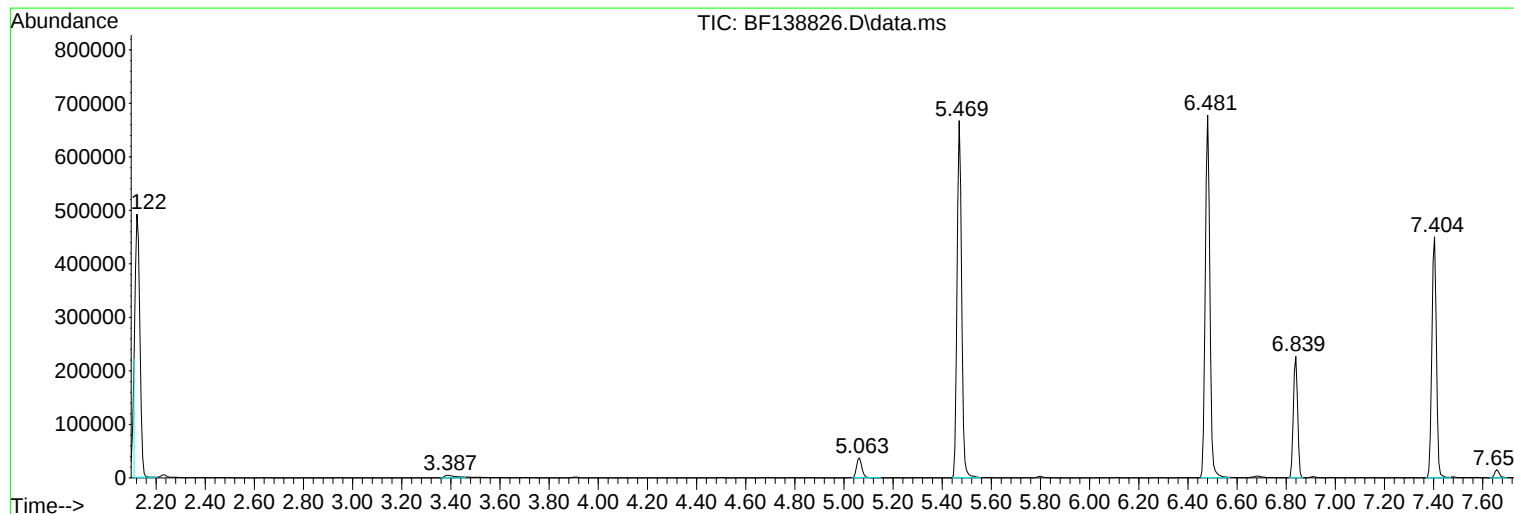

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080624\
Data File : BF138826.D
Acq On : 07 Aug 2024 01:34
Operator : RC/JU
Sample : P3441-01RE
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-02-08012024RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080624\
Data File : BF138826.D
Acq On : 07 Aug 2024 01:34
Operator : RC/JU
Sample : P3441-01RE
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-02-08012024RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------