

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080624\
 Data File : BF138832.D
 Acq On : 07 Aug 2024 04:42
 Operator : RC/JU
 Sample : P3362-02DL 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 VNJ-220DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138832.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.046	498	502	512	rBB	7374	10581	2.69%	0.225%
2	5.469	569	574	594	rBV	127408	181805	46.24%	3.865%
3	6.481	741	746	767	rBV	131872	187465	47.68%	3.986%
4	6.840	802	807	812	rBV	198617	240831	61.25%	5.120%
5	7.398	898	902	914	rBV	86668	114037	29.00%	2.425%
6	8.122	1019	1025	1034	rBV	223761	293242	74.58%	6.235%
7	8.834	1142	1146	1150	rBB	5700	6829	1.74%	0.145%
8	8.928	1158	1162	1167	rBB	11937	14280	3.63%	0.304%
9	9.192	1202	1207	1215	rBV	156271	192077	48.85%	4.084%
10	9.292	1220	1224	1229	rBB	12942	14675	3.73%	0.312%
11	9.457	1247	1252	1257	rBB	15369	21610	5.50%	0.459%
12	9.528	1260	1264	1267	rVV	18826	25093	6.38%	0.533%
13	9.557	1267	1269	1273	rVB	10506	10404	2.65%	0.221%
14	9.645	1280	1284	1290	rVB	5742	8255	2.10%	0.176%
15	9.733	1293	1299	1302	rBV2	4060	4896	1.25%	0.104%
16	9.869	1315	1322	1326	rBV	209876	284041	72.24%	6.039%
17	9.904	1326	1328	1333	rVV	93312	96324	24.50%	2.048%
18	9.963	1333	1338	1345	rVV2	34115	52593	13.38%	1.118%
19	10.028	1345	1349	1353	rVV2	3186	4217	1.07%	0.090%
20	10.075	1353	1357	1361	rVV	54567	66897	17.01%	1.422%
21	10.110	1361	1363	1367	rVB	3950	4280	1.09%	0.091%
22	10.275	1385	1391	1397	rBV3	2673	4860	1.24%	0.103%
23	10.422	1411	1416	1421	rBV	96800	124243	31.60%	2.641%
24	10.504	1421	1430	1433	rVV2	12016	26698	6.79%	0.568%
25	10.575	1435	1442	1446	rVB2	15649	25133	6.39%	0.534%
26	10.663	1452	1457	1462	rBV	73724	100008	25.43%	2.126%
27	10.769	1471	1475	1477	rBV	4221	5336	1.36%	0.113%
28	10.792	1477	1479	1484	rVB2	4199	4452	1.13%	0.095%
29	10.963	1502	1508	1511	rBV2	15227	21618	5.50%	0.460%
30	11.045	1519	1522	1526	rVB3	3804	4427	1.13%	0.094%
31	11.092	1526	1530	1532	rVV5	3711	5919	1.51%	0.126%
32	11.116	1532	1534	1539	rVV3	4900	6235	1.59%	0.133%
33	11.163	1539	1542	1546	rVV2	3477	4519	1.15%	0.096%
34	11.204	1546	1549	1554	rVV2	5831	8689	2.21%	0.185%
35	11.251	1554	1557	1564	rVB	18790	23208	5.90%	0.493%
36	11.357	1570	1575	1577	rBV	198628	269502	68.54%	5.730%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080624\
 Data File : BF138832.D
 Acq On : 07 Aug 2024 04:42
 Operator : RC/JU
 Sample : P3362-02DL 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 VNJ-220DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	11.380	1577	1579	1584	rVV	343418	393194	100.00%	8.360%
38	11.433	1584	1588	1592	rVV	33454	43617	11.09%	0.927%
39	11.469	1592	1594	1600	rVB2	3950	5654	1.44%	0.120%
40	11.592	1609	1615	1622	rBV	15272	22756	5.79%	0.484%
41	11.769	1642	1645	1650	rVB3	3468	4228	1.08%	0.090%
42	11.857	1655	1660	1662	rBV	27551	34187	8.69%	0.727%
43	11.886	1662	1665	1669	rVV	37331	45965	11.69%	0.977%
44	11.933	1669	1673	1676	rVV	11405	16499	4.20%	0.351%
45	11.975	1676	1680	1689	rVB2	46379	76418	19.44%	1.625%
46	12.151	1707	1710	1714	rBV	15245	18100	4.60%	0.385%
47	12.304	1732	1736	1738	rBV	4145	5092	1.30%	0.108%
48	12.404	1749	1753	1757	rBV	9238	13670	3.48%	0.291%
49	12.445	1757	1760	1765	rVV3	5167	9471	2.41%	0.201%
50	12.492	1766	1768	1774	rVB5	4181	6147	1.56%	0.131%
51	12.569	1777	1781	1786	rBV	205663	262107	66.66%	5.573%
52	12.604	1786	1787	1790	rVB2	6237	5317	1.35%	0.113%
53	12.722	1803	1807	1813	rBV2	5186	8972	2.28%	0.191%
54	12.798	1813	1820	1826	rVV2	128220	207511	52.78%	4.412%
55	12.851	1826	1829	1833	rVB3	8123	10284	2.62%	0.219%
56	12.933	1835	1843	1851	rVB	146229	199090	50.63%	4.233%
57	13.016	1852	1857	1861	rBV3	9915	18282	4.65%	0.389%
58	13.127	1868	1876	1880	rBV	25233	41033	10.44%	0.872%
59	13.192	1883	1887	1890	rBV	27129	34344	8.73%	0.730%
60	13.227	1890	1893	1897	rVV2	8643	11131	2.83%	0.237%
61	13.321	1906	1909	1912	rBV2	4302	6774	1.72%	0.144%
62	13.357	1912	1915	1927	rVB9	7870	17205	4.38%	0.366%
63	13.616	1955	1959	1960	rBV3	4487	5530	1.41%	0.118%
64	13.639	1961	1963	1966	rVB3	4315	4940	1.26%	0.105%
65	13.745	1978	1981	1984	rBV	7208	8802	2.24%	0.187%
66	13.774	1984	1986	1989	rVB2	4911	4657	1.18%	0.099%
67	13.851	1995	1999	2007	rVB6	10275	20989	5.34%	0.446%
68	13.998	2016	2024	2035	rVB2	220152	366413	93.19%	7.790%
69	14.104	2039	2042	2045	rVB2	5137	5728	1.46%	0.122%
70	14.380	2087	2089	2093	rVB2	4634	4585	1.17%	0.097%
71	14.610	2124	2128	2133	rVB	21944	27254	6.93%	0.579%
72	15.033	2196	2200	2208	rBV2	16693	30553	7.77%	0.650%
73	15.145	2215	2219	2222	rBV4	6273	11748	2.99%	0.250%
74	15.333	2247	2251	2257	rVB	9651	15625	3.97%	0.332%
75	15.398	2257	2262	2266	rBV	11449	19011	4.84%	0.404%
76	15.457	2267	2272	2281	rBV	116354	178847	45.49%	3.802%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080624\
Data File : BF138832.D
Acq On : 07 Aug 2024 04:42
Operator : RC/JU
Sample : P3362-02DL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VNJ-220DL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	15.886	2342	2345	2351	rVB3	8405	12507	3.18%	0.266%
----	--------	------	------	------	------	------	-------	-------	--------


Sum of corrected areas: 4703516

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080624\
Data File : BF138832.D
Acq On : 07 Aug 2024 04:42
Operator : RC/JU
Sample : P3362-02DL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VNJ-220DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

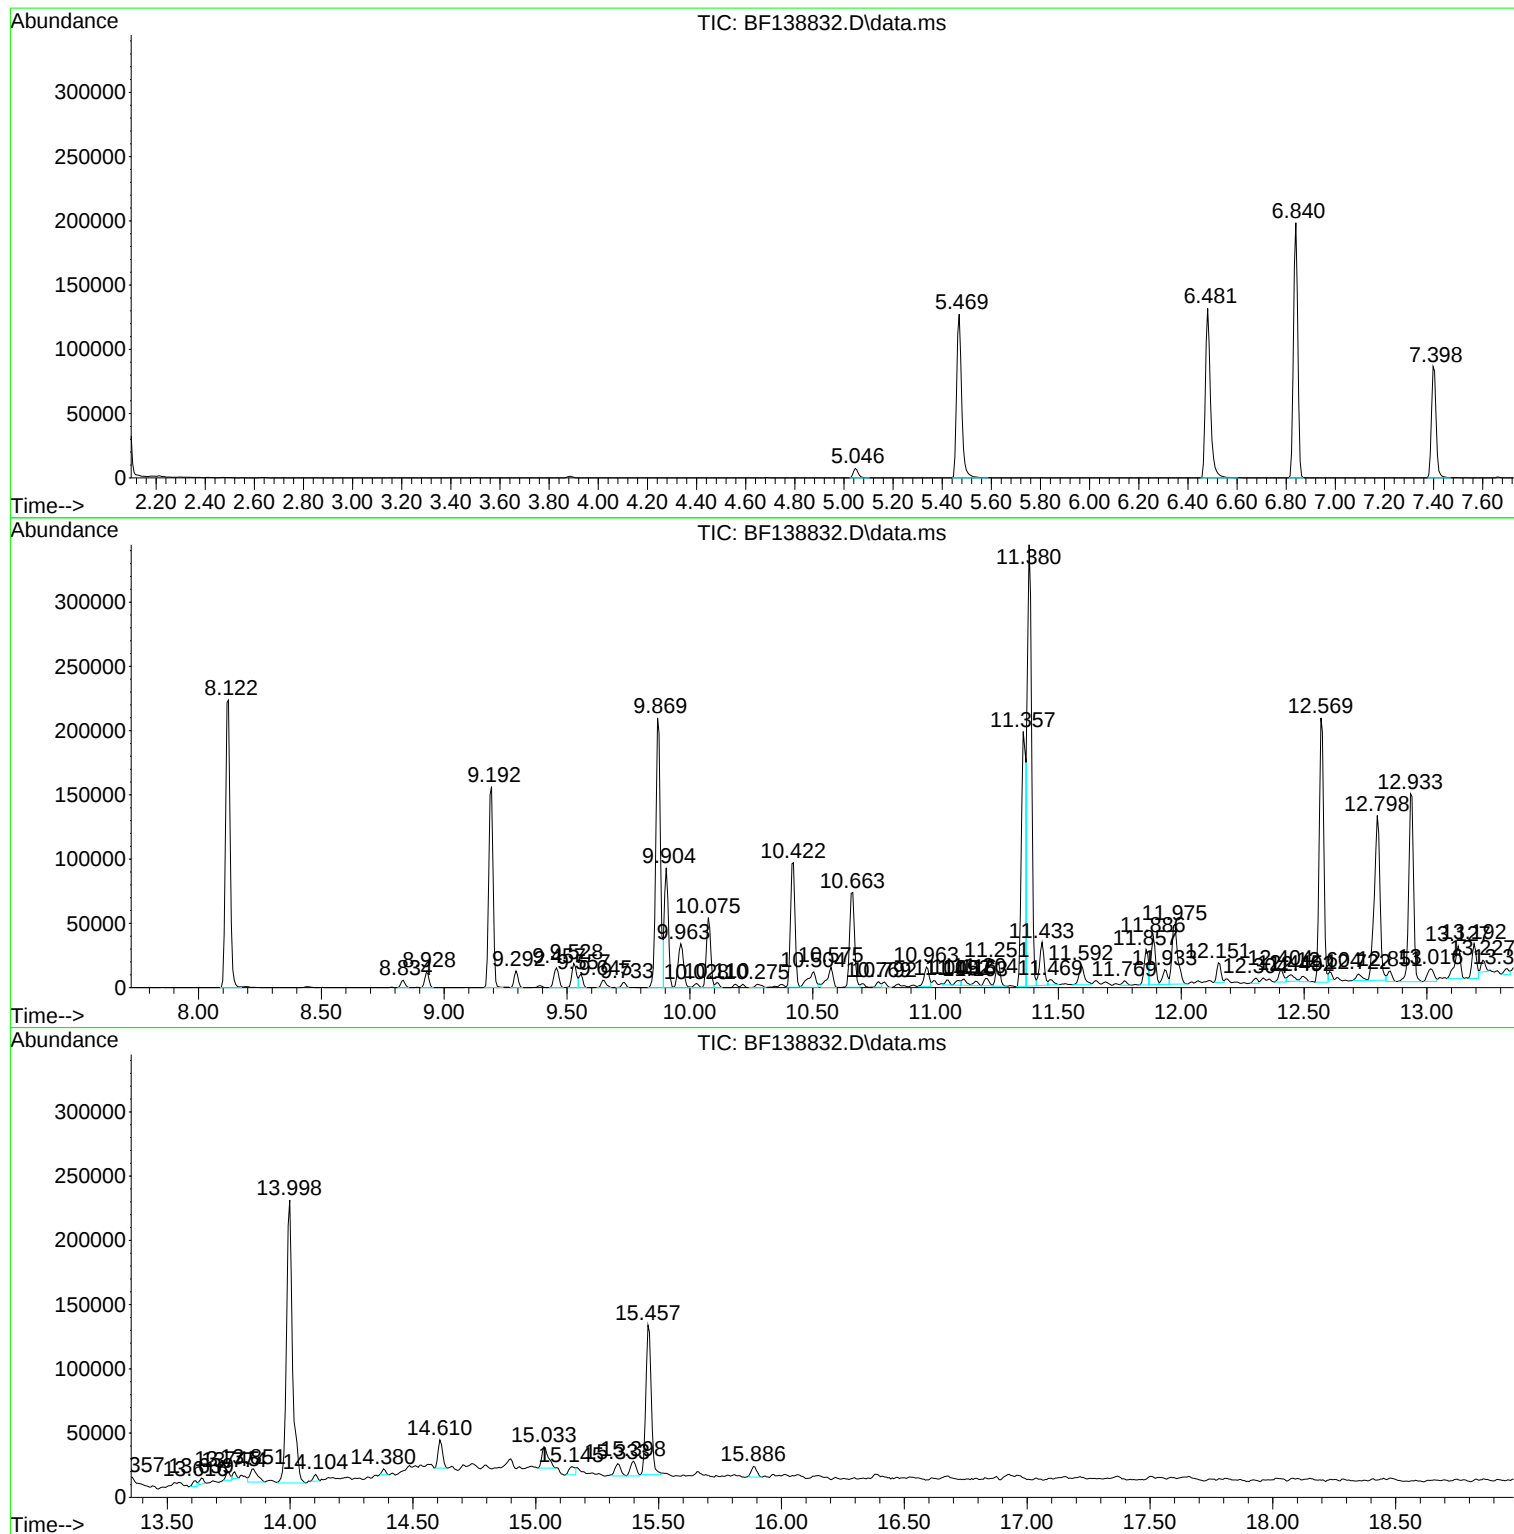

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080624\
Data File : BF138832.D
Acq On : 07 Aug 2024 04:42
Operator : RC/JU
Sample : P3362-02DL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VNJ-220DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080624\
Data File : BF138832.D
Acq On : 07 Aug 2024 04:42
Operator : RC/JU
Sample : P3362-02DL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VNJ-220DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------