


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF080624\  
Data File : BF138804.D  
Acq On : 06 Aug 2024 10:50  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF073024.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue Jul 30 17:50:01 2024

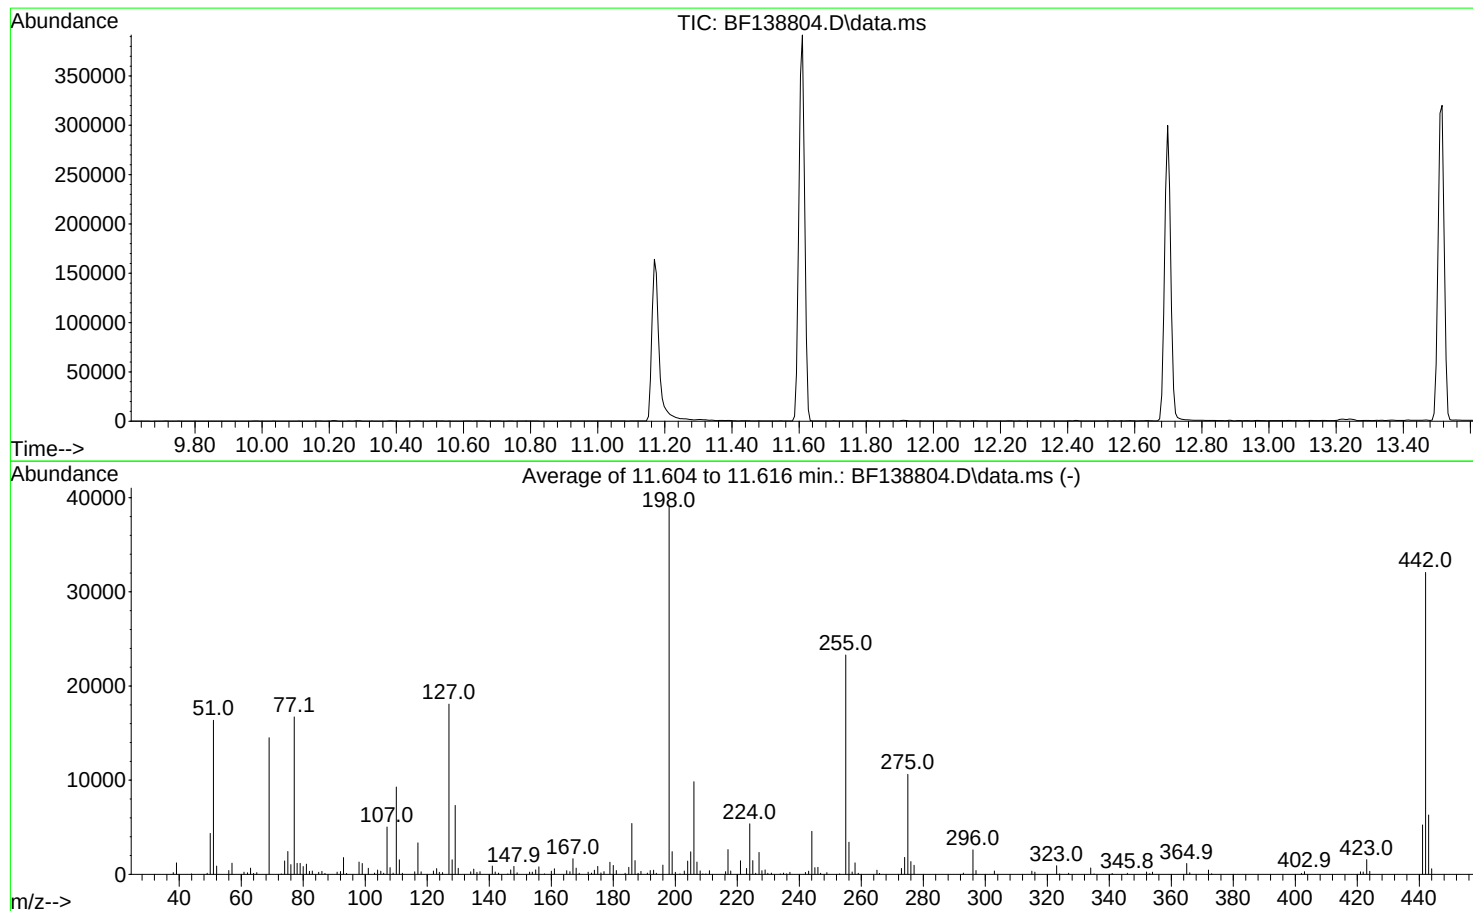




AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1611

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 41.9         | 16369      | PASS                |
| 68             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 69             | 198             | 0.00            | 100             | 37.2         | 14513      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 127            | 198             | 10              | 80              | 46.3         | 18084      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 39064      | PASS                |
| 199            | 198             | 5               | 9               | 6.2          | 2417       | PASS                |
| 275            | 198             | 10              | 60              | 27.2         | 10620      | PASS                |
| 365            | 198             | 1               | 100             | 3.0          | 1153       | PASS                |
| 441            | 198             | 0.01            | 100             | 13.4         | 5246       | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 32069      | PASS                |
| 443            | 442             | 15              | 24              | 19.7         | 6307       | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF080624\  
Data File : BF138804.D  
Acq On : 06 Aug 2024 10:50  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Aug 06 11:43:07 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF073024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jul 30 17:50:01 2024  
Response via : Initial Calibration

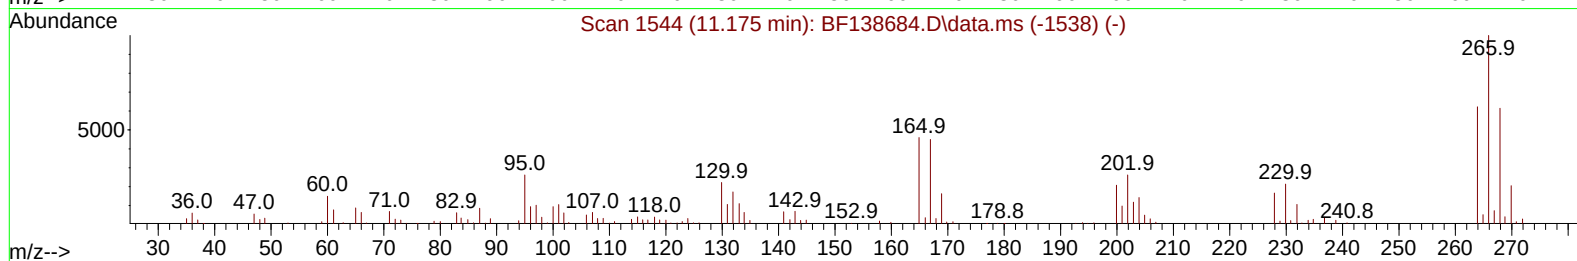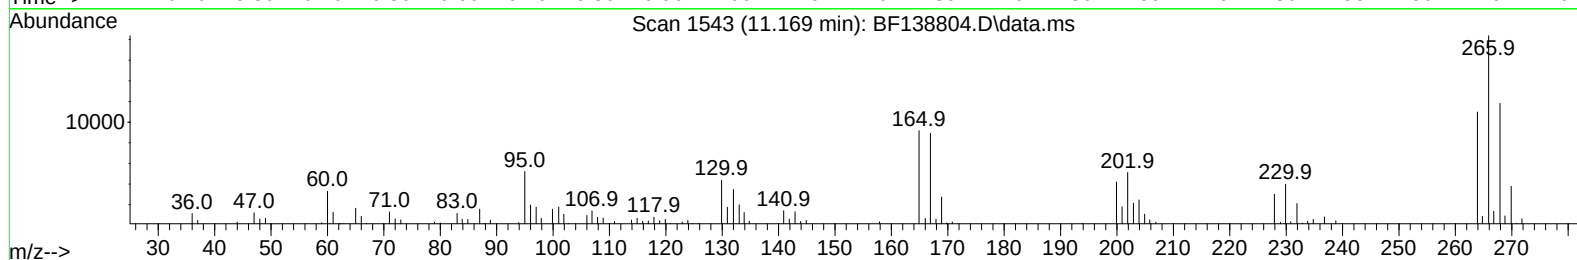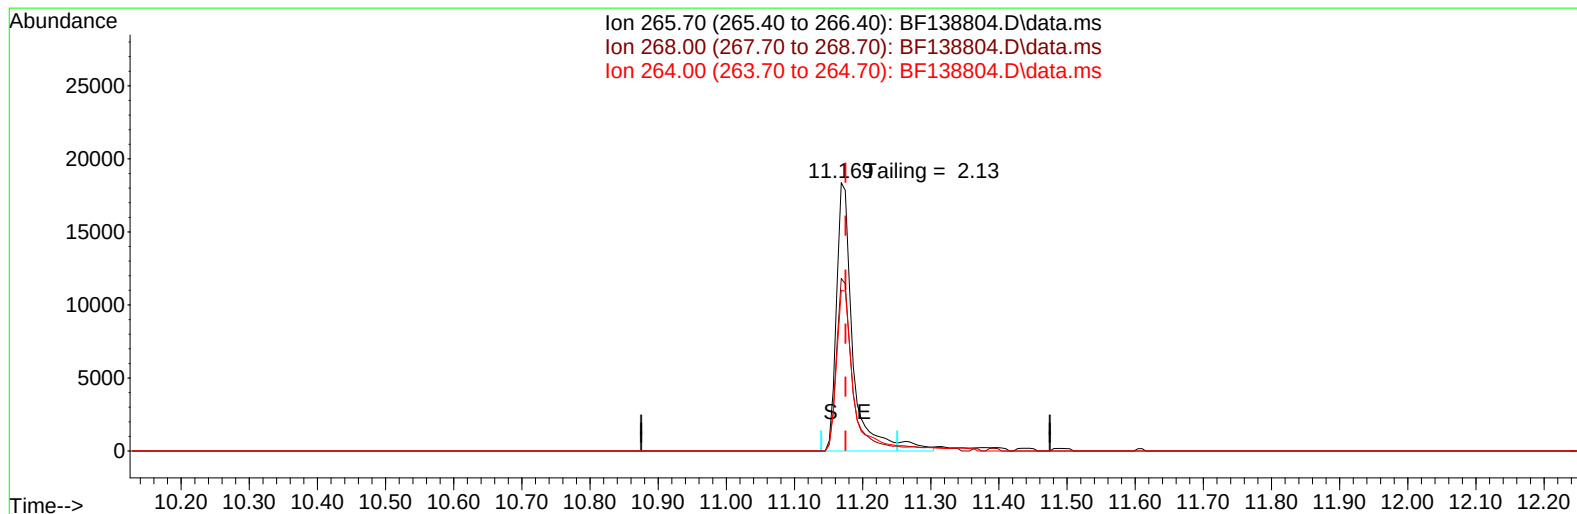

TIC: BF138804.D\data.ms

**(70) Pentachlorophenol (C)**

**11.169min (-0.006) 43761.35 ng**




**response 29768**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.50  | 64.30  |
| 264.00 | 62.20  | 59.78  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF080624\  
Data File : BF138804.D  
Acq On : 06 Aug 2024 10:50  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Aug 06 11:43:07 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF073024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jul 30 17:50:01 2024  
Response via : Initial Calibration

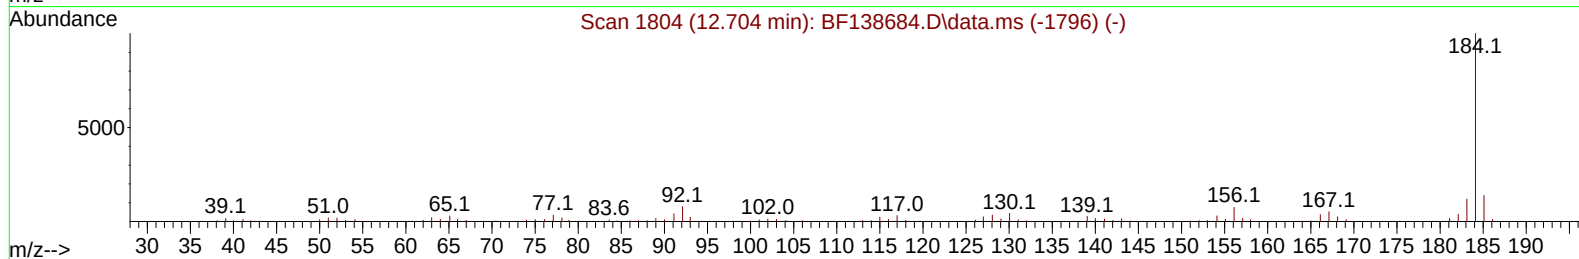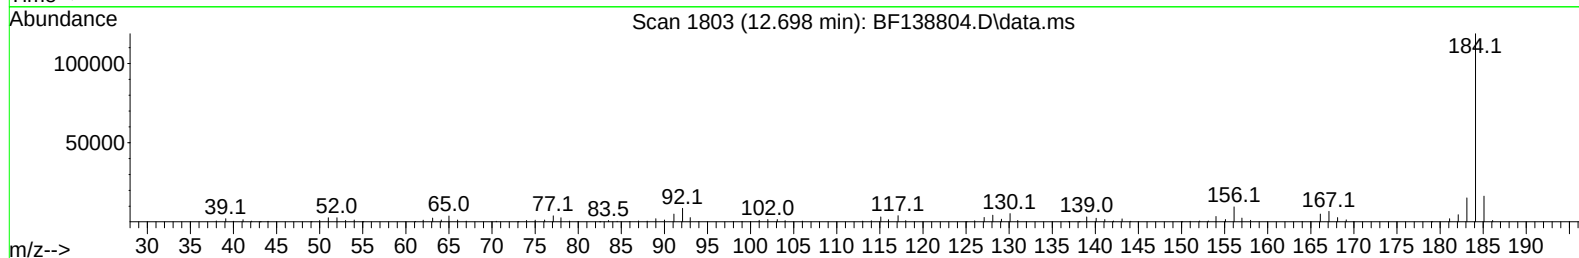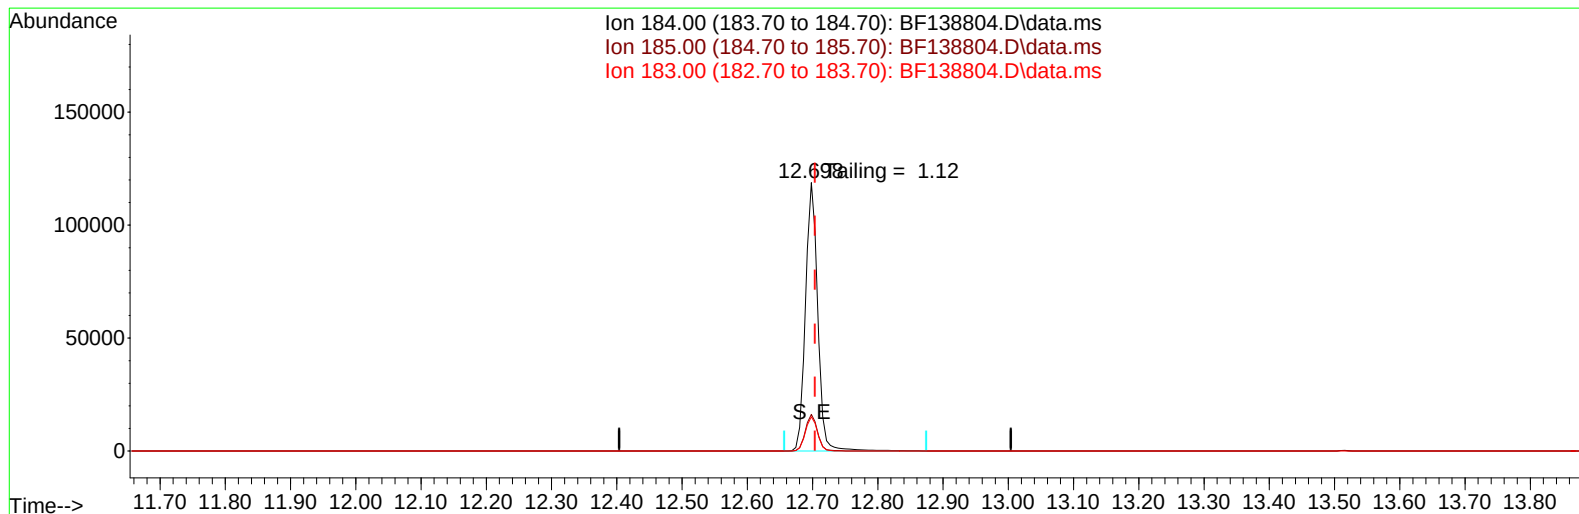

TIC: BF138804.D\data.ms

(77) Benzidine

12.698min (-0.006) 0.00 ng

response 155326

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.90  | 13.69  |
| 183.00 | 12.00  | 12.77  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 8/6/2024      | BNA_F            | <u>BF138804.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 77447            | 13.516             |
| DDD           | 1687             | 13.245             |
| DDE           | 189              | 12.88              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 1876          | 79323            | 2.37               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP