
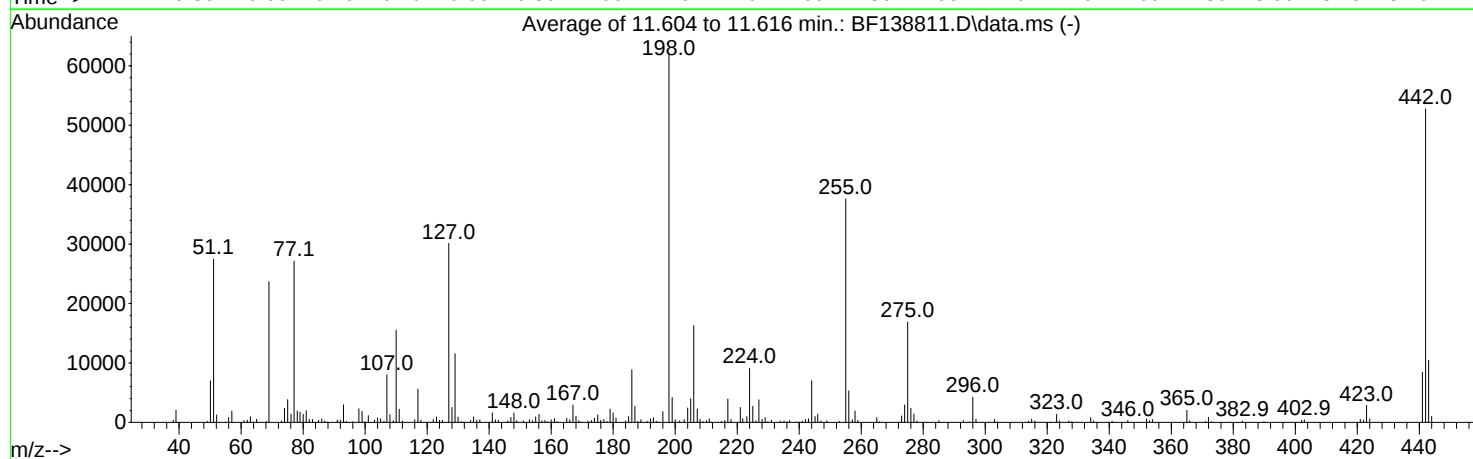


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080624\
Data File : BF138811.D
Acq On : 06 Aug 2024 17:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 30 17:50:01 2024

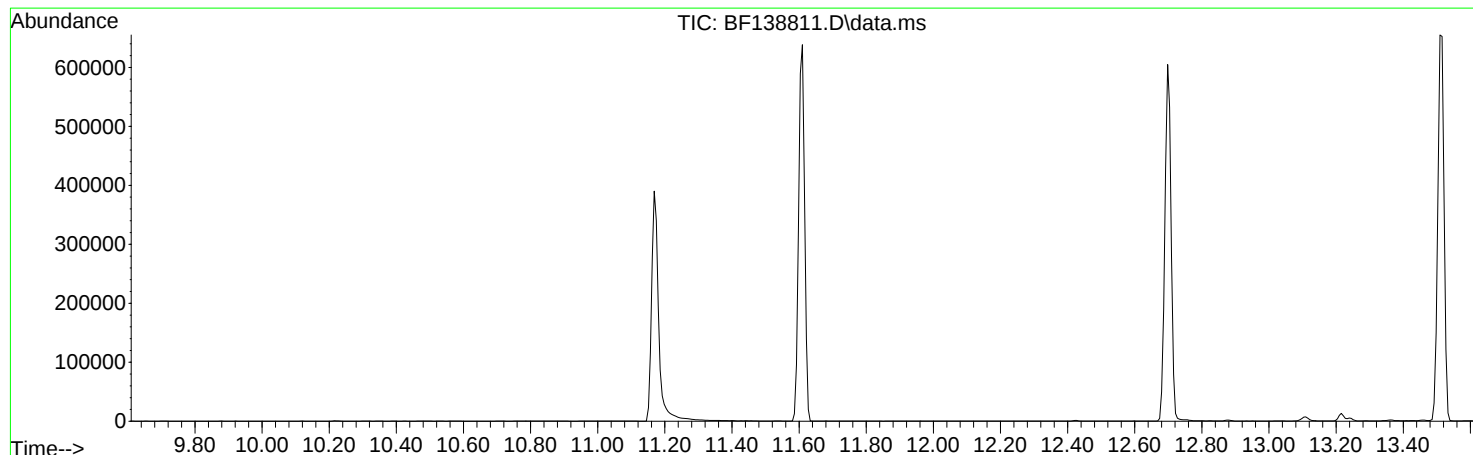




AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.4	27496	PASS
68	69	0.00	2	0.7	155	PASS
69	198	0.00	100	38.3	23701	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.7	30125	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61917	PASS
199	198	5	9	6.8	4193	PASS
275	198	10	60	27.3	16899	PASS
365	198	1	100	3.3	2031	PASS
441	198	0.01	100	13.6	8418	PASS
442	442	50	100	100.0	52747	PASS
443	442	15	24	19.8	10431	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080624\
Data File : BF138811.D
Acq On : 06 Aug 2024 17:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 06 17:56:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

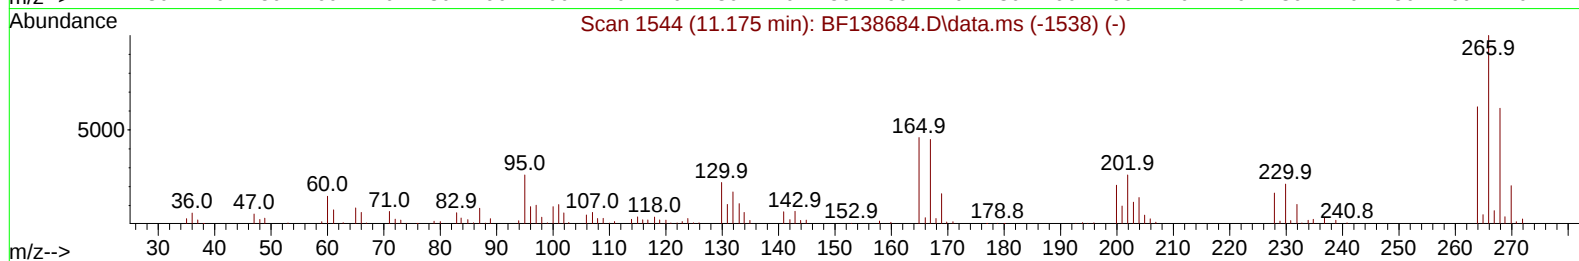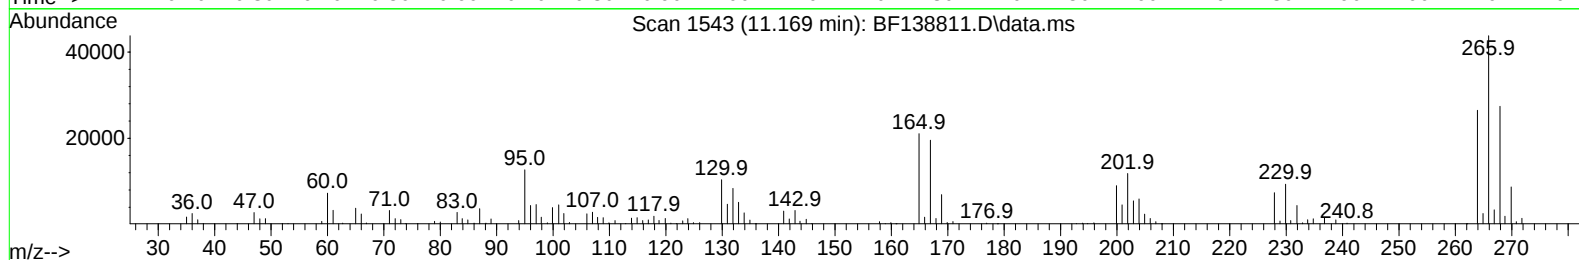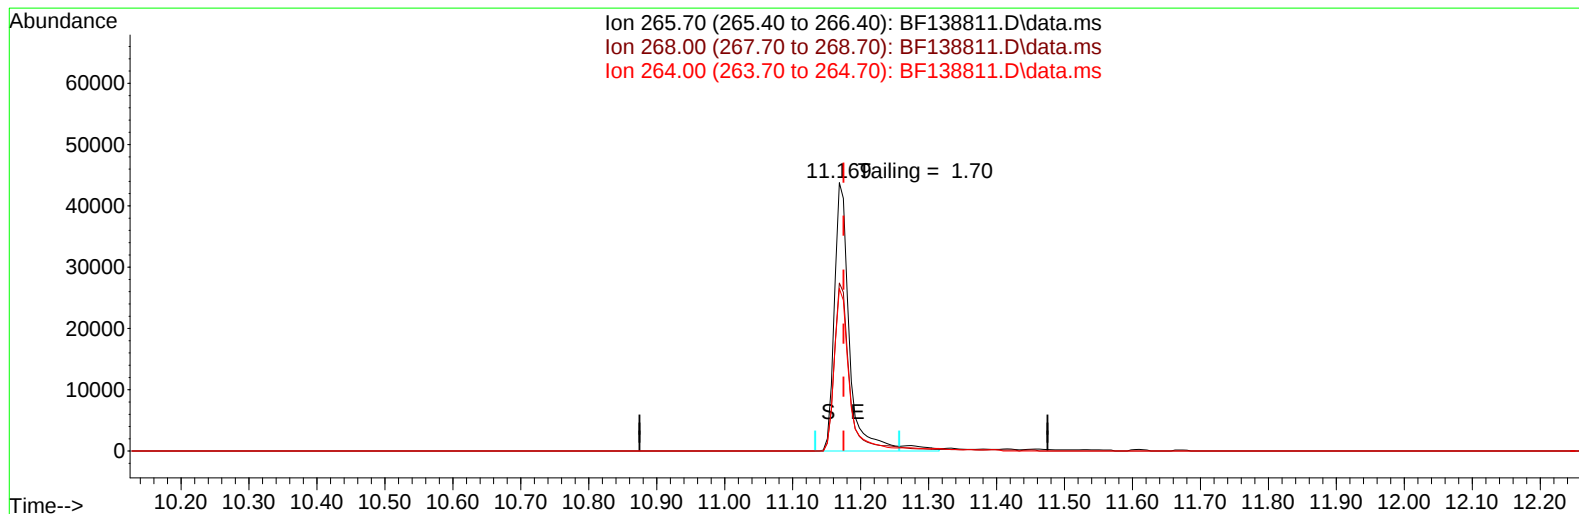

TIC: BF138811.D\data.ms

(70) Pentachlorophenol (C)

11.169min (-0.006) 51517.64 ng




response 66454

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	62.64
264.00	62.20	60.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080624\
Data File : BF138811.D
Acq On : 06 Aug 2024 17:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 06 17:56:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

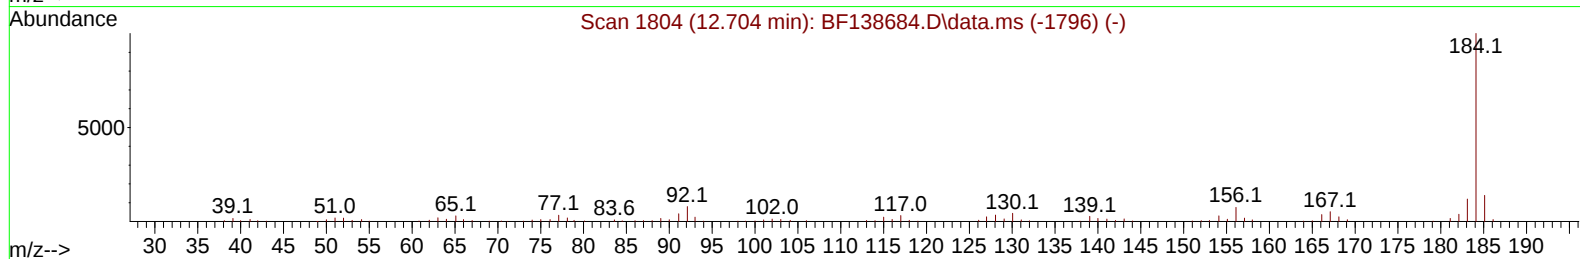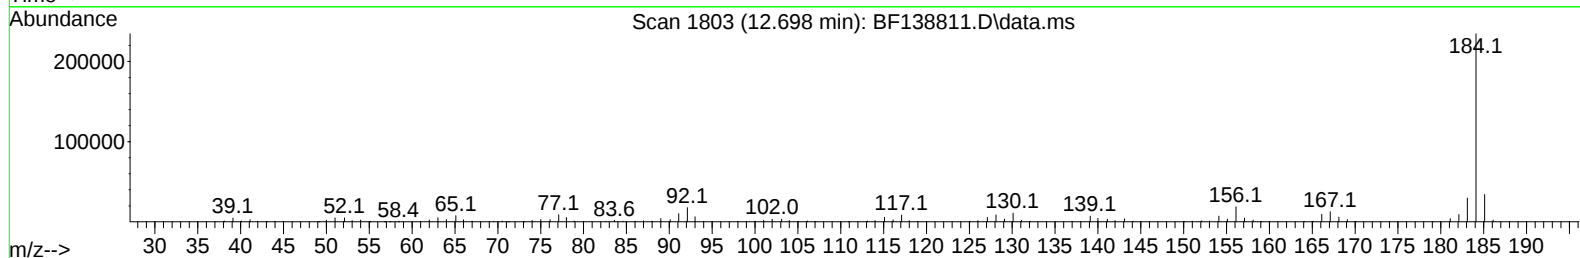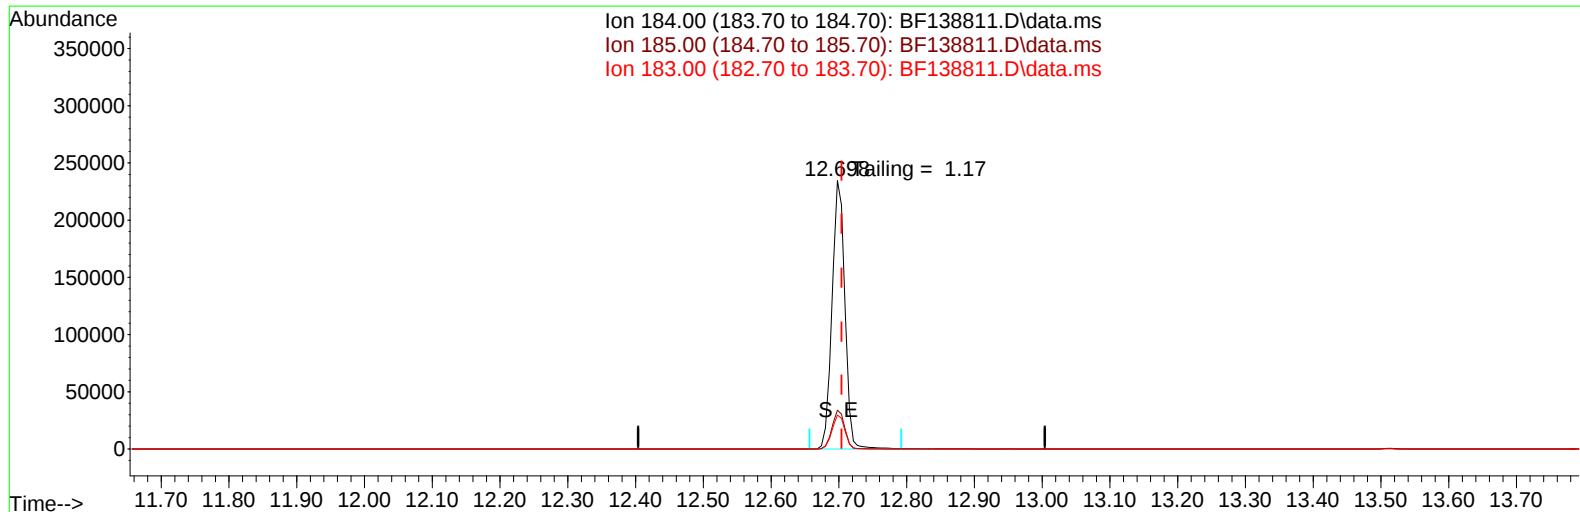

TIC: BF138811.D\data.ms

(77) Benzidine

12.698min (-0.006) 0.00 ng

response 307954

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.50
183.00	12.00	12.65
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/6/2024	BNA_F	<u>BF138811.D</u>
Compound Name	Response	Retention Time
DDT	165633	13.515
DDD	5845	13.216
DDE	576	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6421	172054	3.73

Instrument :
BNA_F
ClientSampleId :
DFTPP