
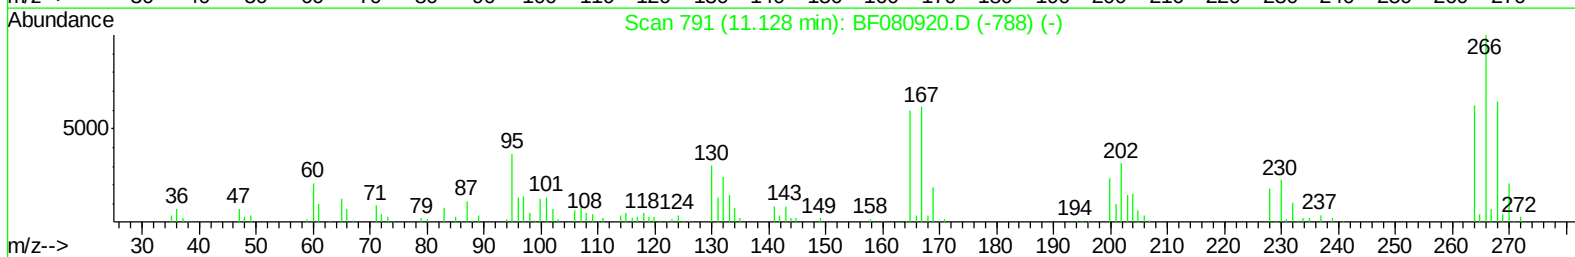
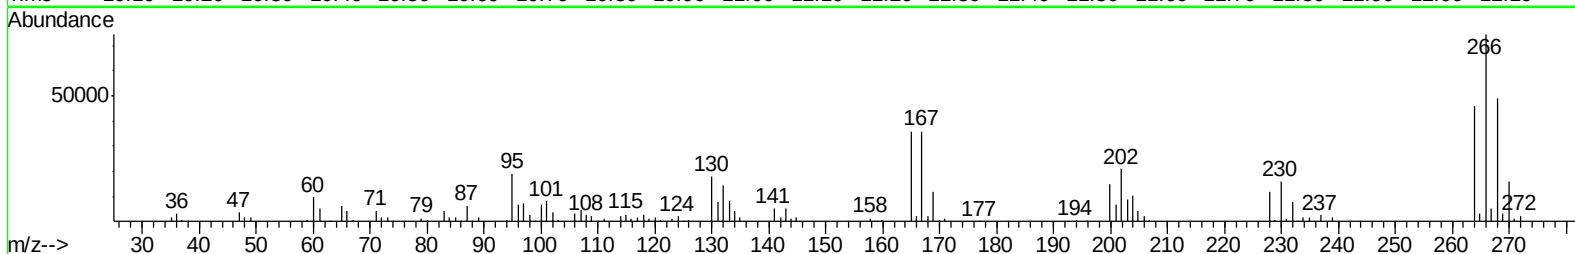


Data Path : Z:\HPCHEM1\BNA_F\Data\BF080715\
Data File : BF080916.D
Acq On : 7 Aug 2015 9:37
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 06:43:34 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 08 01:33:05 2015
Response via : Initial Calibration

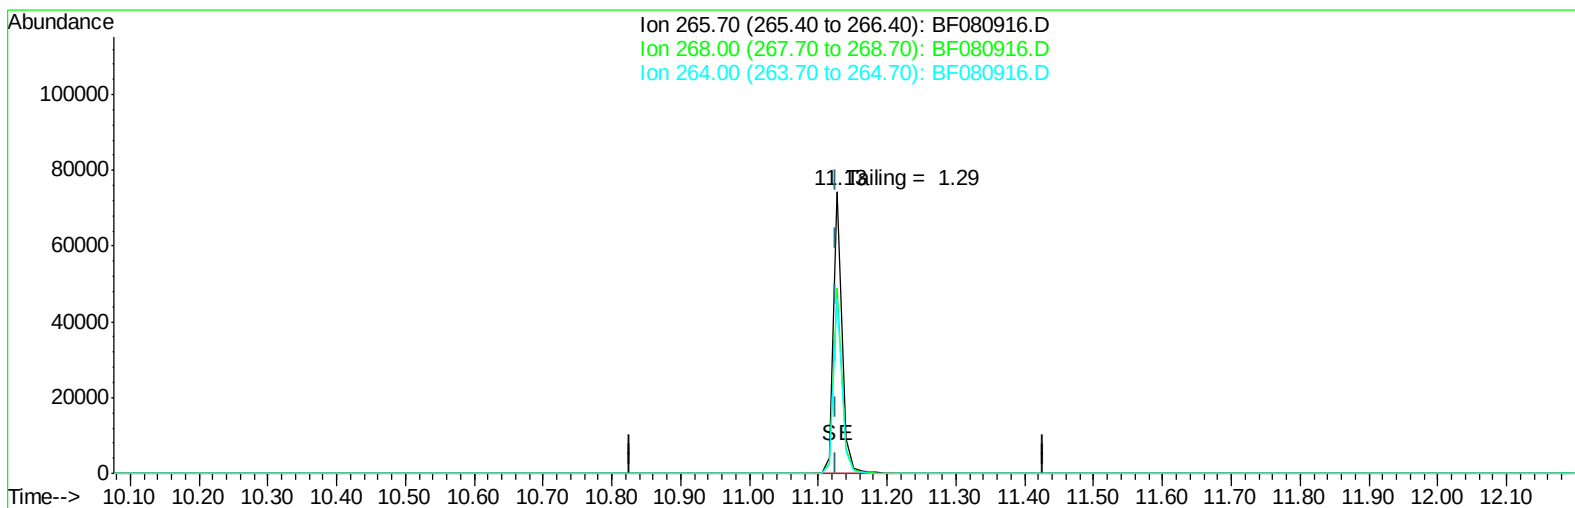

TIC: BF080916.D

(69) Pentachlorophenol (C)

11.128min (+0.001) 11913.25ng

response 62156

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	65.96
264.00	62.60	62.07
0.00	0.00	0.00