
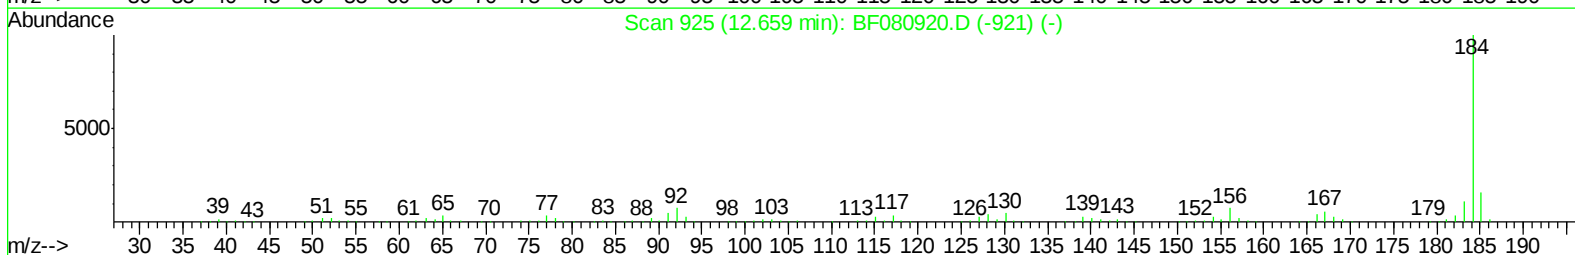
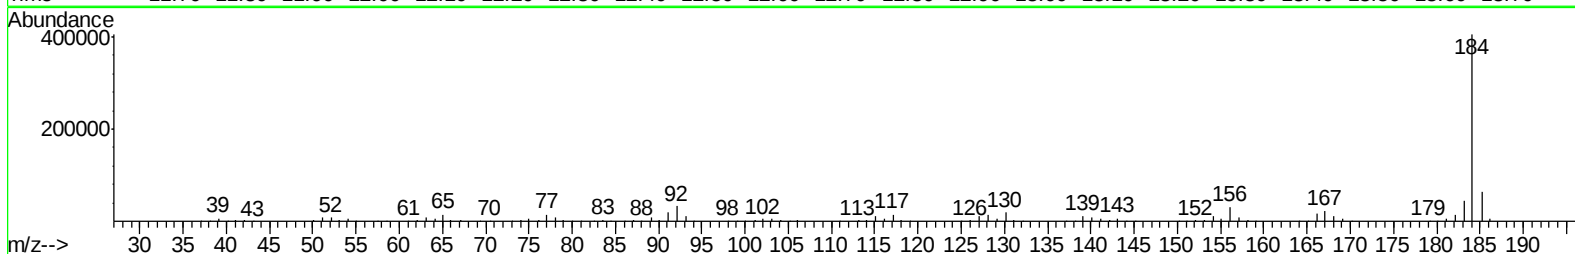


Data Path : Z:\HPCHEM1\BNA_F\Data\BF080715\
 Data File : BF080938.D
 Acq On : 7 Aug 2015 22:02
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 06:45:06 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 08 01:33:05 2015
 Response via : Initial Calibration

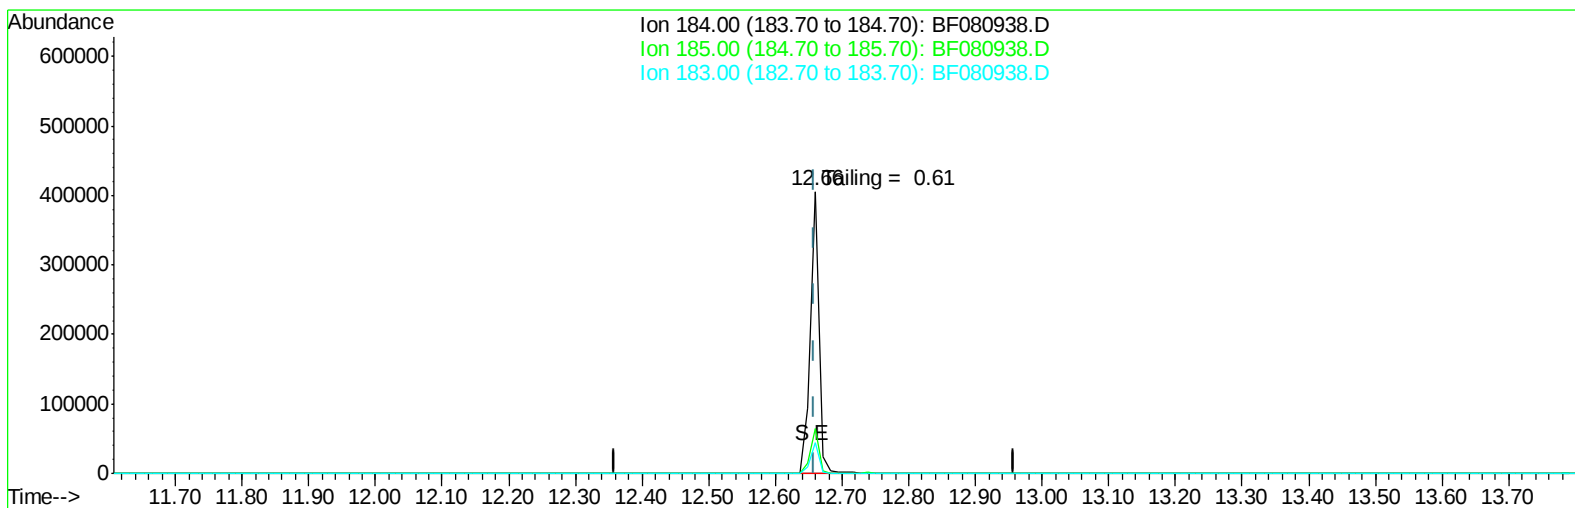

TIC: BF080938.D

(76) Benzidine




12.659min (+0.000) 0.00ng

response 368127

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	15.81
183.00	10.90	11.02
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF080715\
 Data File : BF080938.D
 Acq On : 7 Aug 2015 22:02
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 06:45:06 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 08 01:33:05 2015
 Response via : Initial Calibration

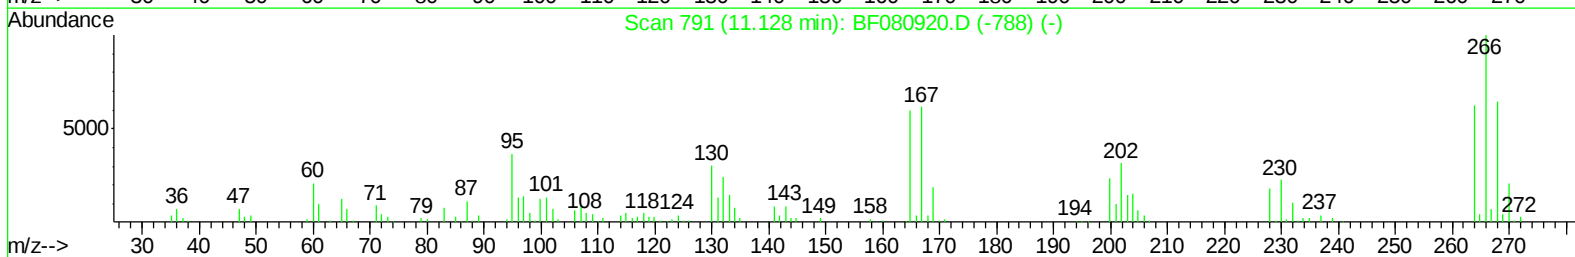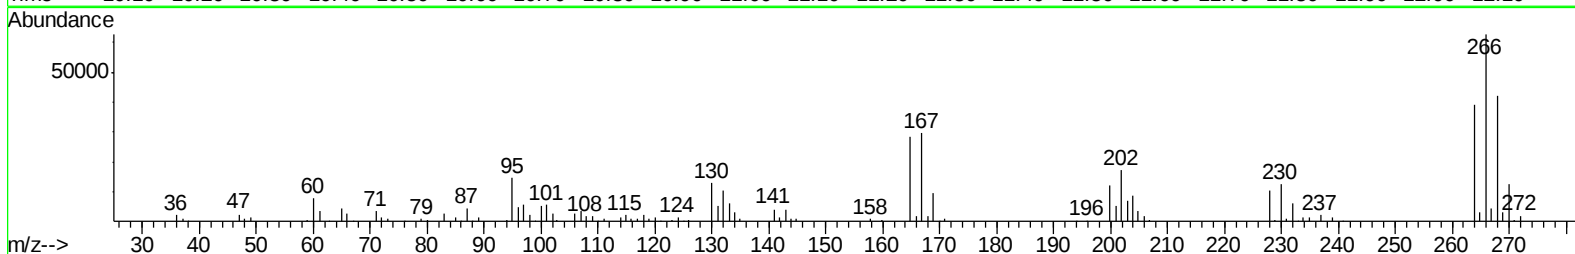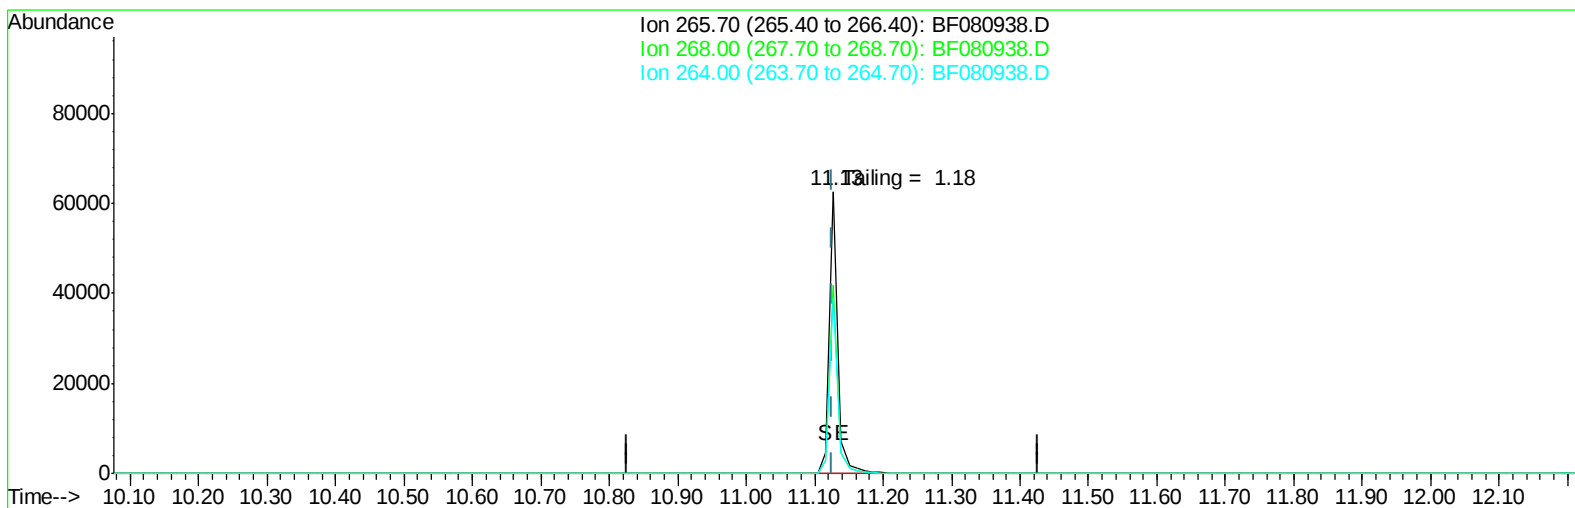

TIC: BF080938.D

(69) Pentachlorophenol (C)

11.128min (+0.001) 0.00ng

response 53643

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	67.04
264.00	62.60	62.20
0.00	0.00	0.00