


Data Path : Z:\HPCHEM1\BNA F\DATA\BF080715\
 Data File : BF080916.D
 Acq On : 7 Aug 2015 9:37
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Aug 08 01:33:05 2015

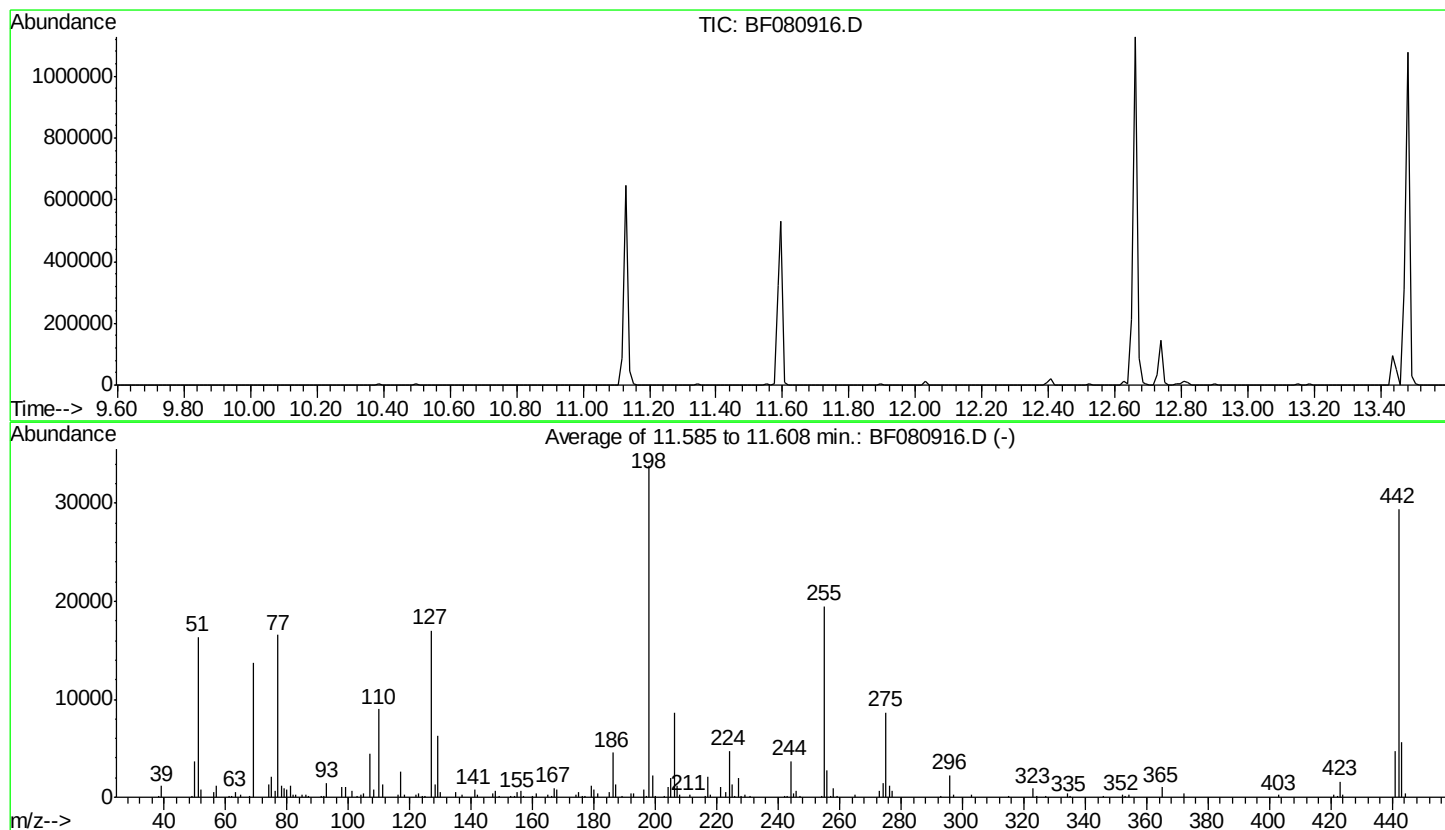

AutoFind: Scans 831, 832, 833; Background Corrected with Scan 827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.4	16385	PASS
68	69	0.00	2	1.1	145	PASS
69	198	0.00	100	40.5	13698	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.4	17050	PASS
197	198	0.00	2	0.5	159	PASS
198	198	100	100	100.0	33850	PASS
199	198	5	9	6.7	2264	PASS
275	198	10	60	25.5	8644	PASS
365	198	1	100	3.0	1027	PASS
441	442	0.01	24	16.1	4752	PASS
442	198	50	100	86.9	29432	PASS
443	442	15	24	19.1	5625	PASS