

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080717\
 Data File : BF097443.D
 Acq On : 7 Aug 2017 21:48
 Operator : SJ/JU
 Sample : I4623-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TEC-WN

Quant Time: Aug 08 04:50:04 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 07 16:02:51 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.41	152	93895	20.00	ng	0.00
21) Naphthalene-d8	7.69	136	369407	20.00	ng	0.00
38) Acenaphthene-d10	9.43	164	160445	20.00	ng	0.00
63) Phenanthrene-d10	10.91	188	208143	20.00	ng	0.00
75) Chrysene-d12	13.53	240	189172	20.00	ng	0.00
86) Perylene-d12	14.87	264	171550	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.00	112	554492	89.02	ng	0.00
7) Phenol-d6	6.08	99	711898	100.12	ng	0.00
23) Nitrobenzene-d5	6.98	82	423580	67.27	ng	-0.01
41) 2,4,6-Tribromophenol	10.22	330	99520	78.51	ng	-0.01
44) 2-Fluorobiphenyl	8.77	172	660453	69.86	ng	0.00
78) Terphenyl-d14	12.49	244	400946	43.21	ng	0.00
Target Compounds						Qvalue
10) Phenol	6.09	94	26595	3.15	ng	# 72
19) n-Nitroso-di-n-propylamine	6.98	70	55478	11.85	ng	# 83
25) Isophorone	6.98	82	423577	34.35	ng	# 67
49) Dimethylphthalate	9.17	163	210049	17.24	ng	99
51) Acenaphthene	9.47	154	72314	7.93	ng	99
54) Dibenzofuran	9.65	168	34151	2.81	ng	98
55) 4-Nitrophenol	9.65	139	12452	6.53	ng	# 28
57) Fluorene	9.98	166	45596	5.00	ng	98
66) 4-Bromophenyl-phenylether	10.22	248	6411	3.09	ng	# 1
70) Phenanthrene	10.93	178	457379	41.01	ng	98
71) Anthracene	10.99	178	125462	10.98	ng	96
72) Carbazole	11.15	167	60817	5.41	ng	97
74) Fluoranthene	12.12	202	569354	52.11	ng	97
77) Pyrene	12.34	202	470601	30.39	ng	99
80) Benzo(a)anthracene	13.52	228	263462	21.52	ng	99
82) Chrysene	13.56	228	237927	19.91	ng	98
85) Indeno(1,2,3-cd)pyrene	16.06	276	74274	7.25	ng	94
87) Benzo(b)fluoranthene	14.53	252	343745	33.33	ng	# 96
88) Benzo(k)fluoranthene	14.53	252	343745	34.98	ng	98
89) Benzo(a)pyrene	14.82	252	191614	20.30	ng	97
91) Benzo(g,h,i)perylene	16.42	276	71738	8.84	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080717\
Data File : BF097443.D
Acq On : 7 Aug 2017 21:48
Operator : SJ/JU
Sample : I4623-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TEC-WN

Quant Time: Aug 08 04:50:04 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 07 16:02:51 2017
Response via : Initial Calibration

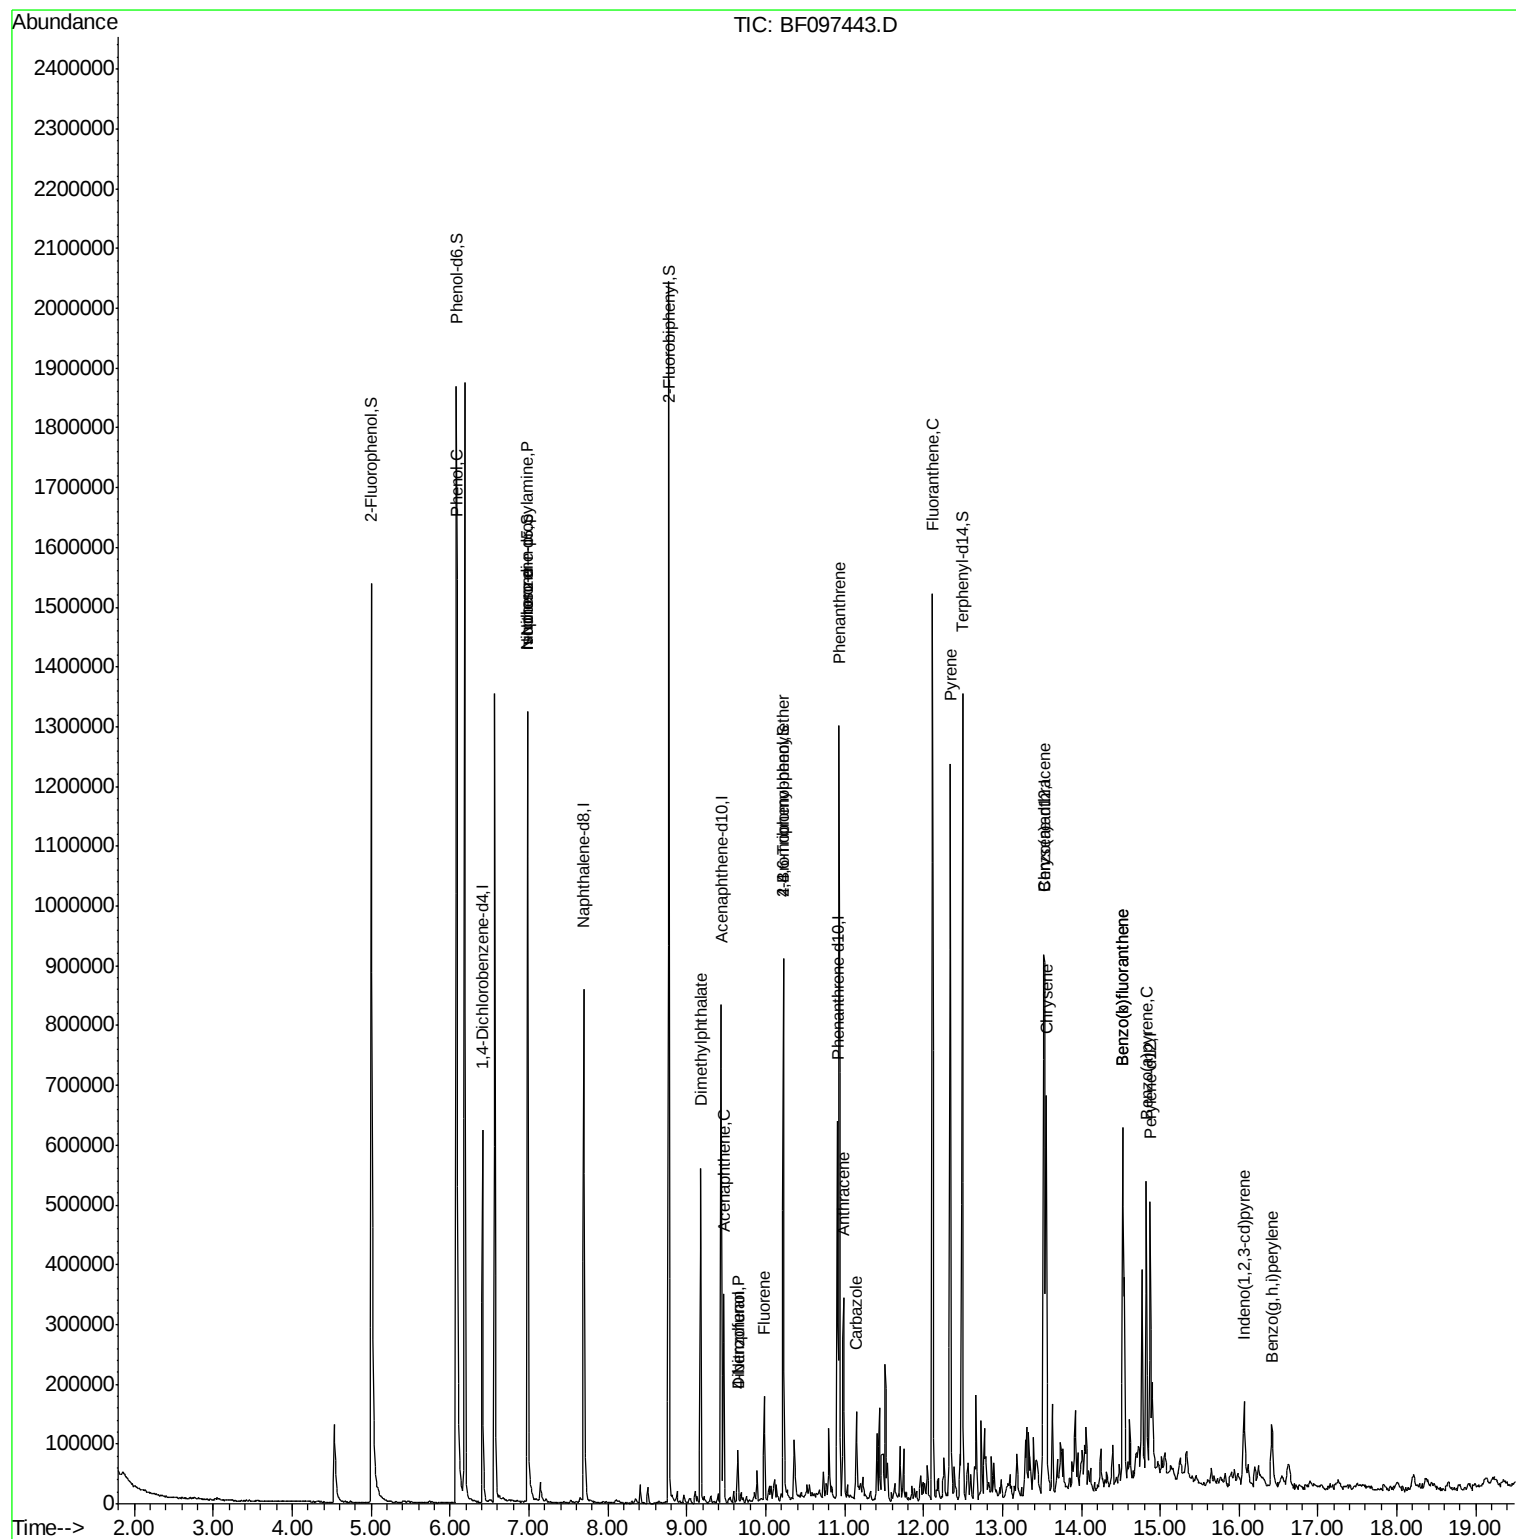

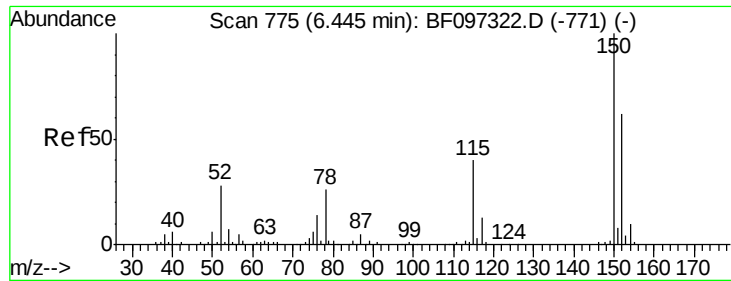


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.41 min Scan# 786
Delta R.T. 0.00 min
Lab File: BF097443.D
Acq: 7 Aug 2017 21:48

Instrument :
BNA_F
ClientSampleId :
TEC-WN

Tot Ion:152 Resp: 93895
Ion Ratio Lower Upper
152 100
150 152.2 126.2 189.2
115 61.6 52.2 78.2

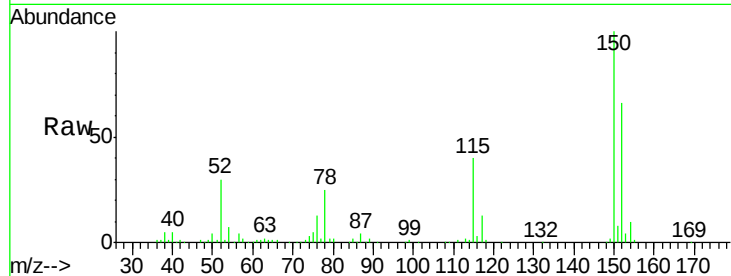


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

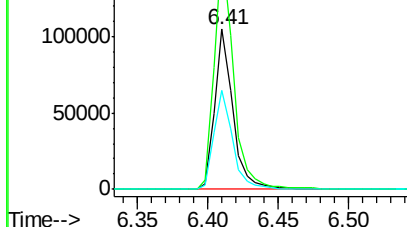



#5


2-Fluorophenol
Concen: 89.02 ng
RT: 5.00 min Scan# 547
Delta R.T. 0.00 min
Lab File: BF097443.D
Acq: 7 Aug 2017 21:48

Tgt Ion:112 Resp: 554492
Ion Ratio Lower Upper
112 100
64 63.6 46.0 69.0
63 32.4 23.4 35.0



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

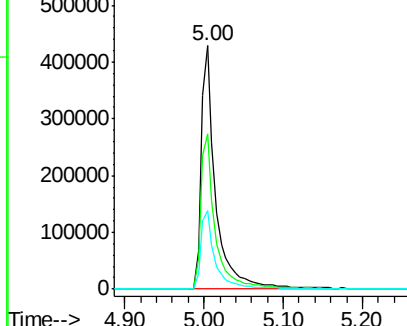

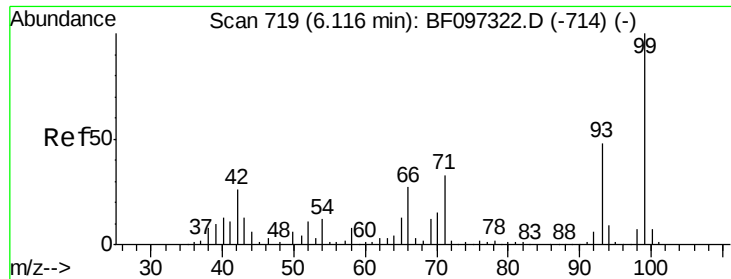

#7

Phenol-d6

Concen: 100.12 ng

RT: 6.08 min Scan# 730

Delta R.T. -0.01 min

Lab File: BF097443.D

Acq: 7 Aug 2017 21:48

Instrument :


BNA_F

ClientSampleId :




TEC-WN

Tot Ion: 99 Resp: 711898

Ion	Ratio	Lower	Upper
99	100		
42	23.9	13.5	20.3#
71	32.8	24.5	36.7

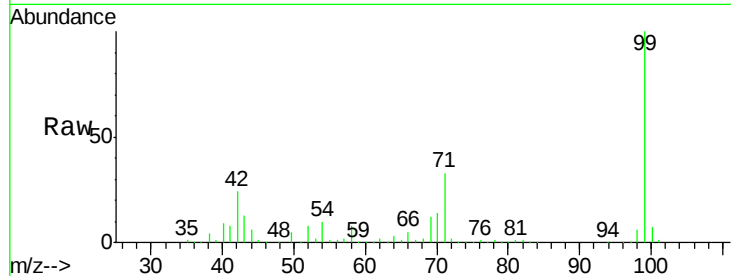

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

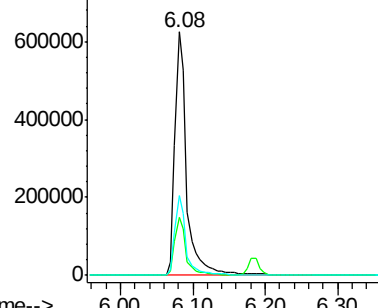

#10

Phenol

Concen: 3.15 ng

RT: 6.09 min Scan# 732


Delta R.T. -0.01 min

Lab File: BF097443.D



Acq: 7 Aug 2017 21:48


Tgt Ion: 94 Resp: 26595

Ion	Ratio	Lower	Upper
94	100		
65	38.6	9.9	49.9
66	66.8	23.1	63.1#



Abundance Ion 94.00 (93.70 to 94.70): BF0
Ion 65.00 (64.70 to 65.70): BF0
Ion 66.00 (65.70 to 66.70): BF0




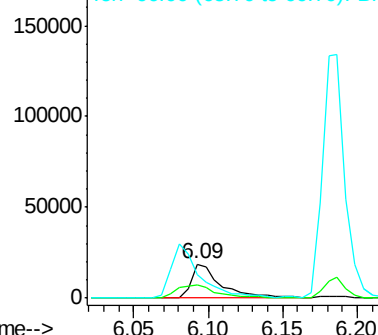




#19
n-Nitroso-di-n-propylamine
Concen: 11.85 ng
RT: 6.98 min Scan# 883
Delta R.T. 0.13 min
Lab File: BF097443.D
Acq: 7 Aug 2017 21:48




Instrument :
BNA_F
ClientSampleId :
TEC-WN


Tot Ion: 70 Resp: 55478
Ion Ratio Lower Upper
70 100
42 65.0 47.2 70.8
101 0.0 7.2 10.8#
130 2.1 15.9 23.9#

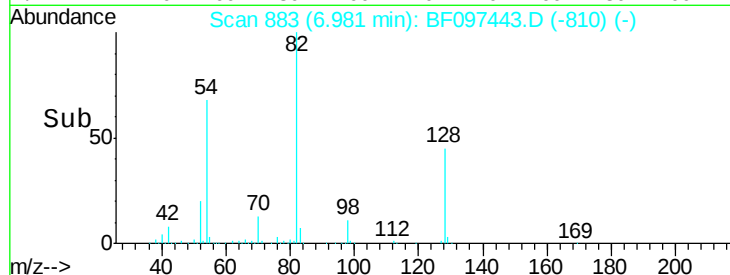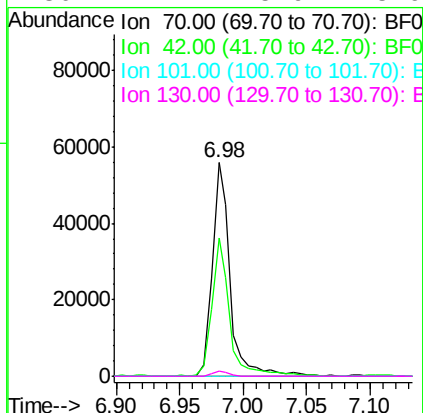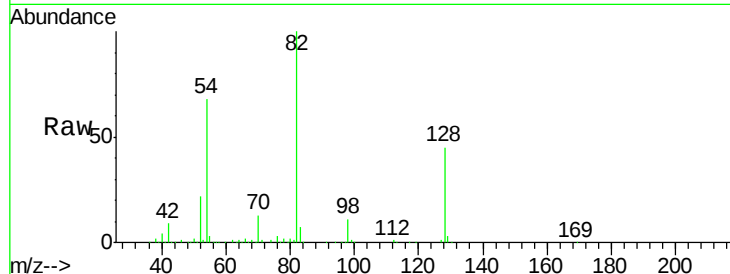

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.69 min Scan# 1004
Delta R.T. -0.01 min
Lab File: BF097443.D
Acq: 7 Aug 2017 21:48

Tgt Ion: 136 Resp: 369407
Ion Ratio Lower Upper
136 100
137 11.1 8.5 12.7
54 10.7 4.9 7.3#
68 5.7 4.1 6.1



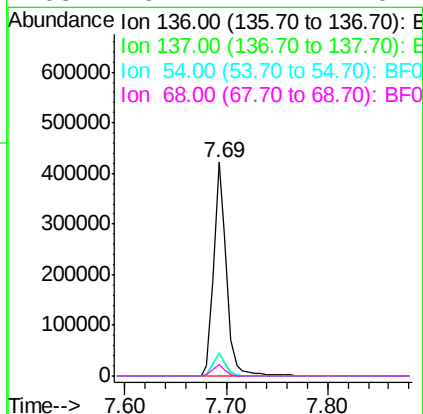
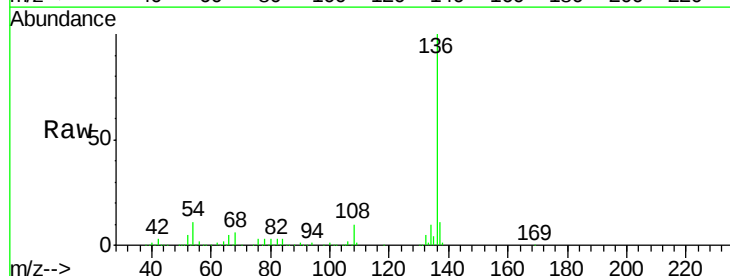


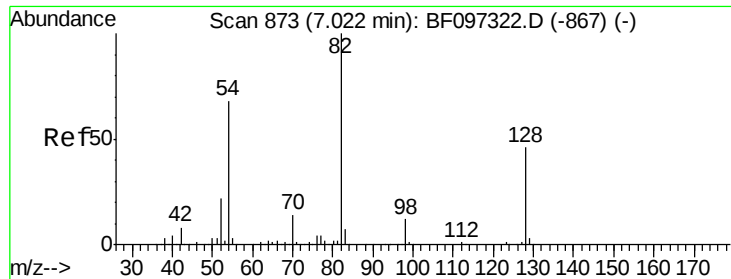

#23
Nitrobenzene-d5
Concen: 67.27 ng
RT: 6.98 min Scan# 883
Delta R.T. -0.01 min
Lab File: BF097443.D
Acq: 7 Aug 2017 21:48




Instrument :
BNA_F
ClientSampleId :
TEC-WN


Tot Ion: 82 Resp: 423580
Ion Ratio Lower Upper
82 100
128 44.9 34.0 51.0
54 68.0 42.2 63.2#

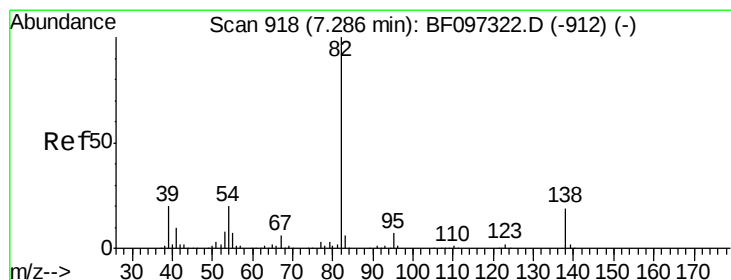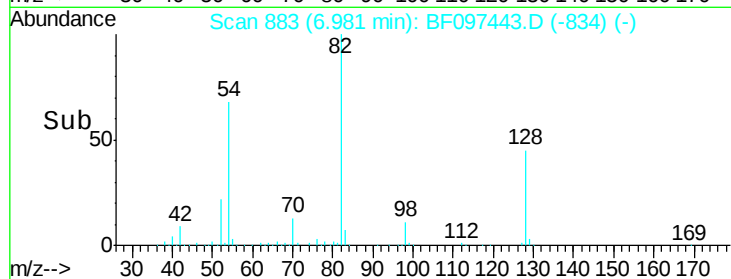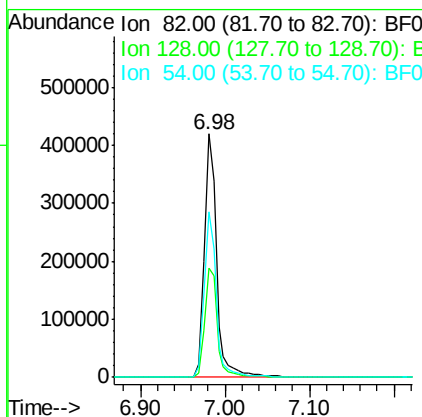

#25
Isophorone
Concen: 34.35 ng
RT: 6.98 min Scan# 883
Delta R.T. -0.27 min
Lab File: BF097443.D
Acq: 7 Aug 2017 21:48

Tgt Ion: 82 Resp: 423577
Ion Ratio Lower Upper
82 100
95 0.0 5.3 7.9#
138 0.0 13.1 19.7#


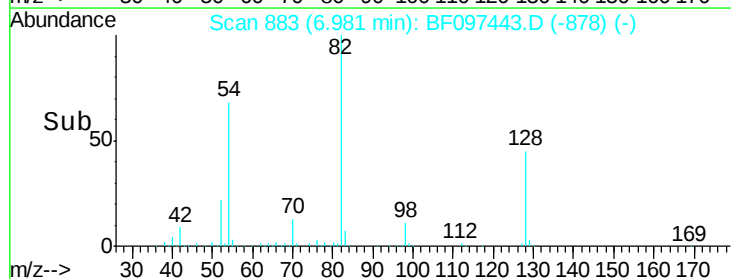
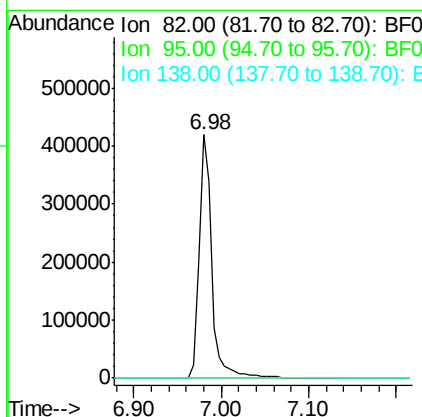
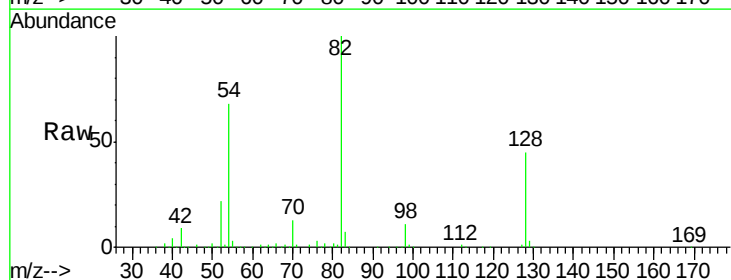


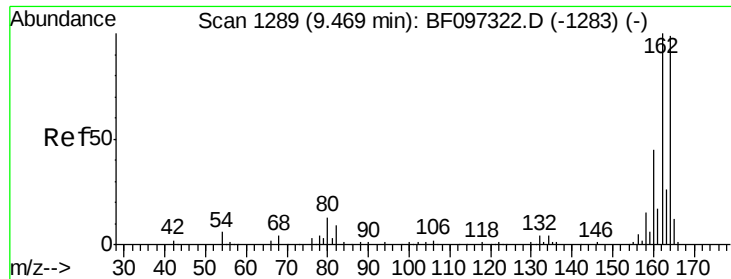

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.43 min Scan# 1300
 Delta R.T. -0.01 min
 Lab File: BF097443.D
 Acq: 7 Aug 2017 21:48




Instrument :
 BNA_F
 ClientSampleId :
 TEC-WN


Tot Ion:164 Resp: 160445
 Ion Ratio Lower Upper
 164 100
 162 102.1 82.6 123.8
 160 44.8 36.2 54.2

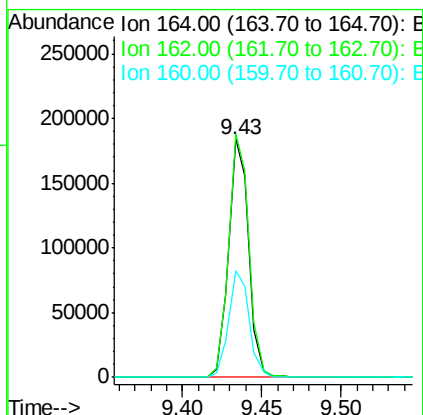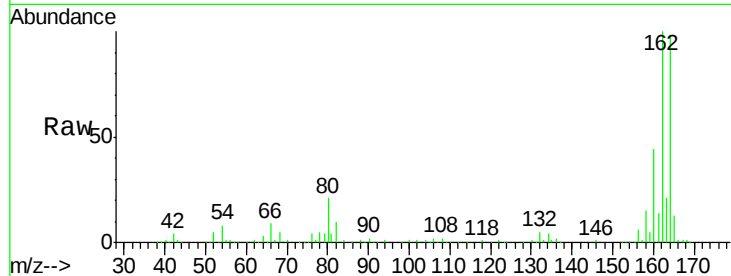

#41
 2,4,6-Tribromophenol
 Concen: 78.51 ng
 RT: 10.22 min Scan# 1434
 Delta R.T. -0.01 min
 Lab File: BF097443.D
 Acq: 7 Aug 2017 21:48

Tgt Ion:330 Resp: 99520
 Ion Ratio Lower Upper
 330 100
 332 93.7 76.6 115.0
 141 38.1 31.4 47.2

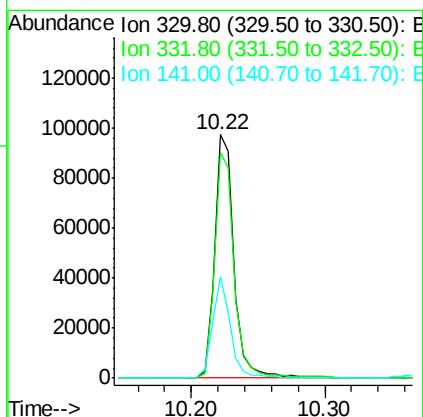


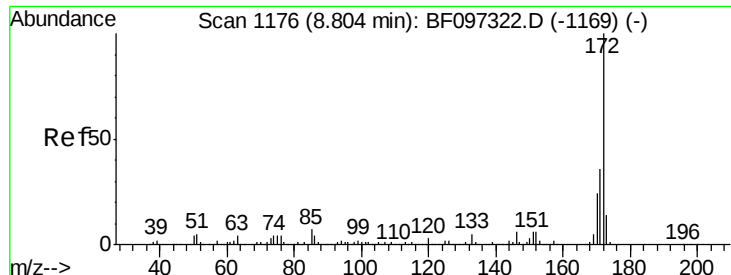




#44
2-Fluorobiphenyl
Concen: 69.86 ng
RT: 8.77 min Scan# 1188
Delta R.T. 0.00 min
Lab File: BF097443.D
Acq: 7 Aug 2017 21:48

Instrument :
BNA_F
ClientSampleId :
TEC-WN

Tot Ion:172 Resp: 660453
Ion Ratio Lower Upper
172 100
171 35.3 29.6 44.4
170 23.4 19.8 29.8

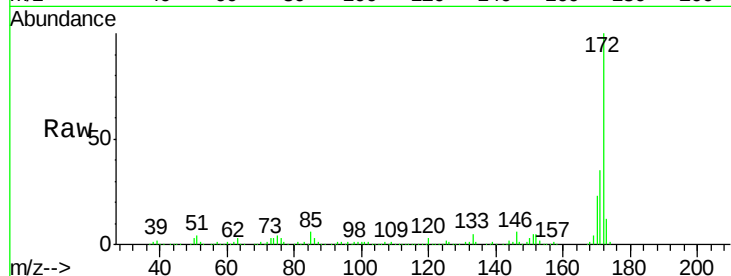


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E


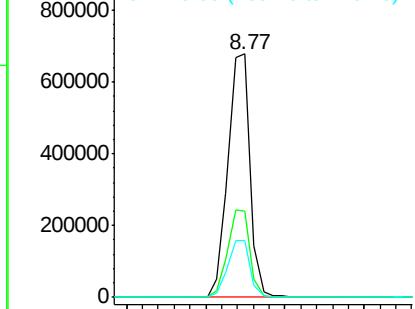



#49
Dimethylphthalate
Concen: 17.24 ng
RT: 9.17 min Scan# 1256
Delta R.T. -0.01 min
Lab File: BF097443.D
Acq: 7 Aug 2017 21:48

Tgt Ion:163 Resp: 210049
Ion Ratio Lower Upper
163 100
194 3.0 2.6 4.0
164 10.2 8.4 12.6



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

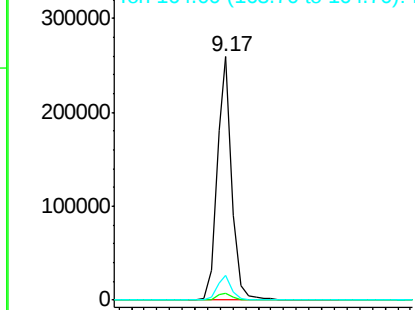

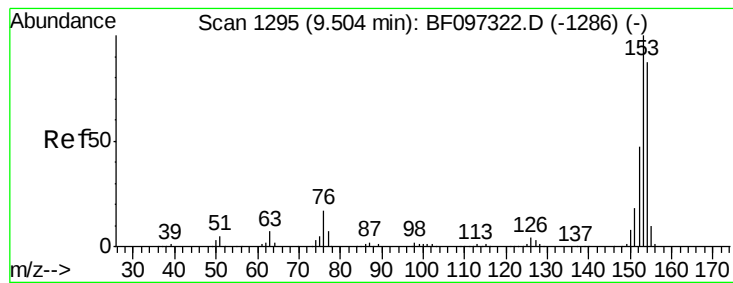

#51

Acenaphthene

Concen: 7.93 ng

RT: 9.47 min Scan# 1306

Delta R.T. -0.01 min

Lab File: BF097443.D

Acq: 7 Aug 2017 21:48

Instrument :

BNA_F

ClientSampleId :

TEC-WN


Tot Ion:154 Resp: 72314

Ion Ratio Lower Upper

154 100

153 114.3 90.5 135.7




152 53.8 43.6 65.4

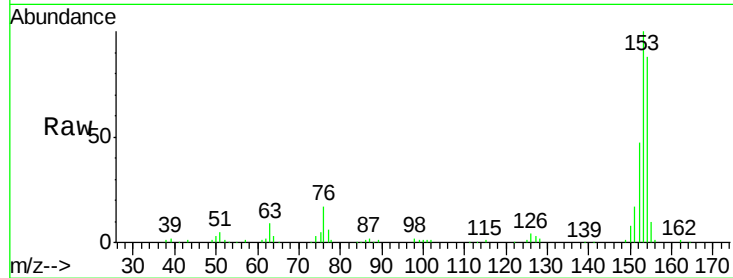

Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

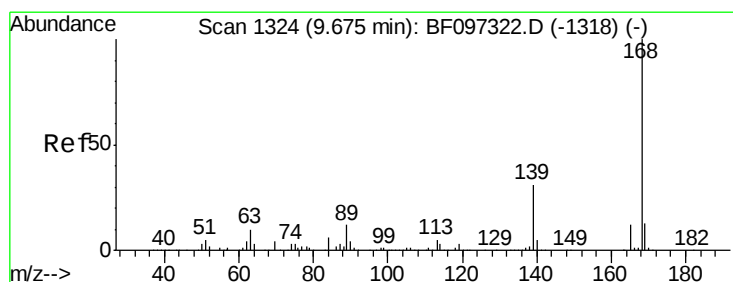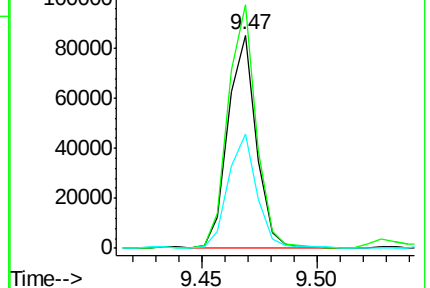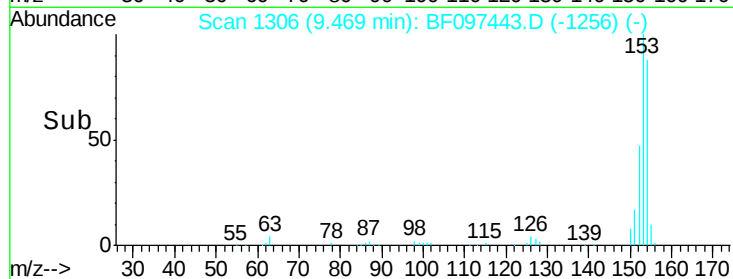

#54

Dibenzofuran

Concen: 2.81 ng

RT: 9.65 min Scan# 1336

Delta R.T. 0.00 min

Lab File: BF097443.D

Acq: 7 Aug 2017 21:48


Tgt Ion:168 Resp: 34151

Ion Ratio Lower Upper

168 100

139 36.7 30.6 45.8



169 13.9 10.8 16.2

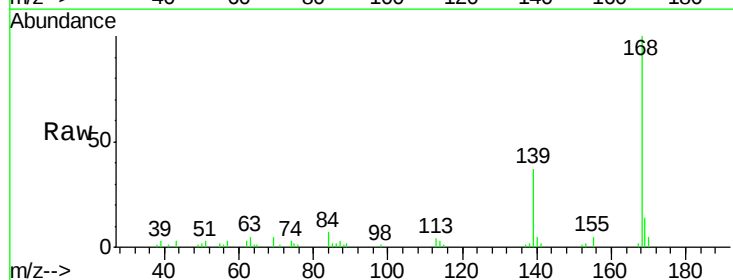


Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 169.00 (168.70 to 169.70): E

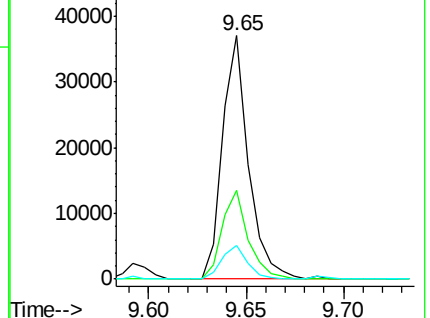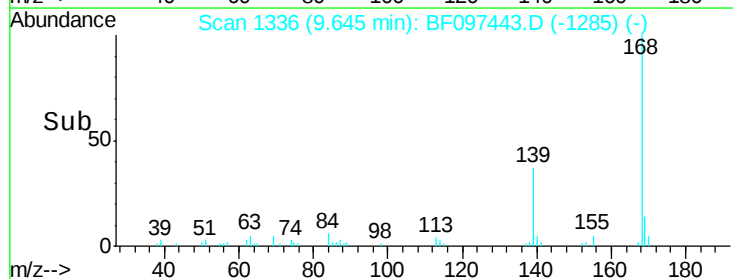







#55
4-Nitrophenol
Concen: 6.53 ng
RT: 9.65 min Scan# 1336
Delta R.T. 0.02 min
Lab File: BF097443.D
Acq: 7 Aug 2017 21:48

Instrument :
BNA_F
ClientSampleId :
TEC-WN

Tot Ion	Ratio	Lower	Upper
139	100		
109	0.0	34.1	74.1#
65	3.1	31.4	71.4#

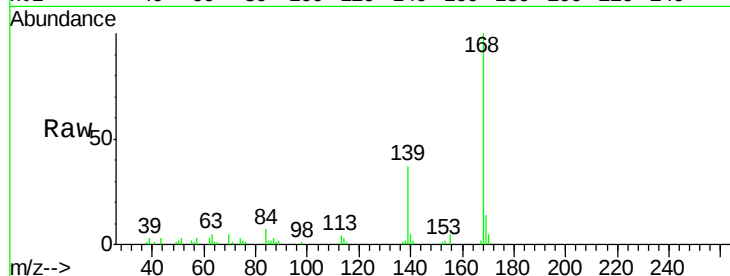


Abundance Ion 139.00 (138.70 to 139.70): E
Ion 109.00 (108.70 to 109.70): E
Ion 65.00 (64.70 to 65.70): E


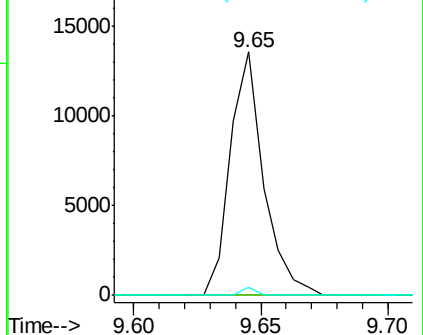



#57
Fluorene
Concen: 5.00 ng
RT: 9.98 min Scan# 1393
Delta R.T. -0.01 min
Lab File: BF097443.D
Acq: 7 Aug 2017 21:48

Tgt Ion	Ratio	Lower	Upper
166	100		
165	100.3	78.8	118.2
167	15.0	10.6	16.0



Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E




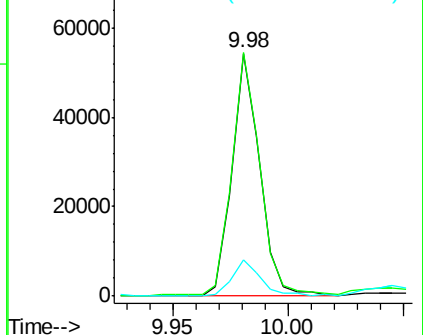


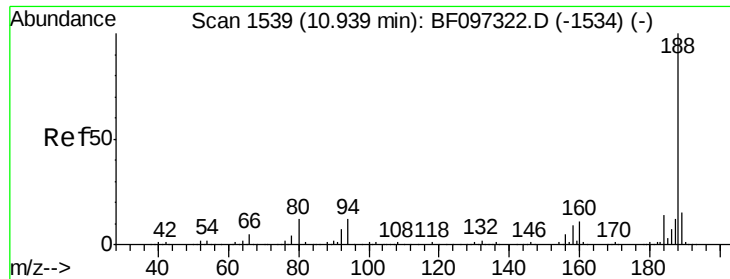

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 10.91 min Scan# 1551
Delta R.T. -0.01 min
Lab File: BF097443.D
Acq: 7 Aug 2017 21:48




Instrument :
BNA_F
ClientSampleId :
TEC-WN


Tot Ion:188 Resp: 208143
Ion Ratio Lower Upper
188 100
94 10.7 9.4 14.2
80 10.3 10.2 15.2

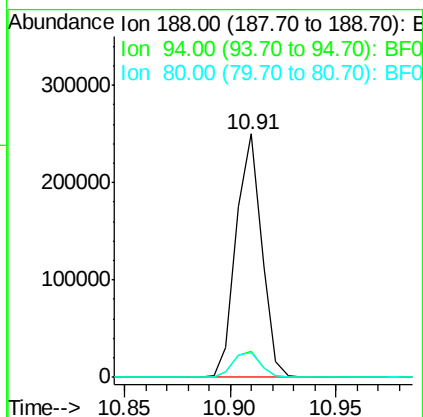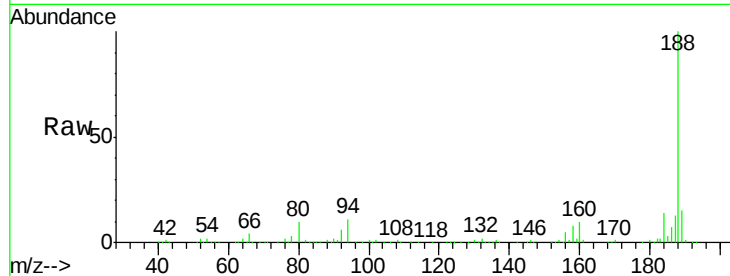

#66
4-Bromophenyl-phenylether
Concen: 3.09 ng
RT: 10.22 min Scan# 1434
Delta R.T. -0.25 min
Lab File: BF097443.D
Acq: 7 Aug 2017 21:48

Tgt Ion:248 Resp: 6411
Ion Ratio Lower Upper
248 100
250 201.1 76.8 115.2#
141 619.7 68.6 103.0#

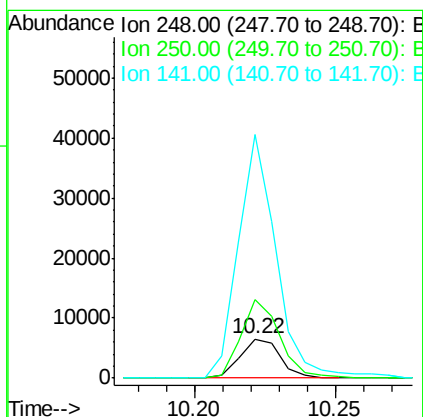



#70

Phenanthrene

Concen: 41.01 ng

RT: 10.93 min Scan# 1555

Delta R.T. -0.01 min

Lab File: BF097443.D

Acq: 7 Aug 2017 21:48

Instrument :

BNA_F

ClientSampleId :

TEC-WN


Tot Ion:178 Resp: 457379

Ion Ratio Lower Upper

178 100

176 19.2 16.2 24.4




179 15.0 12.6 19.0

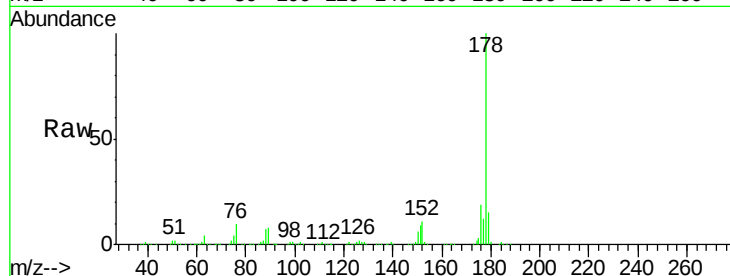

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

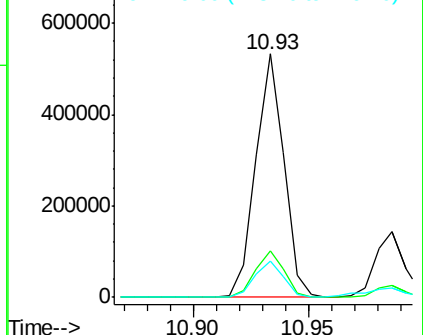

#71

Anthracene

Concen: 10.98 ng

RT: 10.99 min Scan# 1564

Delta R.T. -0.01 min

Lab File: BF097443.D

Acq: 7 Aug 2017 21:48


Tgt Ion:178 Resp: 125462

Ion Ratio Lower Upper

178 100

176 17.7 15.8 23.8



179 14.9 12.7 19.1




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

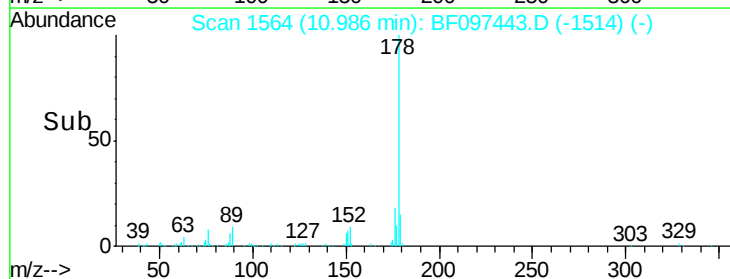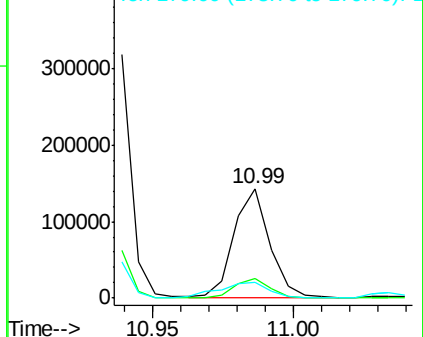

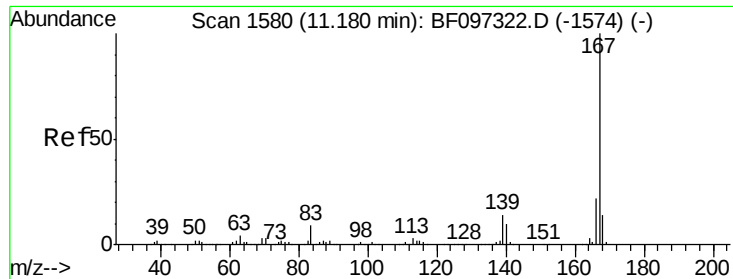

#72

Carbazole

Concen: 5.41 ng

RT: 11.15 min Scan# 1592

Delta R.T. 0.00 min

Lab File: BF097443.D

Acq: 7 Aug 2017 21:48

Instrument :

BNA_F

ClientSampleId :

TEC-WN


Tot Ion:167 Resp: 60817

Ion Ratio Lower Upper

167 100

166 21.4 18.1 27.1




139 12.7 11.7 17.5

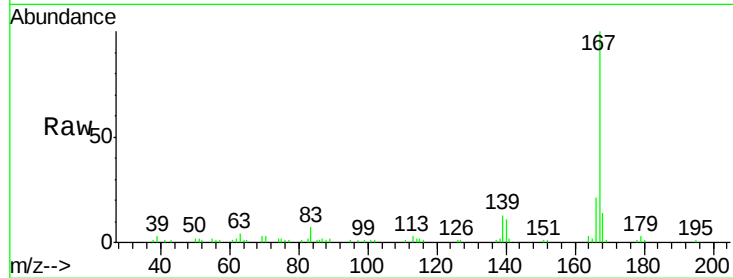

Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

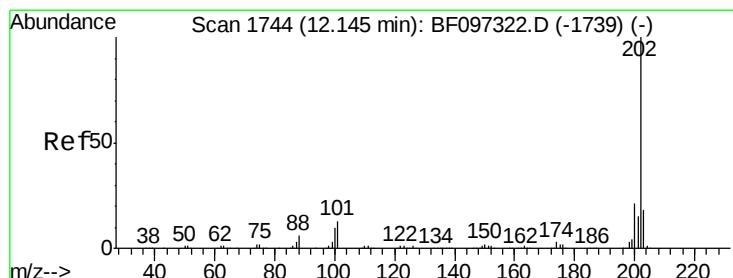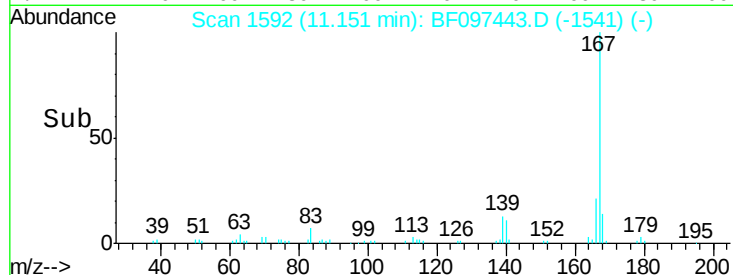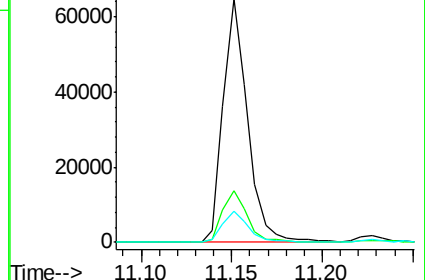

#74

Fluoranthene

Concen: 52.11 ng

RT: 12.12 min Scan# 1756

Delta R.T. 0.00 min

Lab File: BF097443.D

Acq: 7 Aug 2017 21:48


Tgt Ion:202 Resp: 569354

Ion Ratio Lower Upper

202 100

101 14.0 0.0 33.2



203 16.4 0.0 38.1

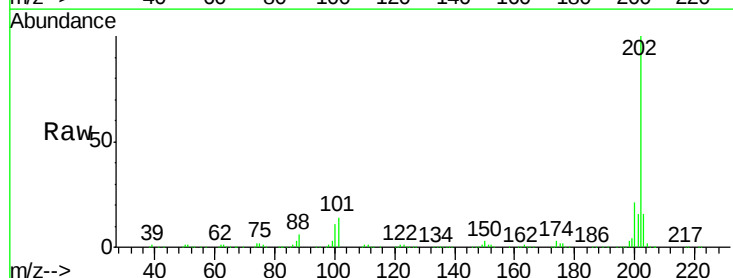


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

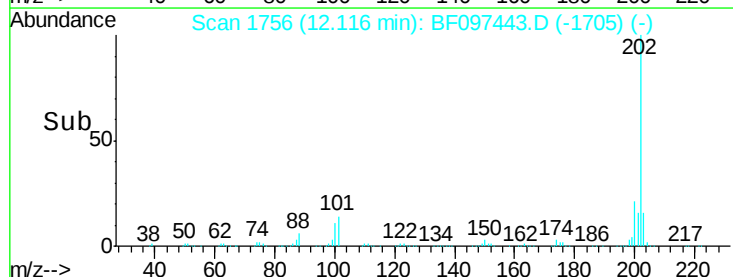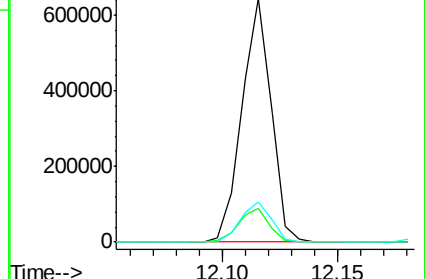



#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.53 min Scan# 1997

Delta R.T. -0.01 min

Lab File: BF097443.D

Acq: 7 Aug 2017 21:48

Instrument :

BNA_F

ClientSampleId :

TEC-WN


Tot Ion:240 Resp: 189172

Ion Ratio Lower Upper

240 100

120 16.3 5.8 8.8#




236 24.1 20.5 30.7

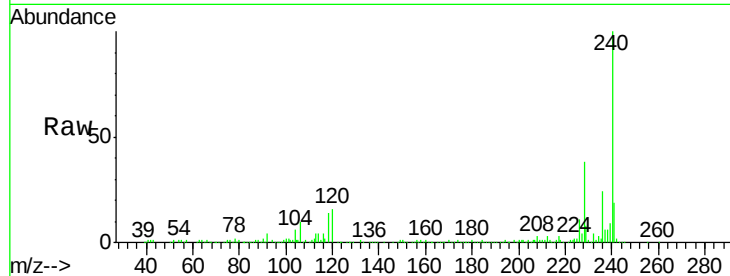

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

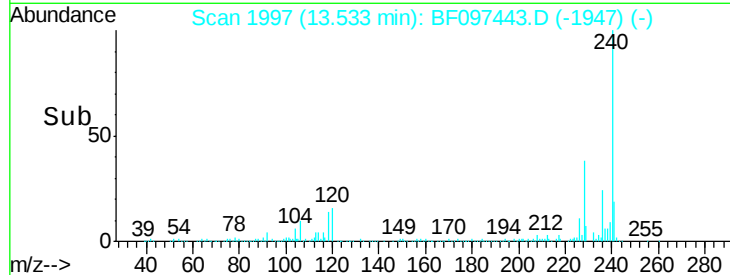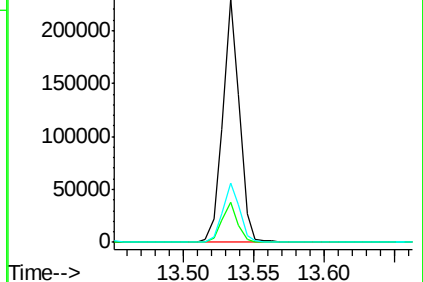

#77

Pyrene

Concen: 30.39 ng

RT: 12.34 min Scan# 1794

Delta R.T. 0.00 min

Lab File: BF097443.D

Acq: 7 Aug 2017 21:48


Tgt Ion:202 Resp: 470601

Ion Ratio Lower Upper

202 100

200 21.3 17.6 26.4



203 17.8 14.4 21.6




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E



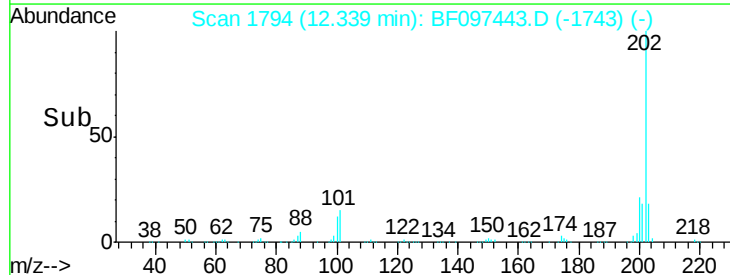
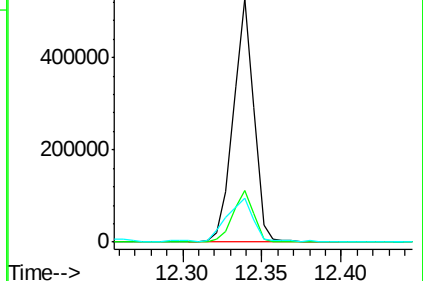




#78
 Terphenyl-d14
 Concen: 43.21 ng
 RT: 12.49 min Scan# 1820
 Delta R.T. -0.01 min
 Lab File: BF097443.D
 Acq: 7 Aug 2017 21:48




Instrument :
 BNA_F
 ClientSampled :
 TEC-WN


Tot Ion:244 Resp: 400946
 Ion Ratio Lower Upper
 244 100
 212 6.9 6.0 9.0
 122 14.4 10.3 15.5

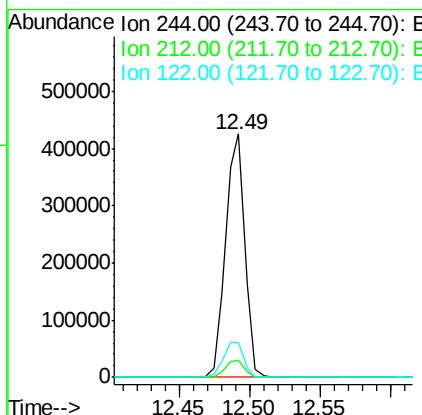

#80
 Benzo(a)anthracene
 Concen: 21.52 ng
 RT: 13.52 min Scan# 1995
 Delta R.T. -0.01 min
 Lab File: BF097443.D
 Acq: 7 Aug 2017 21:48

Tgt Ion:228 Resp: 263462
 Ion Ratio Lower Upper
 228 100
 226 28.3 22.6 33.8
 229 21.7 16.3 24.5

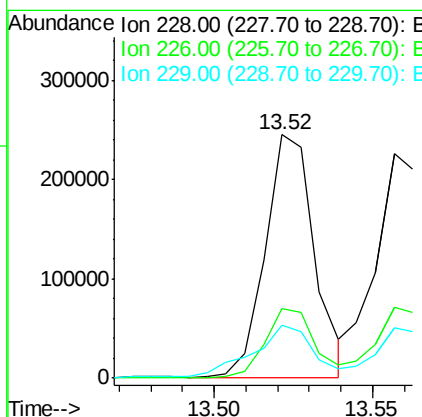



#82

Chrysene

Concen: 19.91 ng

RT: 13.56 min Scan# 2001

Delta R.T. -0.01 min

Lab File: BF097443.D

Acq: 7 Aug 2017 21:48

Instrument :


BNA_F

ClientSampleId :

TEC-WN

Tot Ion:228 Resp: 237927




Ion	Ratio	Lower	Upper
228	100		
226	31.3	24.9	37.3
229	22.2	15.8	23.6



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

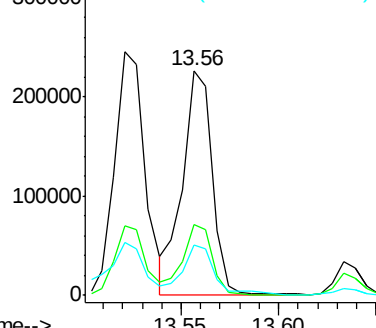

#85

Indeno(1,2,3-cd)pyrene

Concen: 7.25 ng

RT: 16.06 min Scan# 2427


Delta R.T. 0.00 min

Lab File: BF097443.D

Acq: 7 Aug 2017 21:48

Tgt Ion:276 Resp: 74274



Ion	Ratio	Lower	Upper
276	100		
138	30.0	27.8	41.6
277	23.9	20.2	30.4




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

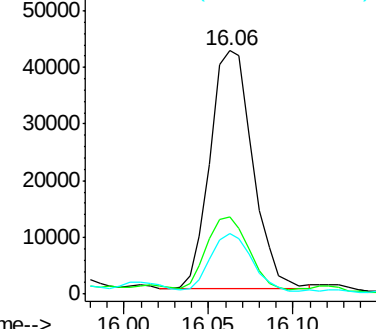




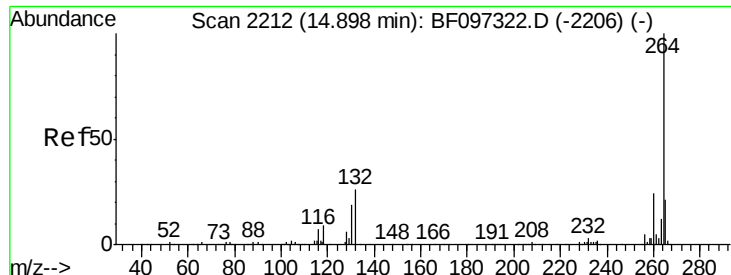


#86
Pervlene-d12
Concen: 20.00 ng
RT: 14.87 min Scan# 2225
Delta R.T. 0.01 min
Lab File: BF097443.D
Acq: 7 Aug 2017 21:48

Instrument :
BNA_F
ClientSampleId :
TEC-WN

Tot Ion:264 Resp: 171550




Ion	Ratio	Lower	Upper
264	100		
260	23.9	19.5	29.3
265	21.3	17.2	25.8

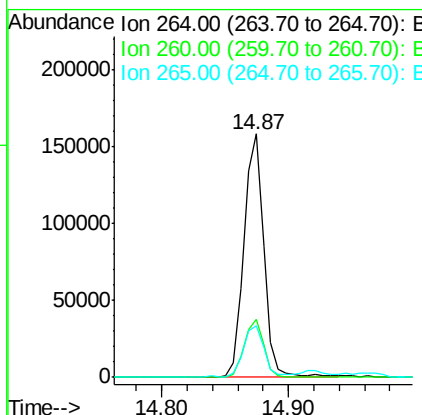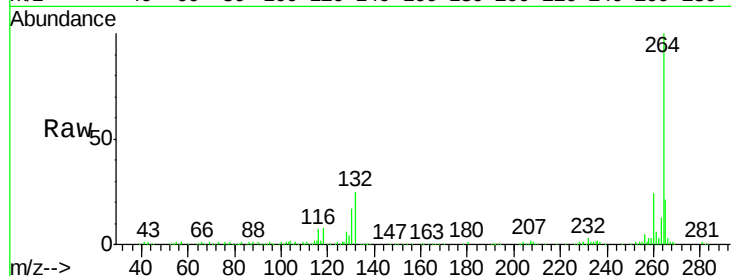


#87
Benzo(b)fluoranthene
Concen: 33.33 ng
RT: 14.53 min Scan# 2166
Delta R.T. 0.00 min
Lab File: BF097443.D
Acq: 7 Aug 2017 21:48

Tgt Ion:252 Resp: 343745

Ion	Ratio	Lower	Upper
252	100		
253	23.5	18.1	27.1
125	15.0	9.8	14.8#



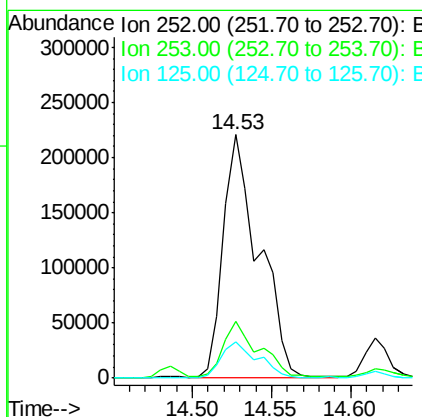





#88
Benzo(k)fluoranthene
Concen: 34.98 ng
RT: 14.53 min Scan# 2166
Delta R.T. -0.02 min
Lab File: BF097443.D
Acq: 7 Aug 2017 21:48




Instrument :
BNA_F
ClientSampleId :
TEC-WN


Tot Ion:252 Resp: 343745
Ion Ratio Lower Upper
252 100
253 23.5 18.4 27.6
125 15.0 13.1 19.7

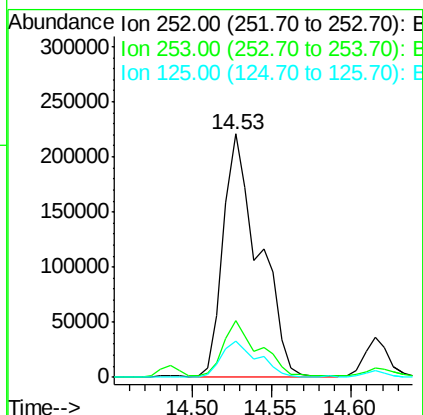

#89
Benzo(a)pyrene
Concen: 20.30 ng
RT: 14.82 min Scan# 2216
Delta R.T. 0.00 min
Lab File: BF097443.D
Acq: 7 Aug 2017 21:48

Tgt Ion:252 Resp: 191614
Ion Ratio Lower Upper
252 100
253 22.7 17.5 26.3
125 15.8 11.0 16.4

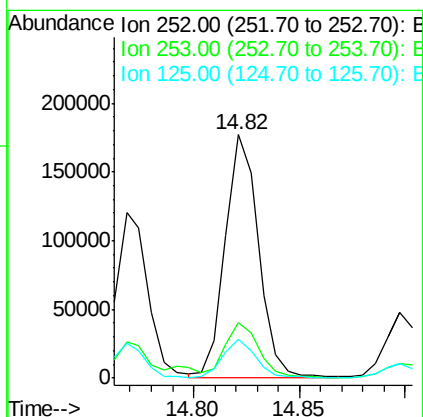

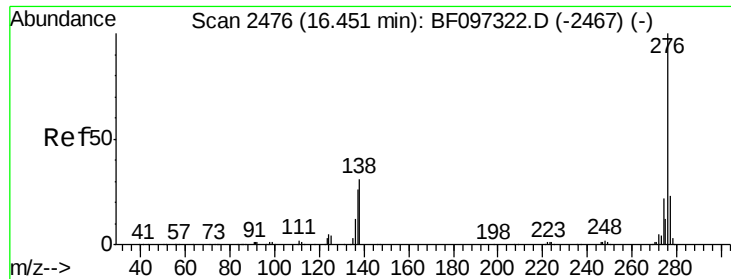

#91

Benzo(a,h,i)perylene

Concen: 8.84 ng

RT: 16.42 min Scan# 2487

Delta R.T. 0.01 min

Lab File: BF097443.D

Acq: 7 Aug 2017 21:48

Instrument :

BNA_F

ClientSampleId :

TEC-WN

Tot Ion:276 Resp: 71738

Ion Ratio Lower Upper

276 100

277 24.9 18.6 28.0

138 31.0 25.4 38.0

