
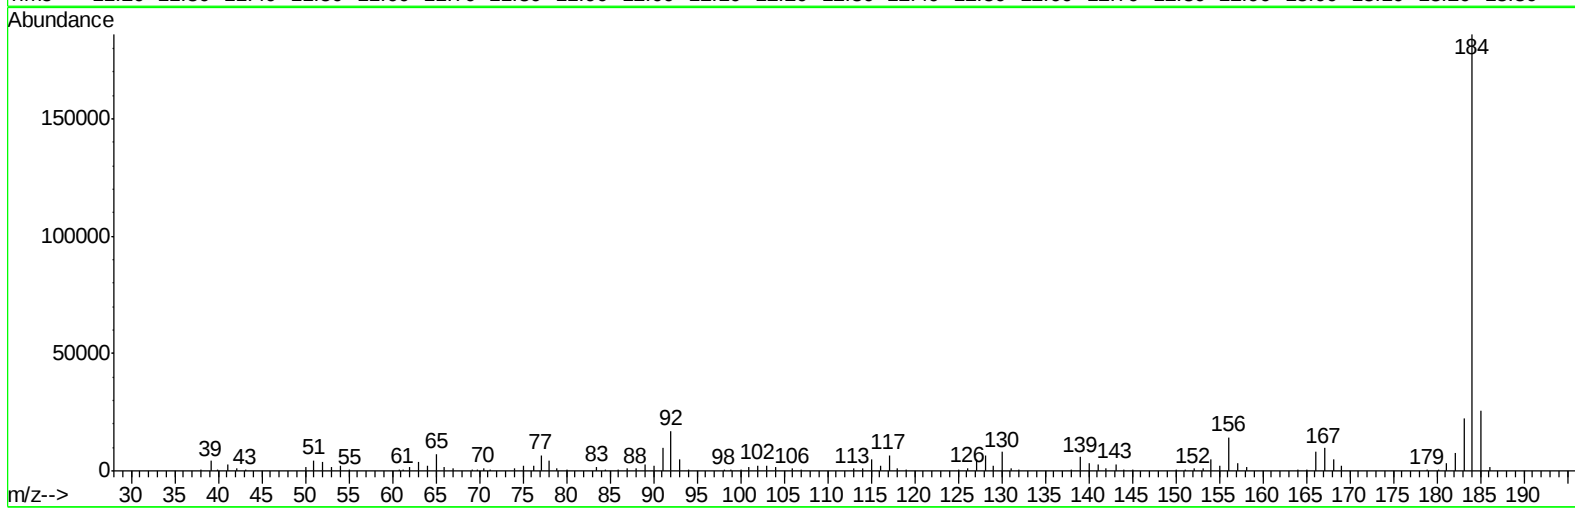


Data Path : Z:\HPCHEM1\BNA F\DATA\BF080717\
 Data File : BF097450.D
 Acq On : 8 Aug 2017 1:49
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 08 08:45:56 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 07 16:02:51 2017
 Response via : Initial Calibration

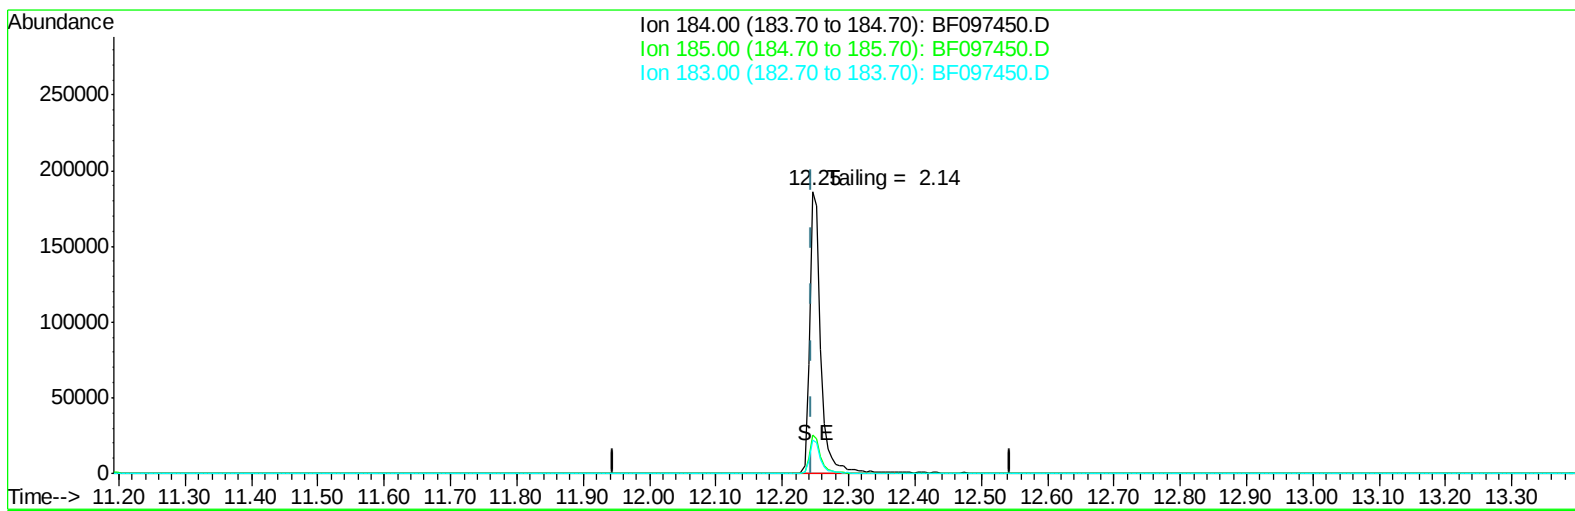

TIC: BF097450.D

(76) Benzidine



12.245min (+0.000) 0.00ng

response 218675

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.85#
183.00	12.20	11.98
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080717\
Data File : BF097450.D
Acq On : 8 Aug 2017 1:49
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 08 08:45:56 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 07 16:02:51 2017
Response via : Initial Calibration

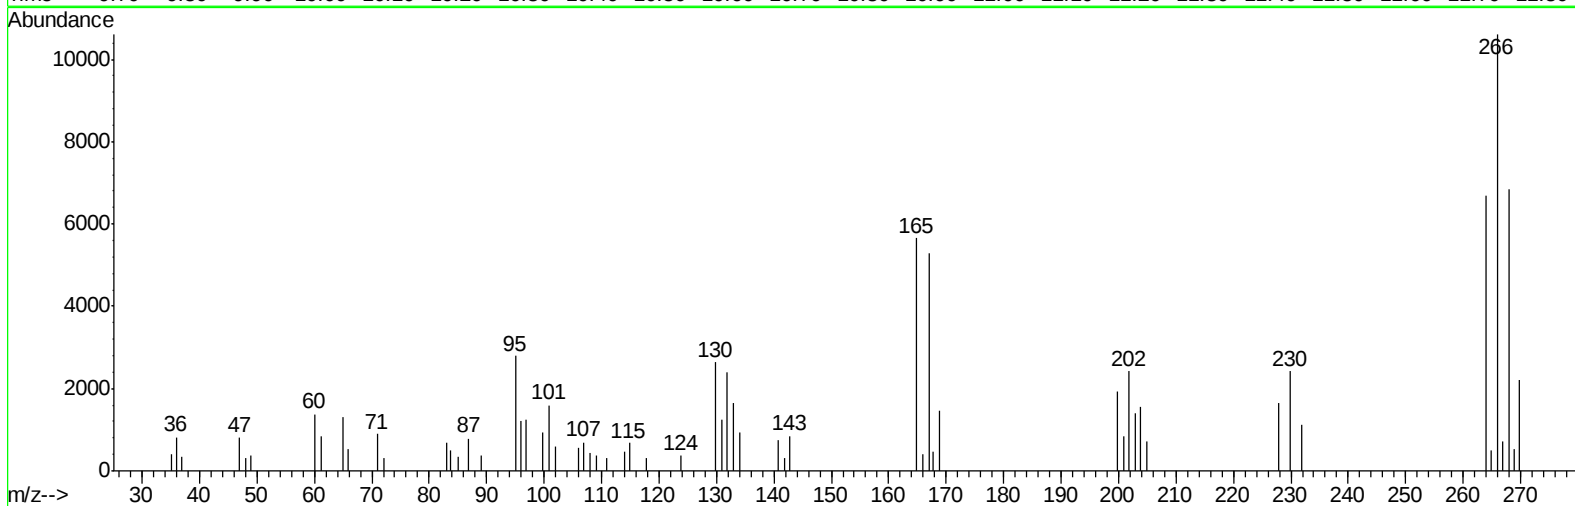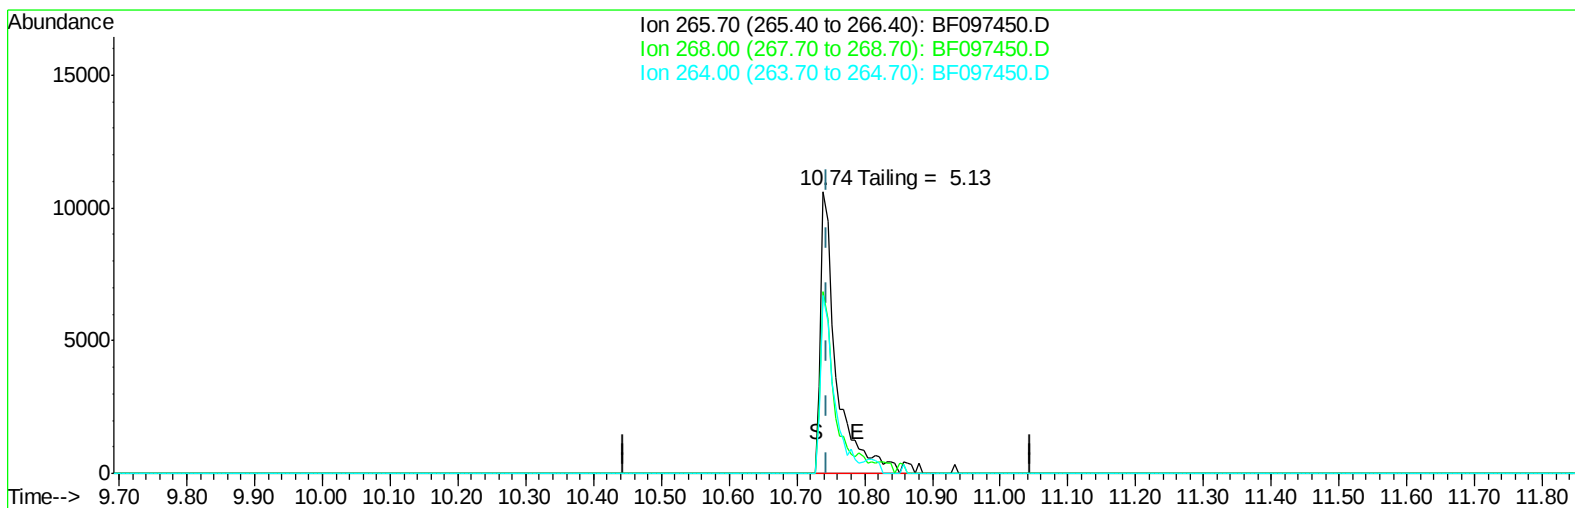

TIC: BF097450.D

(69) Pentachlorophenol (C)

10.739min (-0.006) 0.00ng

response 16851

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.47
264.00	64.60	63.07
0.00	0.00	0.00