

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080717\
 Data File : BF097436.D
 Acq On : 7 Aug 2017 18:30
 Operator : SJ/JU
 Sample : I4623-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TEC-BC

Quant Time: Aug 08 05:29:00 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 07 16:02:51 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.41	152	96720	20.00	ng	0.00
21) Naphthalene-d8	7.69	136	389126	20.00	ng	0.00
38) Acenaphthene-d10	9.43	164	157127	20.00	ng	0.00
63) Phenanthrene-d10	10.91	188	225714	20.00	ng	0.00
75) Chrysene-d12	13.53	240	203947	20.00	ng	0.00
86) Perylene-d12	14.87	264	151739	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.00	112	611875	95.37	ng	0.00
7) Phenol-d6	6.09	99	742951	101.43	ng	0.00
23) Nitrobenzene-d5	6.98	82	470658	70.96	ng	-0.01
41) 2,4,6-Tribromophenol	10.23	330	112663	90.75	ng	0.00
44) 2-Fluorobiphenyl	8.77	172	746596	80.64	ng	0.00
78) Terphenyl-d14	12.49	244	436166	43.60	ng	0.00
Target Compounds						
10) Phenol	6.10	94	29563	3.403	ng	84
49) Dimethylphthalate	9.17	163	114791	9.620	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080717\
Data File : BF097436.D
Acq On : 7 Aug 2017 18:30
Operator : SJ/JU
Sample : I4623-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TEC-BC

Quant Time: Aug 08 05:29:00 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 07 16:02:51 2017
Response via : Initial Calibration

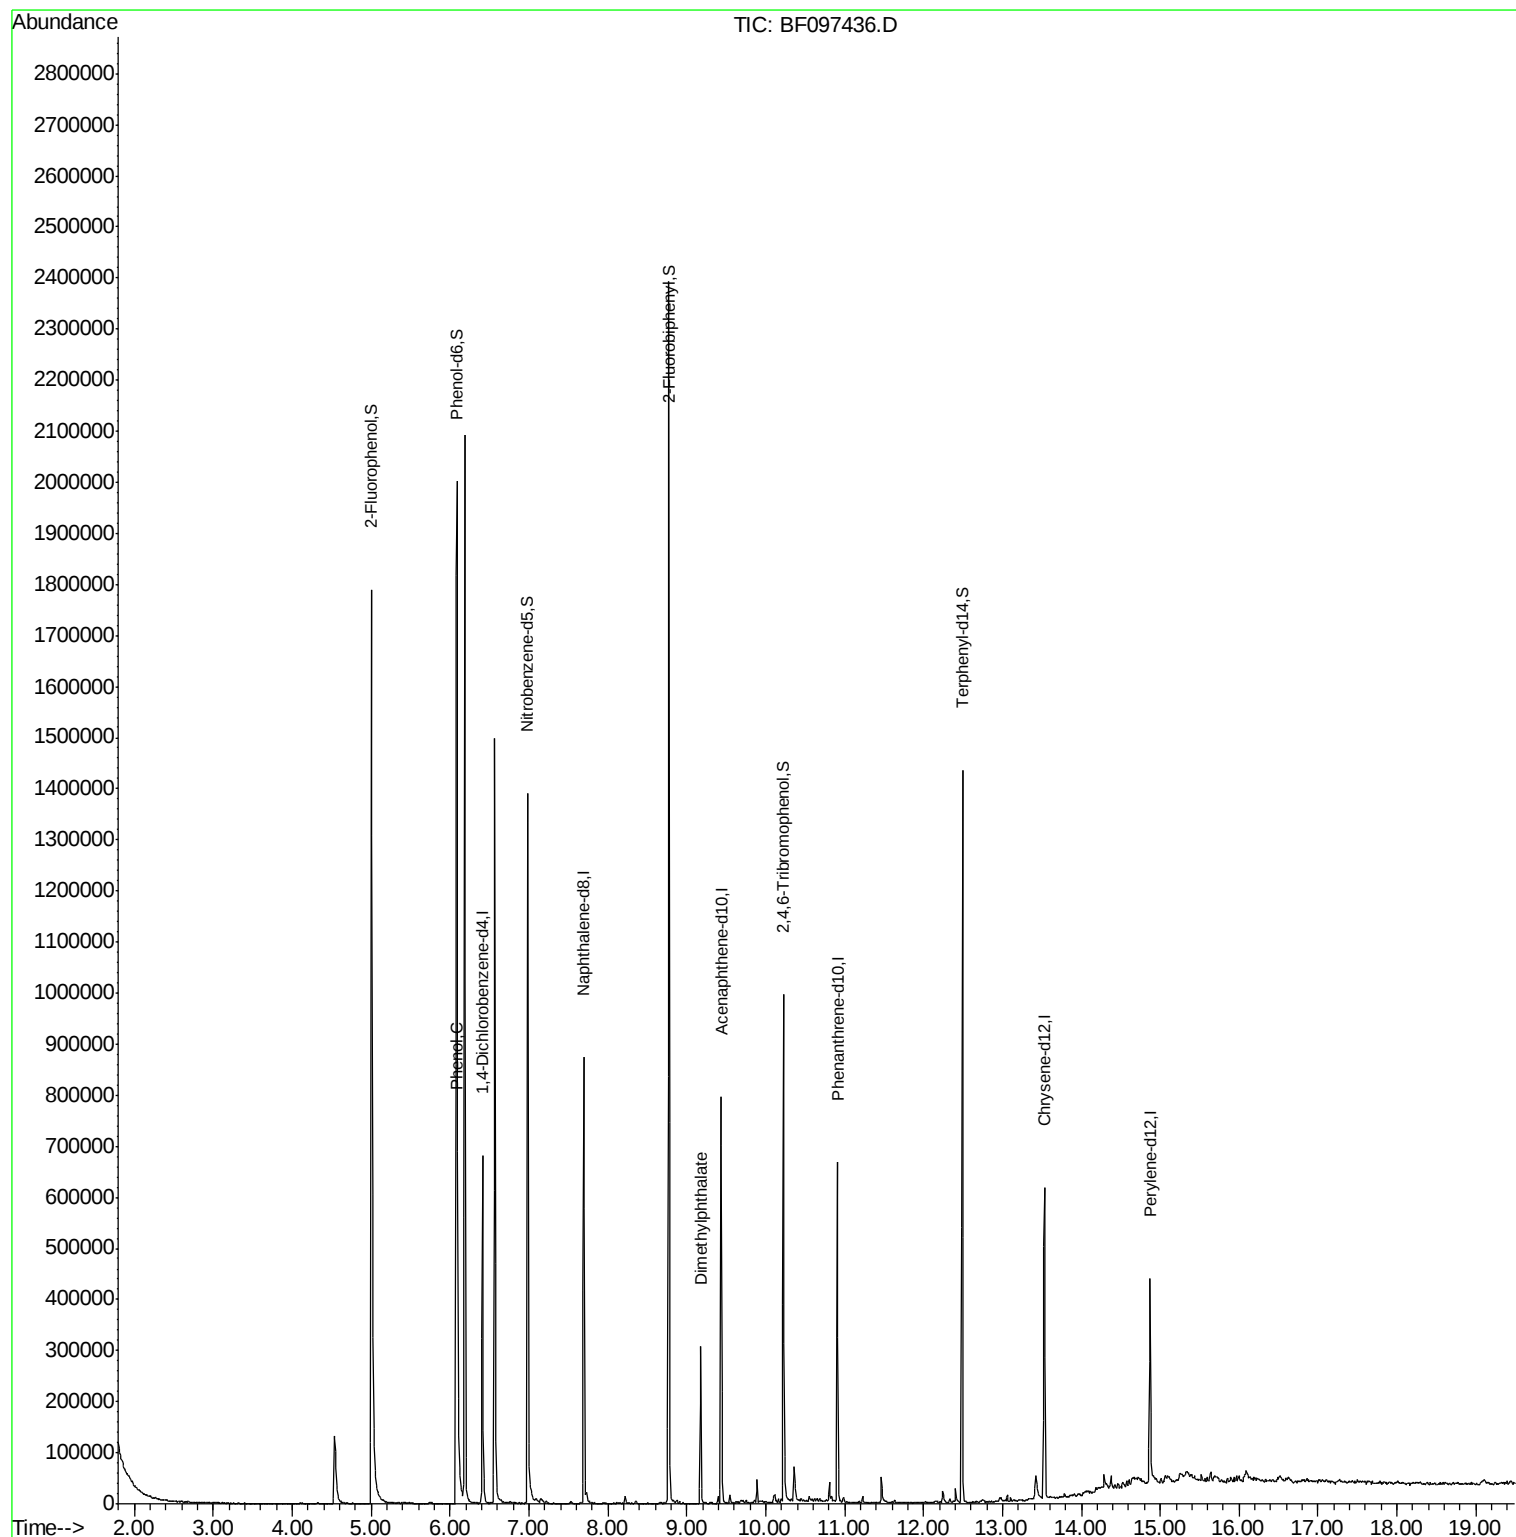

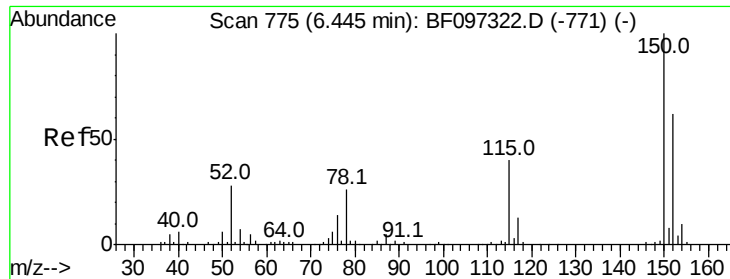


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.41 min Scan# 786
 Delta R.T. 0.00 min
 Lab File: BF097436.D
 Acq: 7 Aug 2017 18:30

Instrument :
 BNA_F
 ClientSampleId :
 TEC-BC

Tot Ion:152 Resp: 96720
 Ion Ratio Lower Upper
 152 100
 150 160.5 126.2 189.2
 115 64.8 52.2 78.2

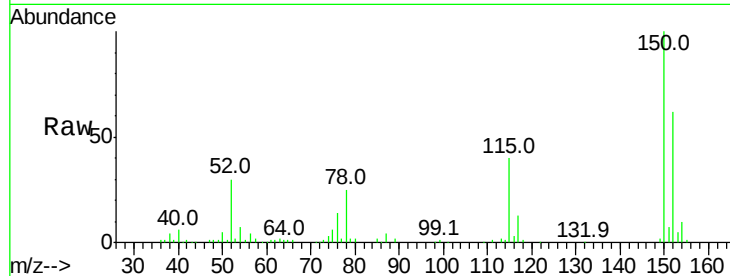


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

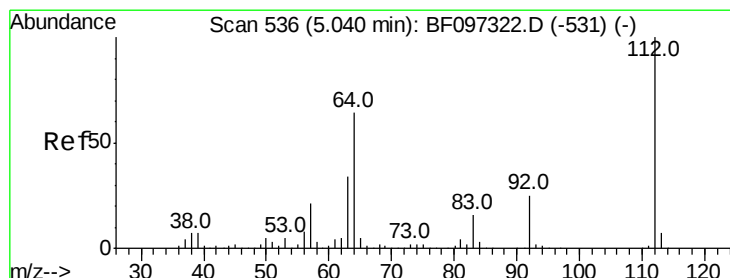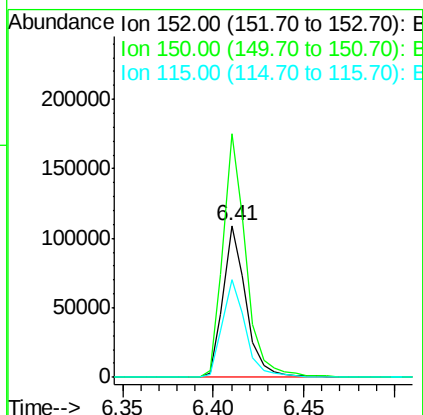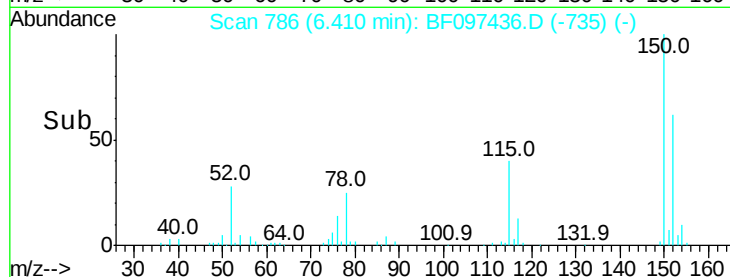



#5


2-Fluorophenol
 Concen: 95.368 ng
 RT: 5.00 min Scan# 547
 Delta R.T. 0.00 min
 Lab File: BF097436.D
 Acq: 7 Aug 2017 18:30

Tgt Ion:112 Resp: 611875
 Ion Ratio Lower Upper
 112 100
 64 64.6 46.0 69.0
 63 33.0 23.4 35.0

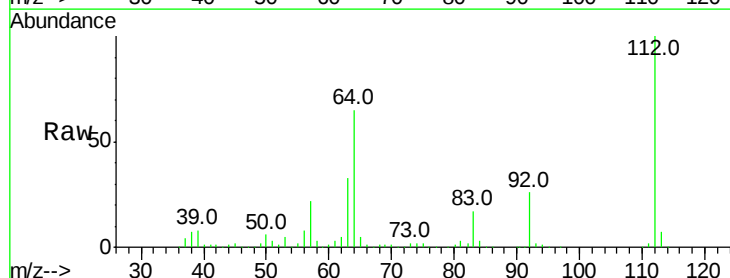

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

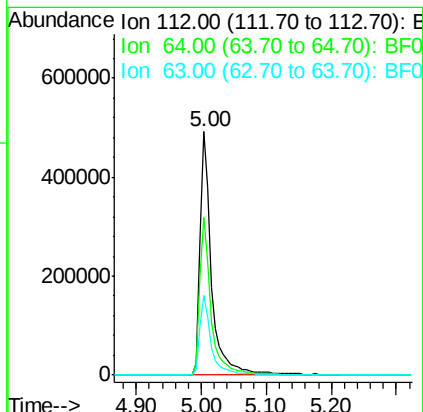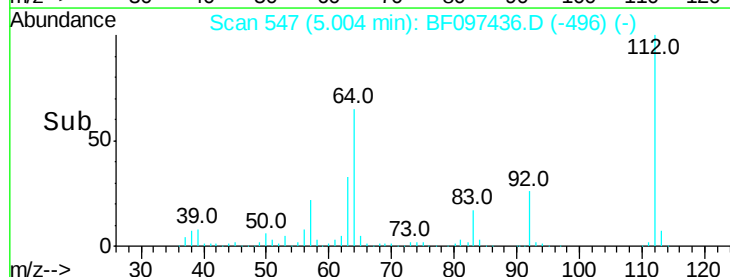

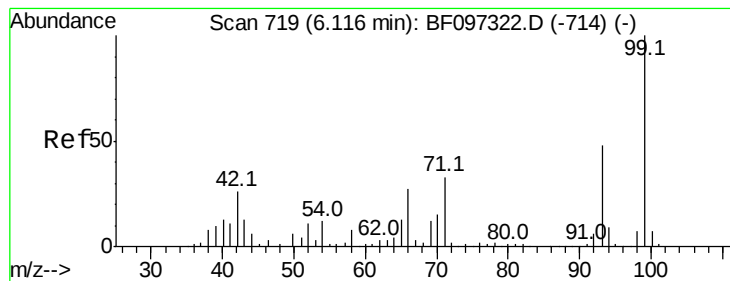

#7

Phenol-d6

Concen: 101.432 ng

RT: 6.09 min Scan# 731

Delta R.T. 0.00 min

Lab File: BF097436.D

Acq: 7 Aug 2017 18:30

Instrument :


BNA_F

ClientSampleId :

TEC-BC

Tot Ion: 99 Resp: 742951




Ion	Ratio	Lower	Upper
99	100		
42	23.1	13.5	20.3#
71	32.0	24.5	36.7

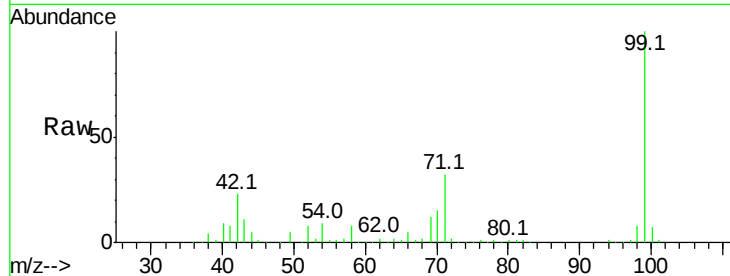

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

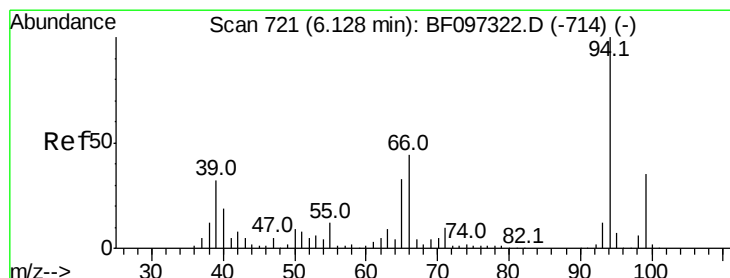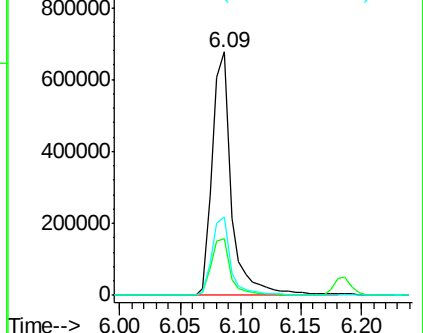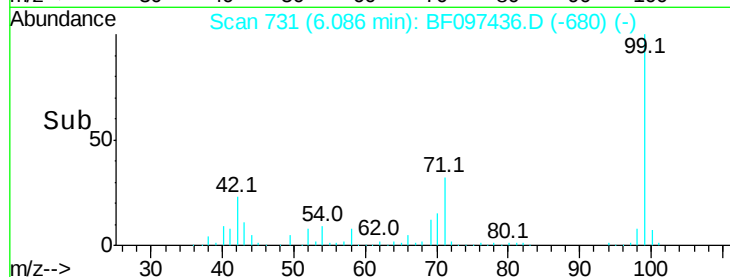

#10

Phenol

Concen: 3.403 ng

RT: 6.10 min Scan# 733


Delta R.T. 0.00 min

Lab File: BF097436.D

Acq: 7 Aug 2017 18:30

Tgt Ion: 94 Resp: 29563



Ion	Ratio	Lower	Upper
94	100		
65	34.0	9.9	49.9
66	57.1	23.1	63.1

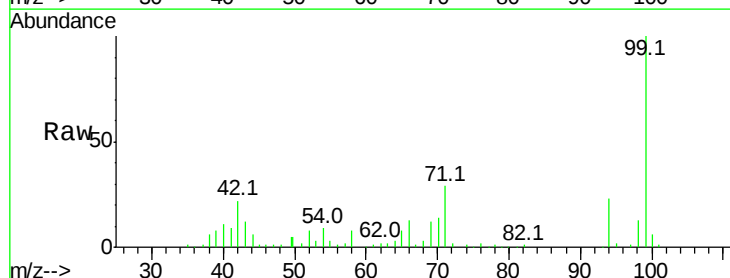


Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0

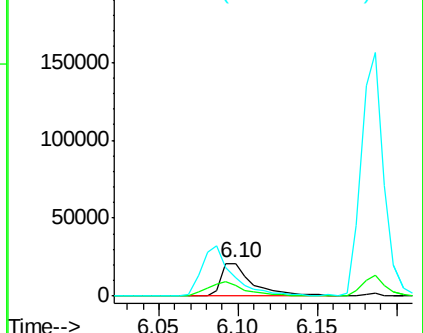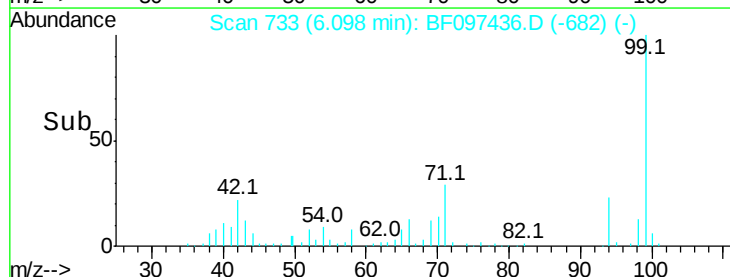



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.69 min Scan# 1004

Delta R.T. -0.01 min

Lab File: BF097436.D

Acq: 7 Aug 2017 18:30

Instrument :

BNA_F

ClientSampleId :

TEC-BC

Tot Ion:136 Resp: 389126


Ion Ratio Lower Upper

136 100

137 10.8 8.5 12.7

54 10.8 4.9 7.3#

68 5.5 4.1 6.1



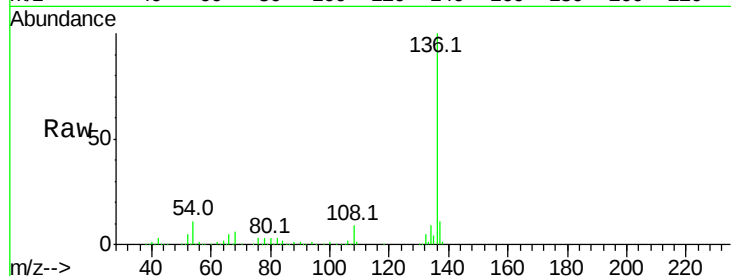


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

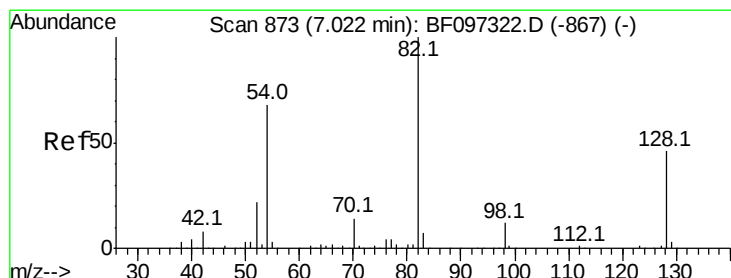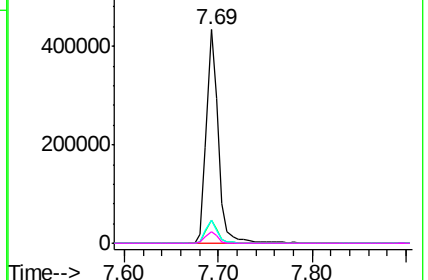

#23

Nitrobenzene-d5

Concen: 70.956 ng

RT: 6.98 min Scan# 883

Delta R.T. -0.01 min

Lab File: BF097436.D

Acq: 7 Aug 2017 18:30


Tgt Ion: 82 Resp: 470658

Ion Ratio Lower Upper

82 100

128 44.4 34.0 51.0



54 69.2 42.2 63.2#

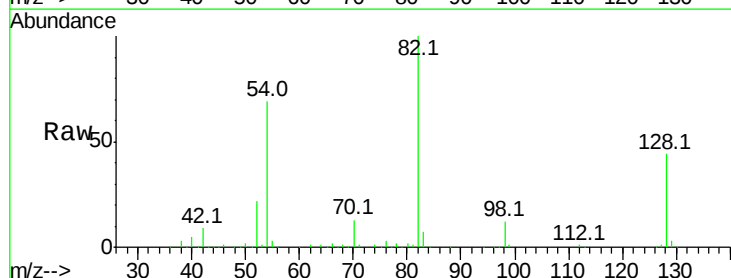


Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

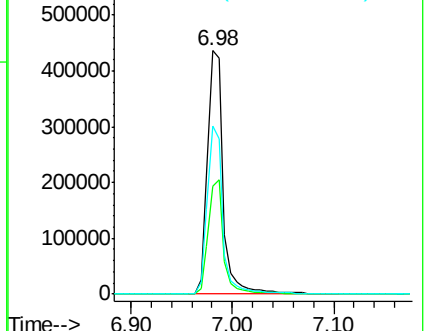







#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.43 min Scan# 1300
Delta R.T. -0.01 min
Lab File: BF097436.D
Acq: 7 Aug 2017 18:30

Instrument :
BNA_F
ClientSampleID :
TEC-BC

Tot Ion:164 Resp: 157127
Ion Ratio Lower Upper
164 100
162 103.2 82.6 123.8
160 45.0 36.2 54.2

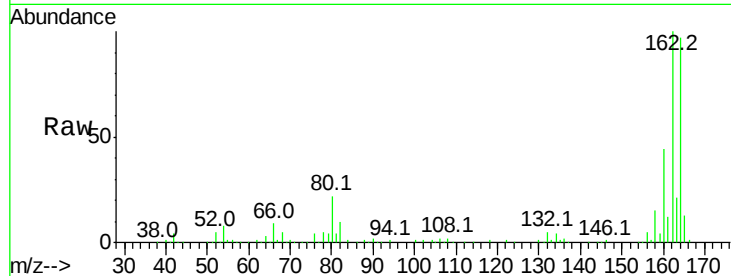


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

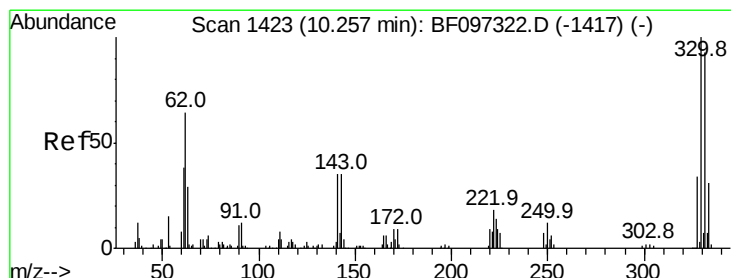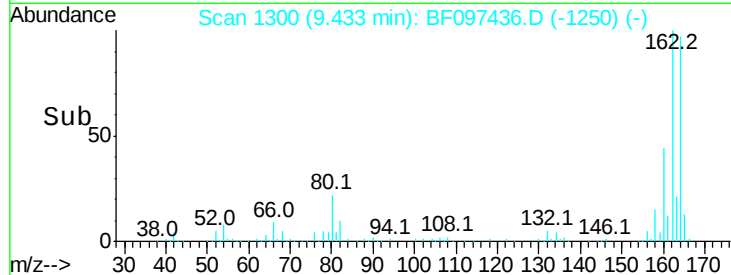
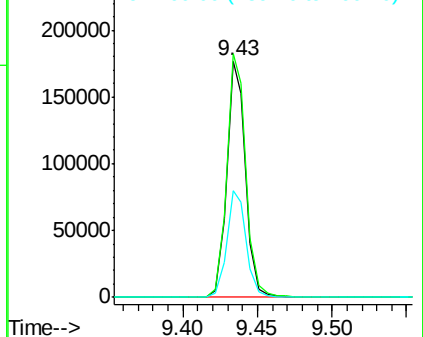



#41
2,4,6-Tribromophenol
Concen: 90.751 ng
RT: 10.23 min Scan# 1435
Delta R.T. -0.01 min
Lab File: BF097436.D
Acq: 7 Aug 2017 18:30

Tgt Ion:330 Resp: 112663
Ion Ratio Lower Upper
330 100
332 98.0 76.6 115.0
141 39.1 31.4 47.2

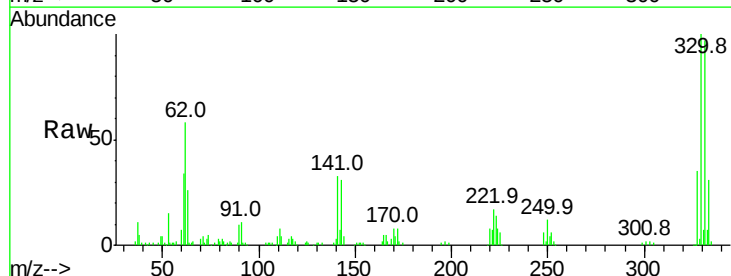

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E



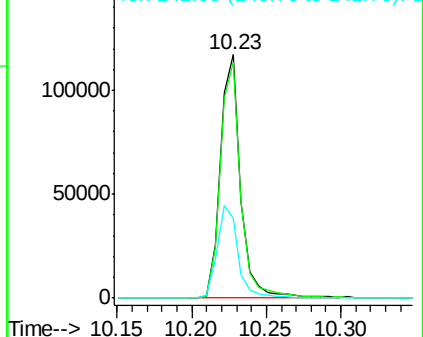




#44
2-Fluorobiphenyl
Concen: 80.638 ng
RT: 8.77 min Scan# 1188
Delta R.T. 0.00 min
Lab File: BF097436.D
Acq: 7 Aug 2017 18:30




Instrument :
BNA_F
ClientSampleId :
TEC-BC


Tot Ion:172 Resp: 746596
Ion Ratio Lower Upper
172 100
171 35.3 29.6 44.4
170 24.0 19.8 29.8

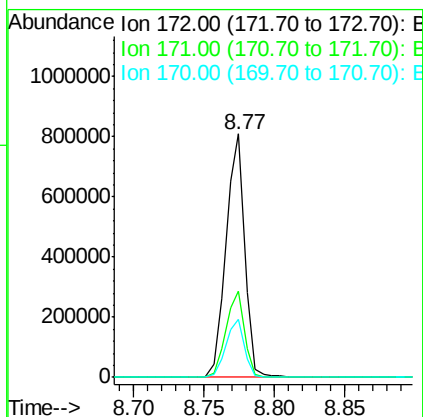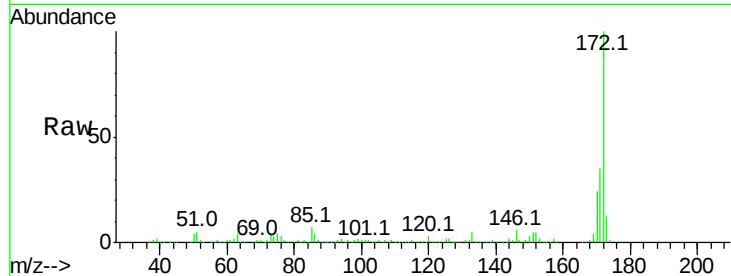

#49
Dimethylphthalate
Concen: 9.620 ng
RT: 9.17 min Scan# 1256
Delta R.T. -0.01 min
Lab File: BF097436.D
Acq: 7 Aug 2017 18:30

Tgt Ion:163 Resp: 114791
Ion Ratio Lower Upper
163 100
194 3.4 2.6 4.0
164 10.4 8.4 12.6


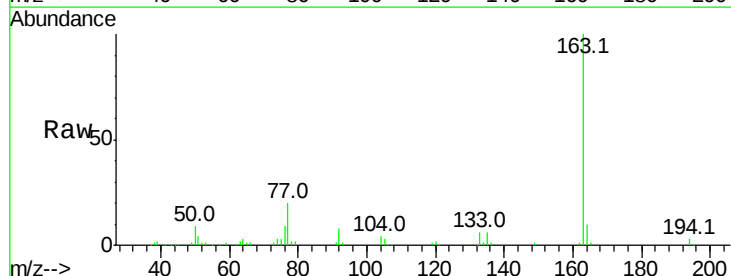
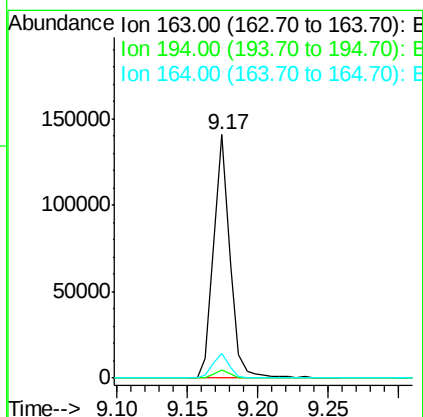
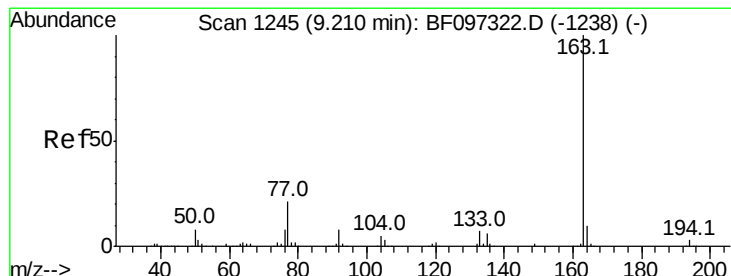


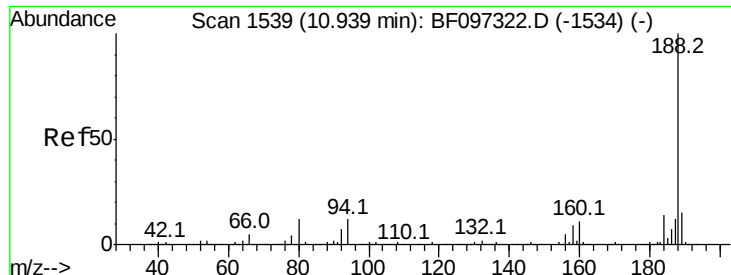

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 10.91 min Scan# 1551
Delta R.T. -0.01 min
Lab File: BF097436.D
Acq: 7 Aug 2017 18:30




Instrument :
BNA_F
ClientSampleId :
TEC-BC


Tot Ion:188 Resp: 225714
Ion Ratio Lower Upper
188 100
94 11.1 9.4 14.2
80 11.4 10.2 15.2

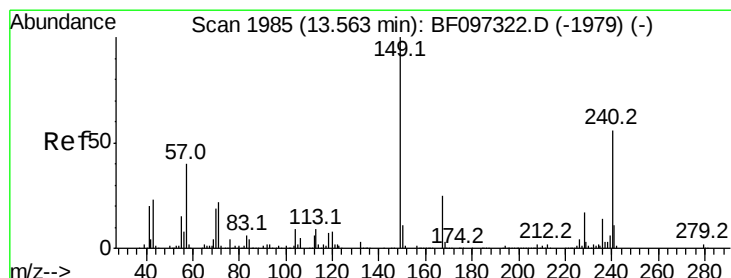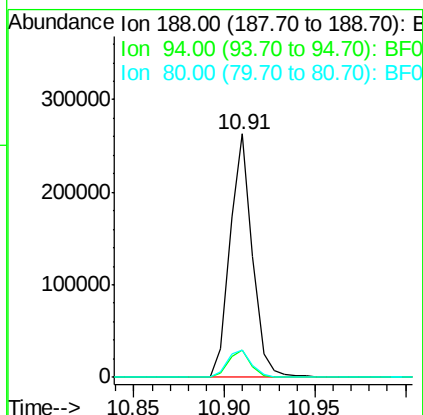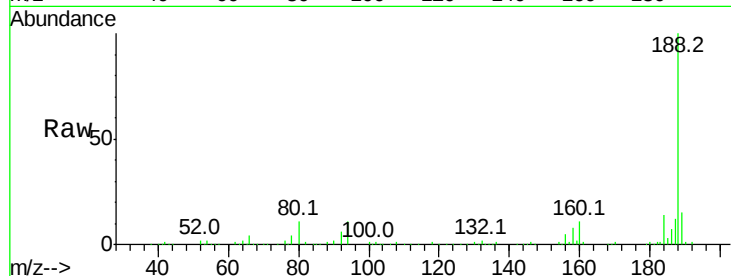

#75
Chrysene-d12
Concen: 20.000 ng
RT: 13.53 min Scan# 1997
Delta R.T. -0.01 min
Lab File: BF097436.D
Acq: 7 Aug 2017 18:30

Tgt Ion:240 Resp: 203947
Ion Ratio Lower Upper
240 100
120 15.4 5.8 8.8#
236 25.8 20.5 30.7

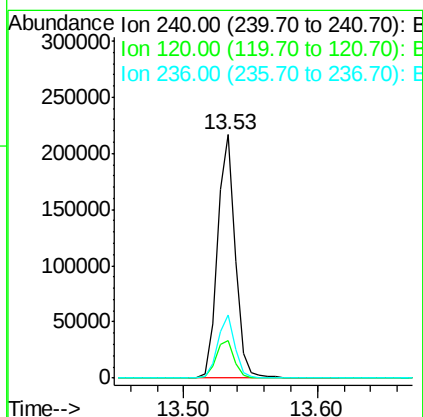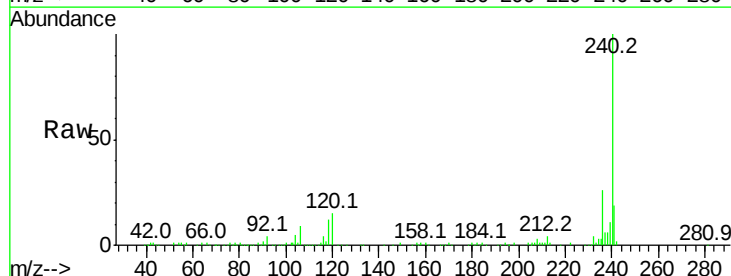

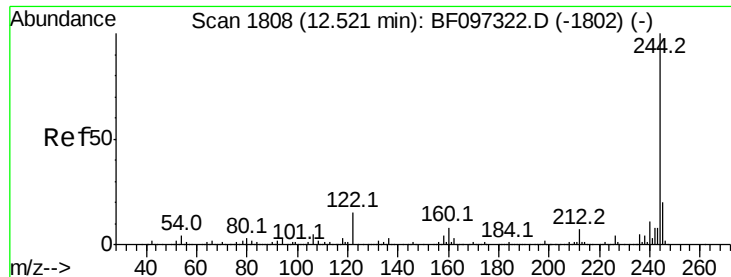

#78

Terphenyl-d14

Concen: 43.603 ng

RT: 12.49 min Scan# 1820

Delta R.T. -0.01 min

Lab File: BF097436.D

Acq: 7 Aug 2017 18:30

Instrument :

BNA_F

ClientSampleId :

TEC-BC


Tot Ion:244 Resp: 436166

Ion Ratio Lower Upper




244 100

212 6.7 6.0 9.0

122 14.3 10.3 15.5

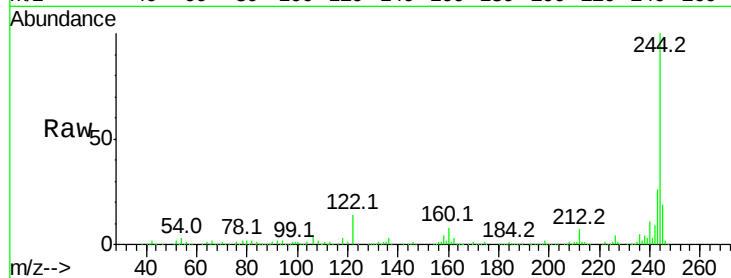

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

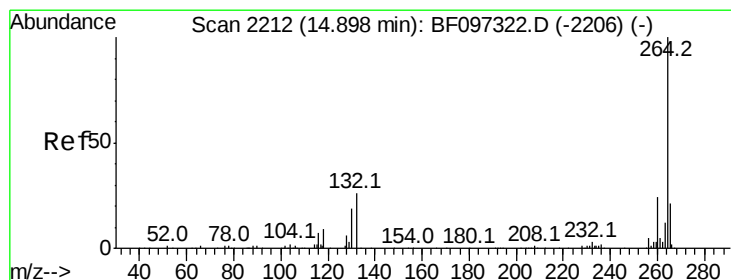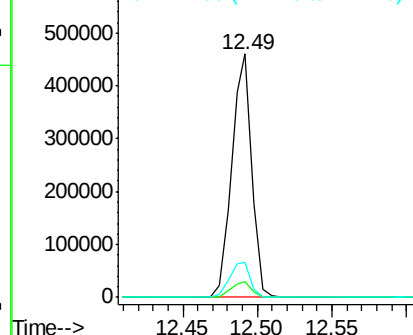

#86

Perylene-d12

Concen: 20.000 ng

RT: 14.87 min Scan# 2224

Delta R.T. 0.00 min

Lab File: BF097436.D

Acq: 7 Aug 2017 18:30


Tgt Ion:264 Resp: 151739

Ion Ratio Lower Upper

264 100

260 23.9 19.5 29.3

265 21.3 17.2 25.8

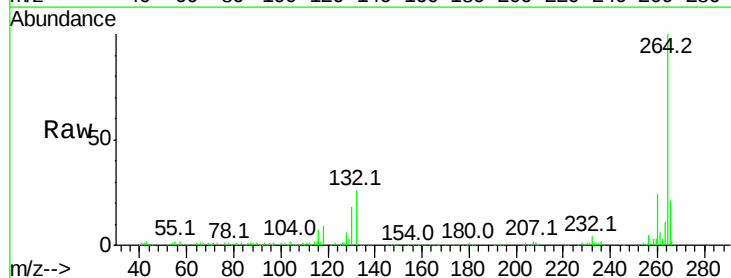

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

