


Data Path : Z:\HPCHEM1\BNA F\Data\BF080717\
 Data File : BF097425.D
 Acq On : 7 Aug 2017 13:08
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 07 16:02:51 2017

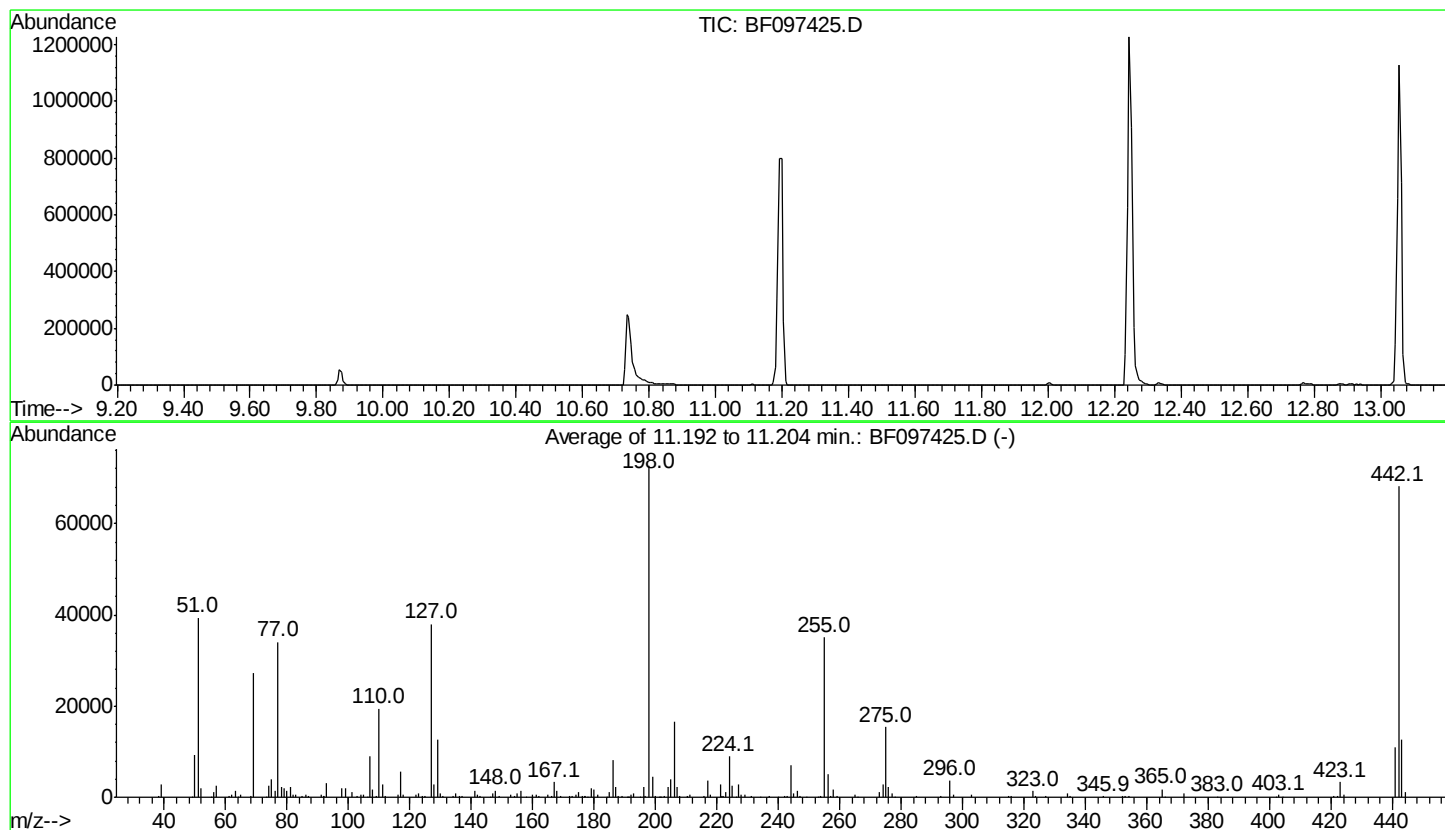

AutoFind: Scans 1599, 1600, 1601; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.1	39344	PASS
68	69	0.00	2	1.5	411	PASS
69	198	0.00	100	37.5	27256	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.3	38029	PASS
197	198	0.00	2	0.5	393	PASS
198	198	100	100	100.0	72706	PASS
199	198	5	9	6.2	4536	PASS
275	198	10	60	21.2	15395	PASS
365	198	1	100	2.5	1823	PASS
441	442	0.01	24	16.1	10993	PASS
442	198	50	100	93.7	68090	PASS
443	442	15	24	18.6	12657	PASS