


Data Path : Z:\HPCHEM1\BNA F\Data\BF080717\
 Data File : BF097450.D
 Acq On : 8 Aug 2017 1:49
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 07 16:02:51 2017

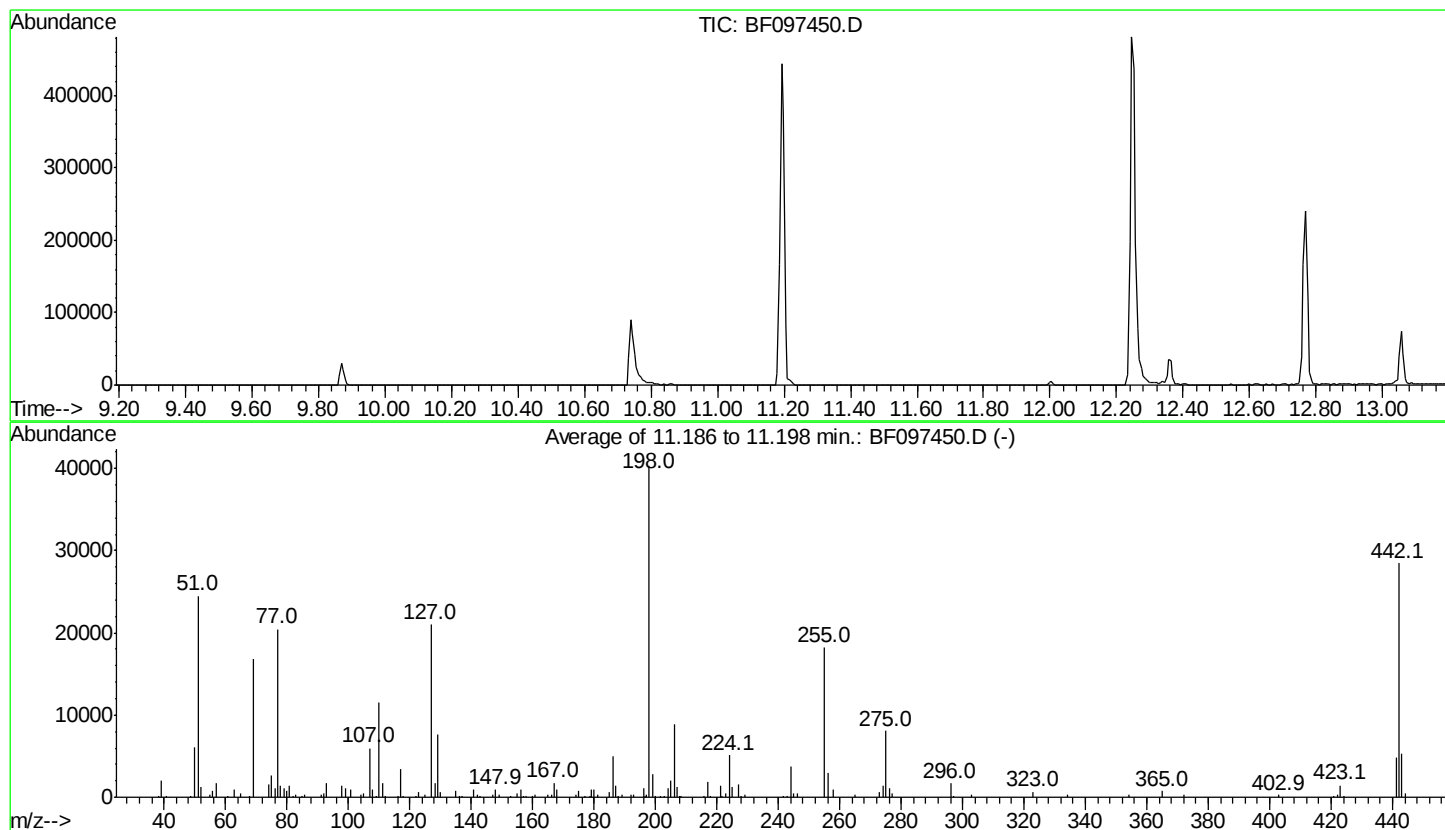

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.7	24480	PASS
68	69	0.00	2	1.1	182	PASS
69	198	0.00	100	41.6	16790	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.1	21027	PASS
197	198	0.00	2	0.6	248	PASS
198	198	100	100	100.0	40357	PASS
199	198	5	9	6.8	2745	PASS
275	198	10	60	20.1	8095	PASS
365	198	1	100	1.8	717	PASS
441	442	0.01	24	16.8	4786	PASS
442	198	50	100	70.6	28508	PASS
443	442	15	24	18.8	5357	PASS