
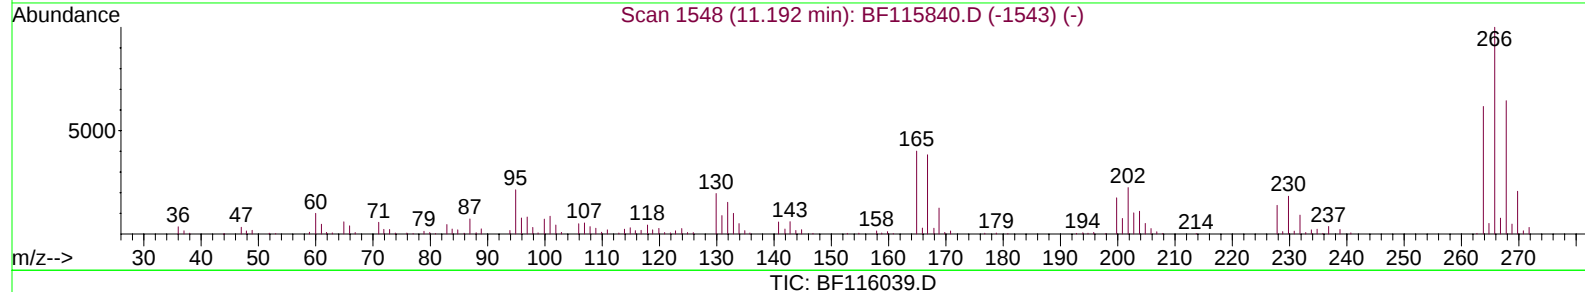
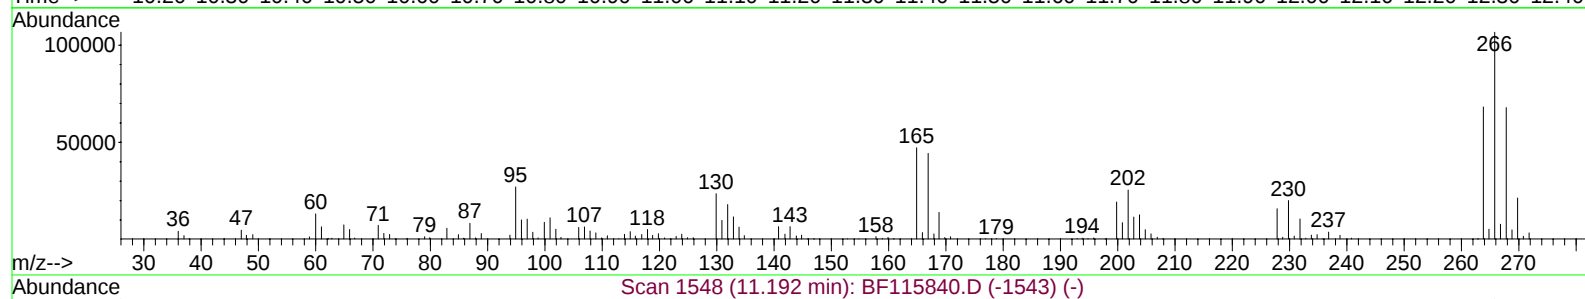


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF080719\
 Data File : BF116039.D
 Acq On : 7 Aug 2019 9:34
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 11:06:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 31 15:31:51 2019
 Response via : Initial Calibration

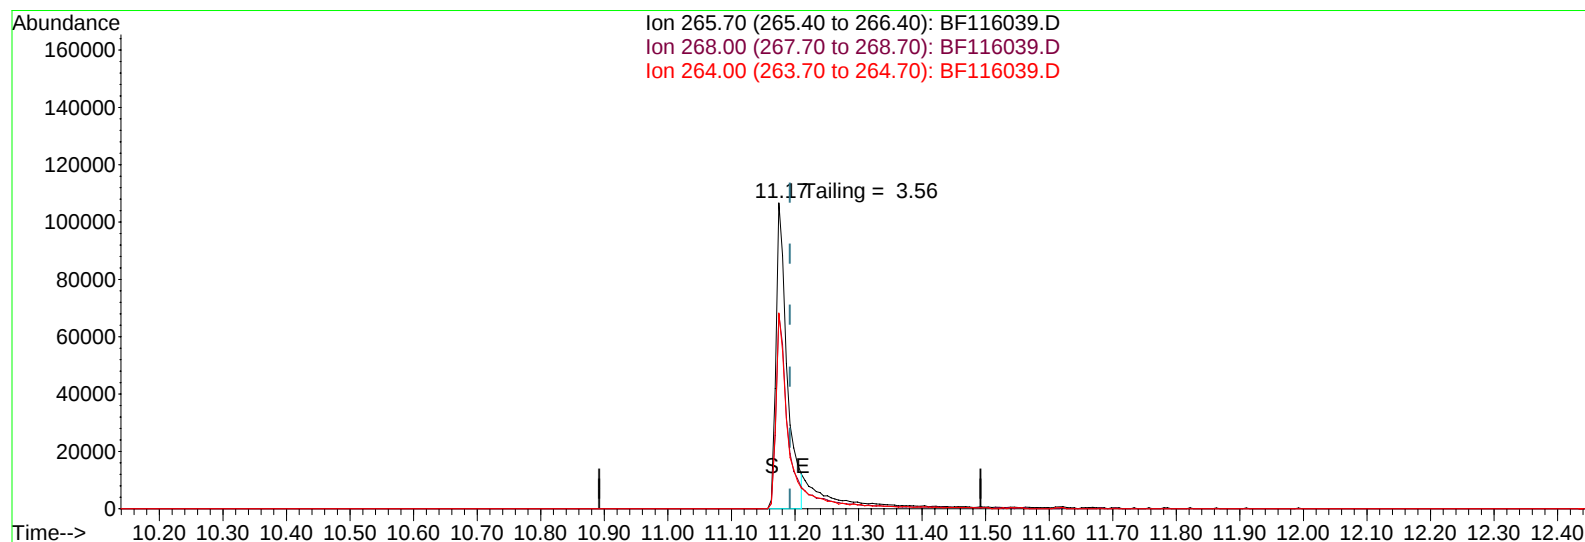

(70) Pentachlorophenol (C)




11.175min (-0.017) 246974.24ng

response 164753

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	63.65
264.00	61.70	64.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF080719\
 Data File : BF116039.D
 Acq On : 7 Aug 2019 9:34
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 11:06:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 31 15:31:51 2019
 Response via : Initial Calibration

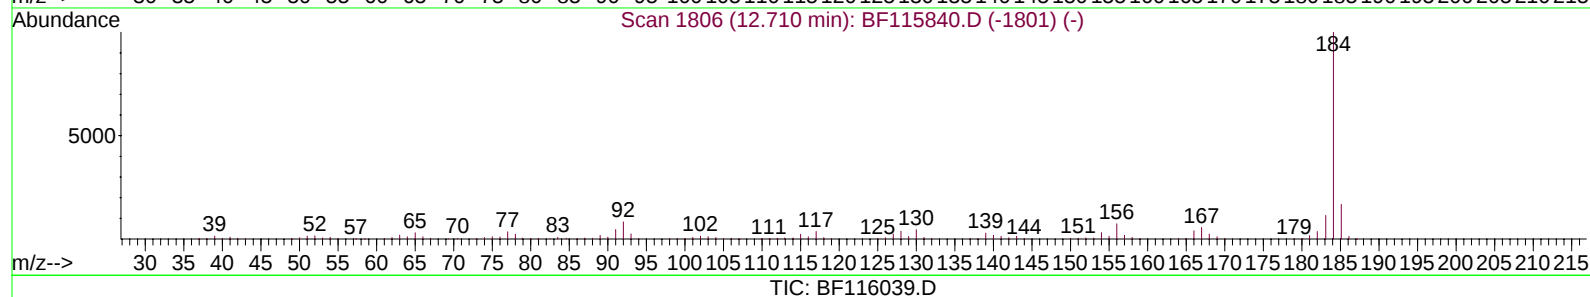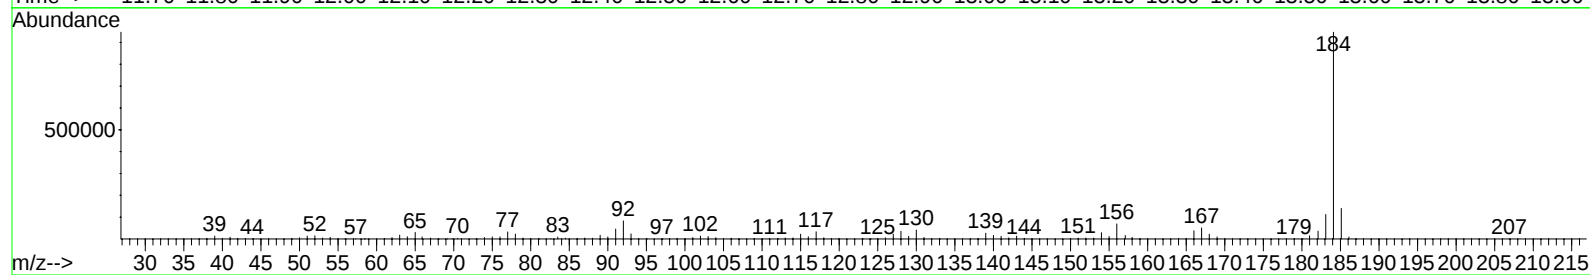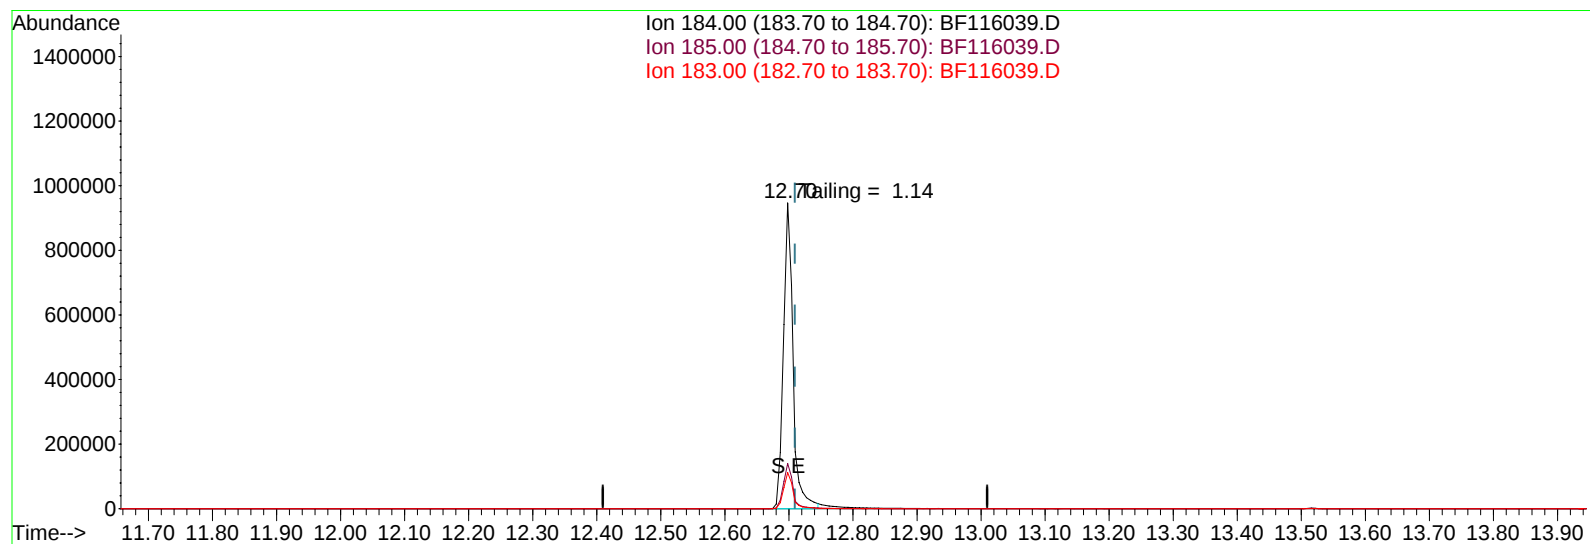

(77) Benzidine

12.698min (-0.012) 0.00ng

response 1024646

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.80
183.00	11.40	11.85
0.00	0.00	0.00