
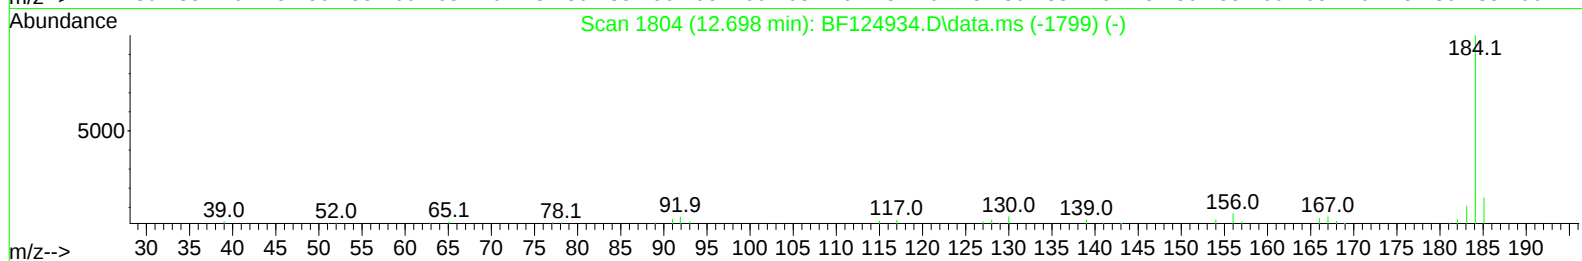
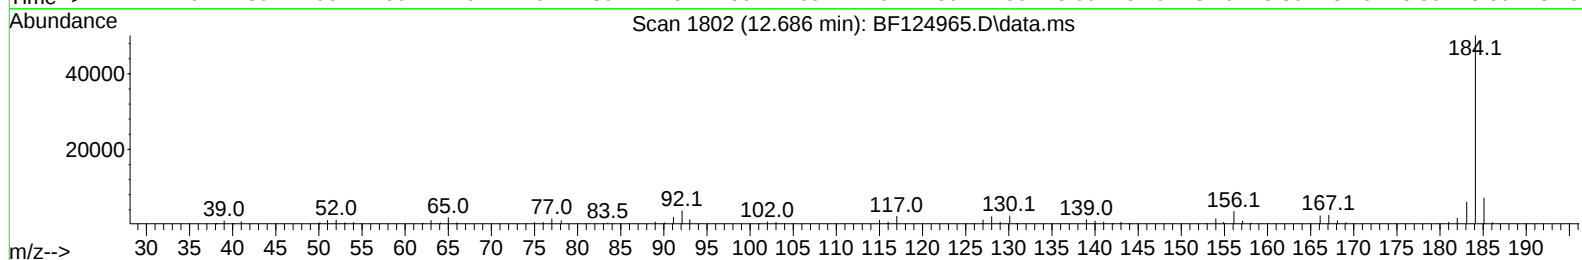


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080721\
 Data File : BF124965.D
 Acq On : 7 Aug 2021 9:25
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 11:03:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 06 11:27:24 2021
 Response via : Initial Calibration

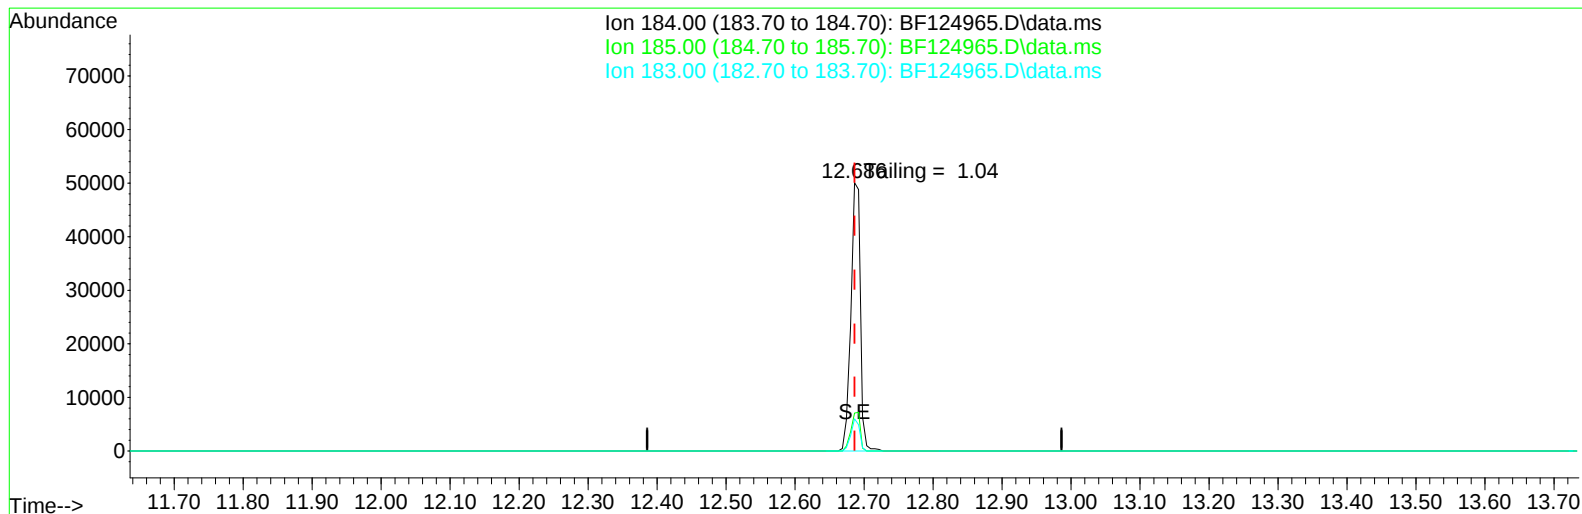

TIC: BF124965.D\data.ms

(77) Benzidine




12.686min (+ 0.000) 0.00 ng

response 48337

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.13
183.00	10.10	12.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080721\
Data File : BF124965.D
Acq On : 7 Aug 2021 9:25
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 11:03:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 06 11:27:24 2021
Response via : Initial Calibration

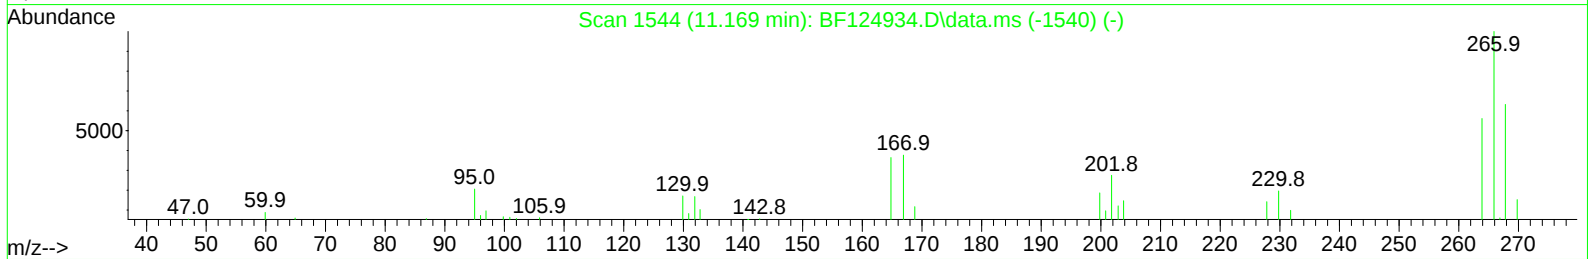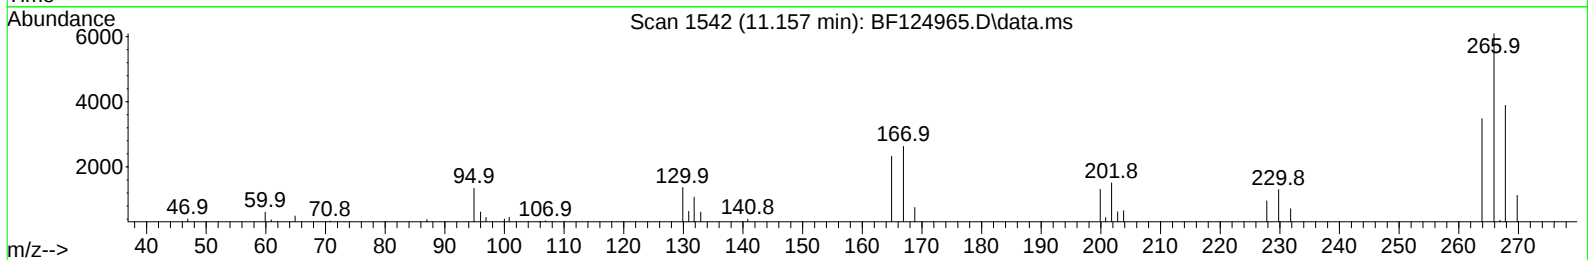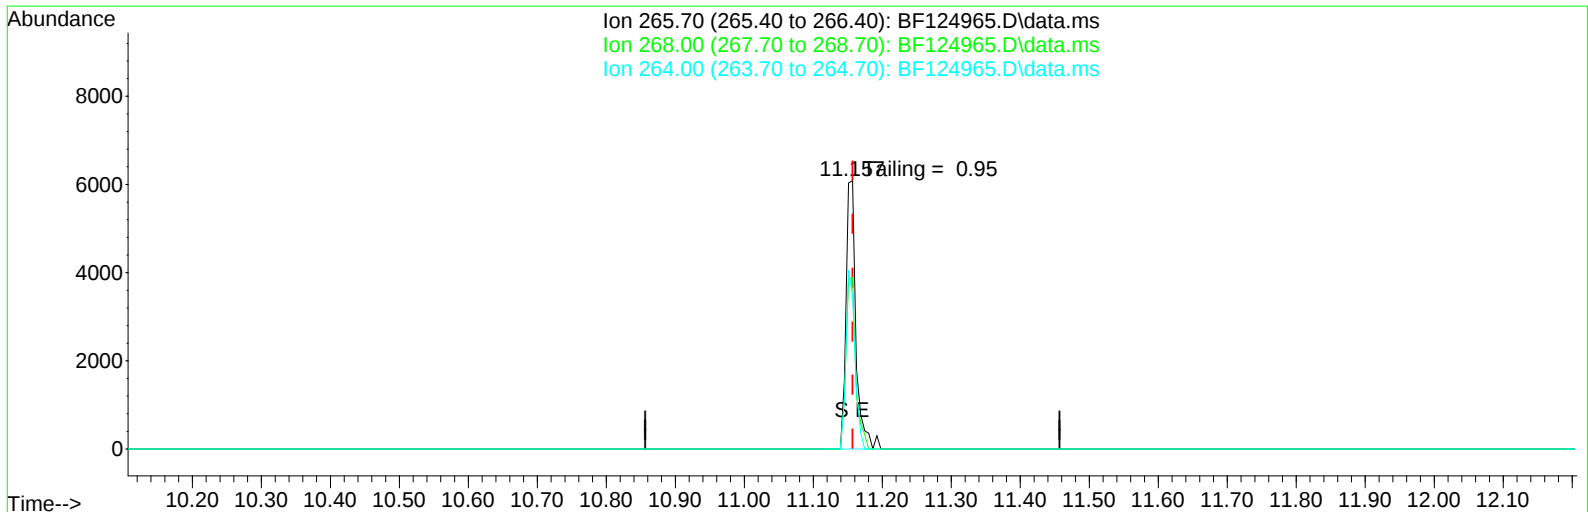

TIC: BF124965.D\data.ms

(70) Pentachlorophenol (C)

11.157min (+ 0.000) 0.00 ng

response 6115

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	63.86
264.00	69.90	57.17
0.00	0.00	0.00