

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080721\
 Data File : BF124967.D
 Acq On : 7 Aug 2021 10:29
 Operator : JU/CG
 Sample : PB138219BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB138219BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124967.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.451	568	572	575	rBV	166921	157793	45.98%	8.652%
2	6.457	738	743	746	rBV	165679	158352	46.14%	8.683%
3	6.828	803	806	809	rBB	59287	46881	13.66%	2.571%
4	6.986	829	833	836	rBB	237388	211363	61.59%	11.590%
5	7.392	897	902	905	rBB	155072	164125	47.82%	8.999%
6	8.110	1019	1024	1027	rBB	64841	60339	17.58%	3.309%
7	9.186	1201	1207	1210	rBB	323739	312223	90.98%	17.120%
8	9.863	1318	1322	1325	rBB	87568	71134	20.73%	3.900%
9	10.651	1452	1456	1459	rBV	134436	108766	31.69%	5.964%
10	11.351	1571	1575	1578	rBB	92759	75302	21.94%	4.129%
11	12.939	1840	1845	1848	rBV	369320	343182	100.00%	18.818%
12	13.986	2020	2023	2026	rBB	77854	60856	17.73%	3.337%
13	15.445	2266	2271	2276	rBB	48715	53414	15.56%	2.929%




Sum of corrected areas: 1823730

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080721\
Data File : BF124967.D
Acq On : 7 Aug 2021 10:29
Operator : JU/CG
Sample : PB138219BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138219BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

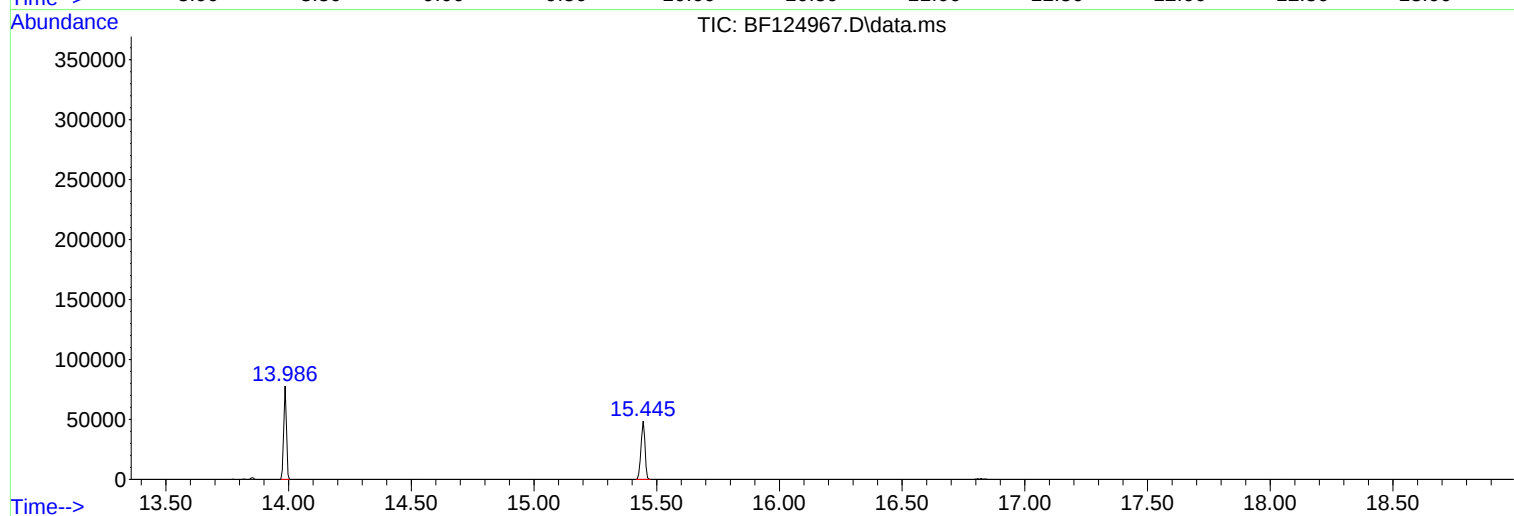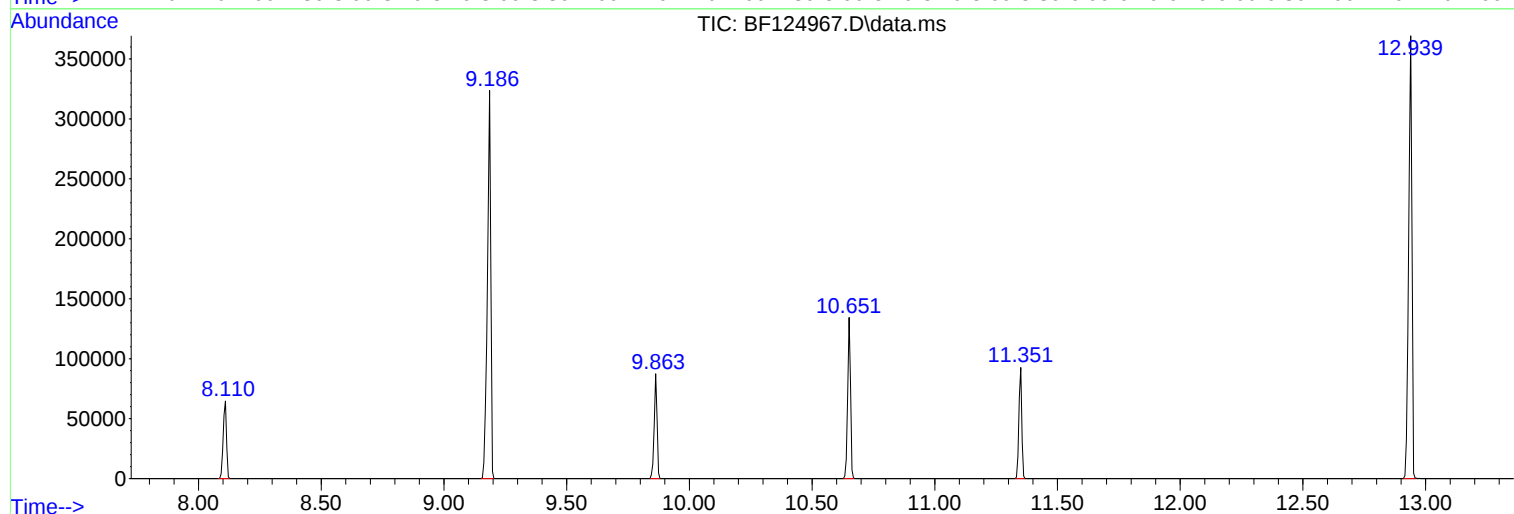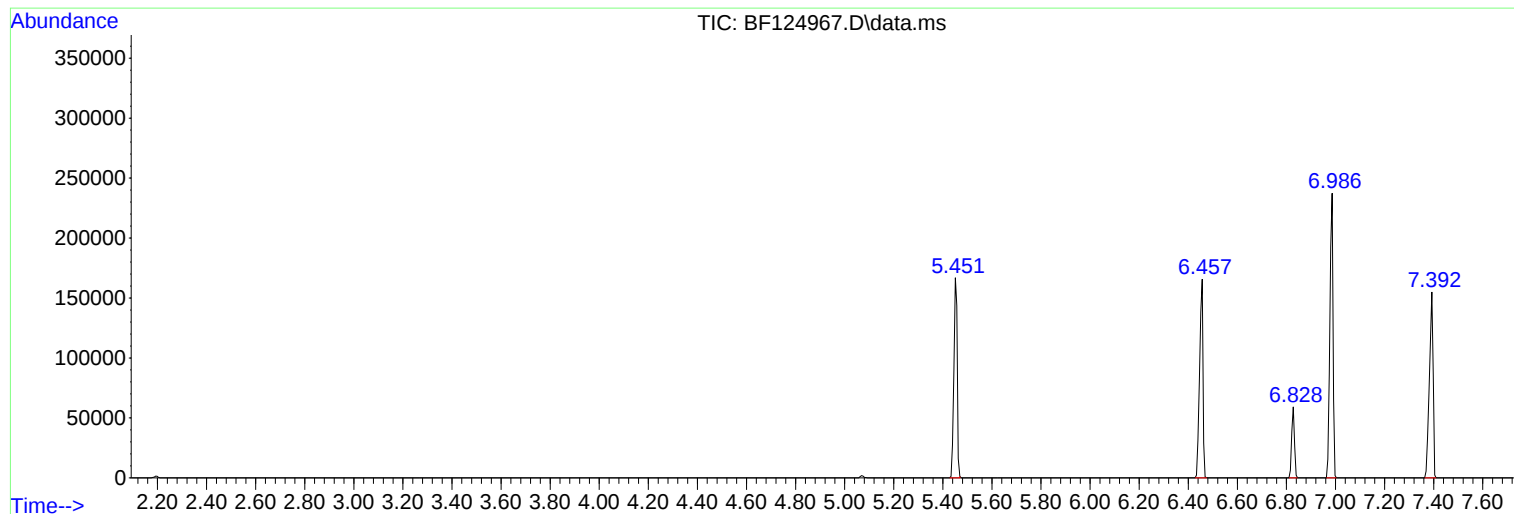

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080721\
Data File : BF124967.D
Acq On : 7 Aug 2021 10:29
Operator : JU/CG
Sample : PB138219BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138219BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080721\
Data File : BF124967.D
Acq On : 7 Aug 2021 10:29
Operator : JU/CG
Sample : PB138219BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138219BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------