

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080721\
 Data File : BF124982.D
 Acq On : 7 Aug 2021 19:31
 Operator : JU/CG
 Sample : M3305-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SA-01-080521

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124982.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.046	500	503	507	rBB	5717	6336	3.81%	0.654%
2	5.446	567	571	574	rBV	146450	127954	77.00%	13.217%
3	6.463	739	744	747	rBB	146409	135062	81.27%	13.951%
4	6.828	803	806	809	rBB	45426	31979	19.24%	3.303%
5	7.392	898	902	905	rBB	104724	87778	52.82%	9.067%
6	8.010	1005	1007	1010	rBB	12048	8228	4.95%	0.850%
7	8.110	1021	1024	1027	rBB	60440	43768	26.34%	4.521%
8	9.186	1203	1207	1210	rBB	221990	166183	100.00%	17.165%
9	9.863	1319	1322	1325	rBB	66449	51009	30.69%	5.269%
10	10.651	1453	1456	1459	rBB	109044	84205	50.67%	8.698%
11	11.351	1571	1575	1578	rBB	56382	43792	26.35%	4.523%
12	12.933	1840	1844	1847	rBB	158428	117258	70.56%	12.112%
13	13.821	1993	1995	1999	rBB	3141	2802	1.69%	0.289%
14	13.986	2020	2023	2026	rBB	35016	28216	16.98%	2.914%
15	15.445	2266	2271	2276	rBB2	26733	31270	18.82%	3.230%
16	15.892	2341	2347	2351	rBB2	1421	2297	1.38%	0.237%




Sum of corrected areas: 968137

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080721\
Data File : BF124982.D
Acq On : 7 Aug 2021 19:31
Operator : JU/CG
Sample : M3305-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SA-01-080521

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

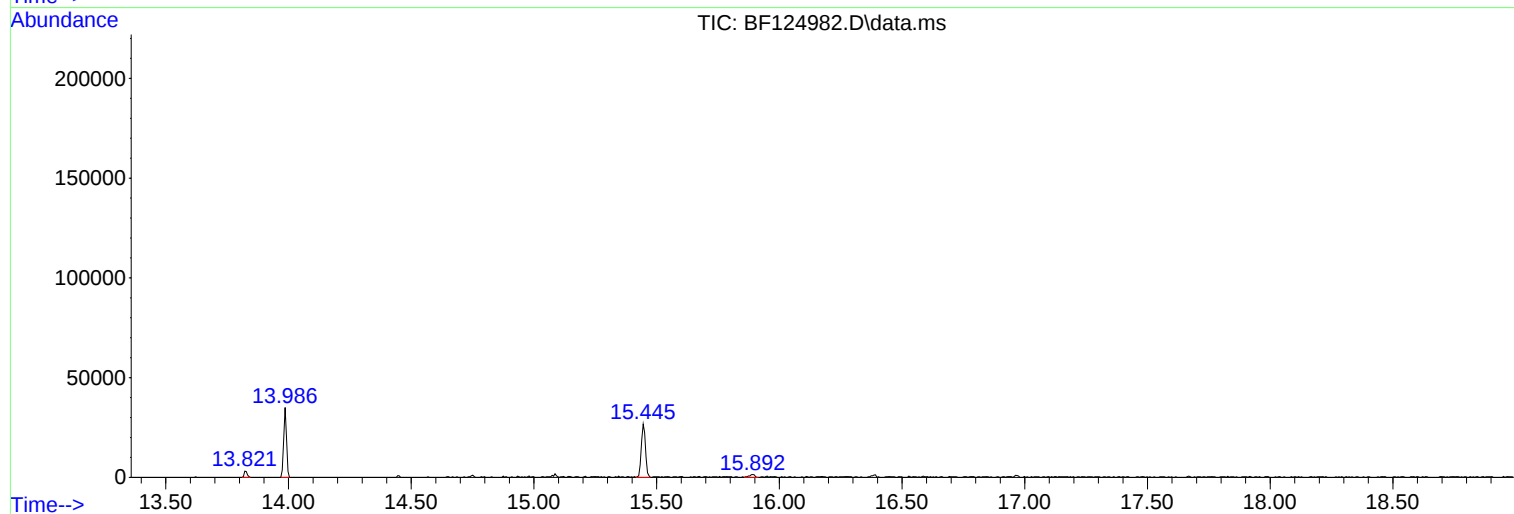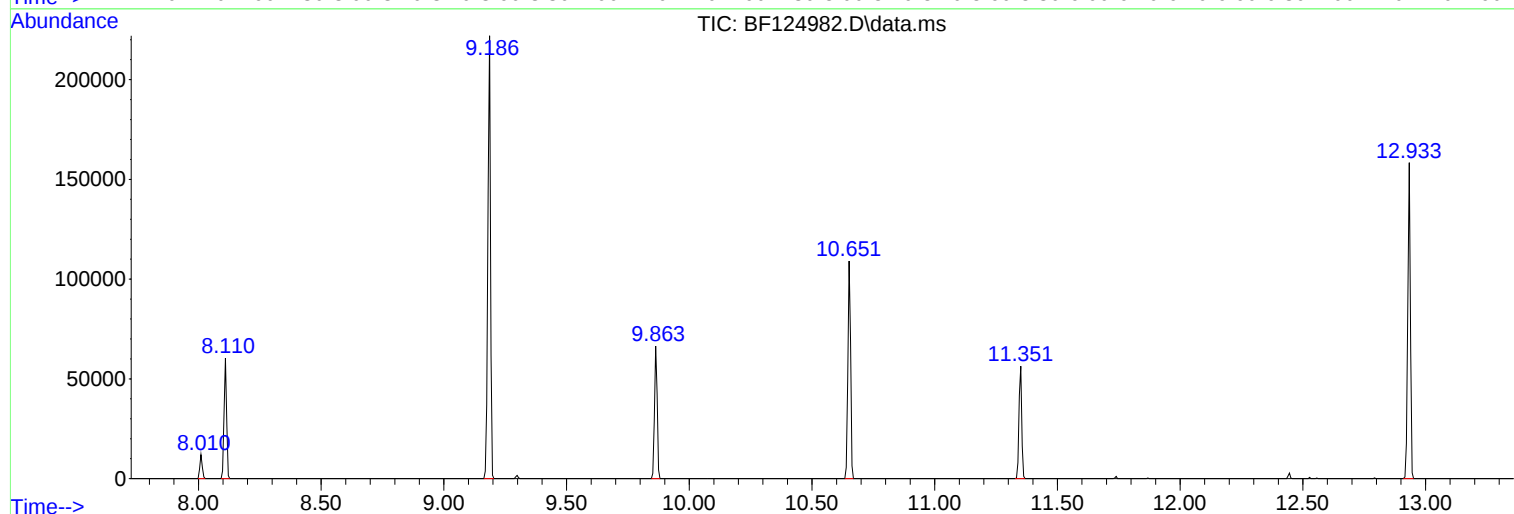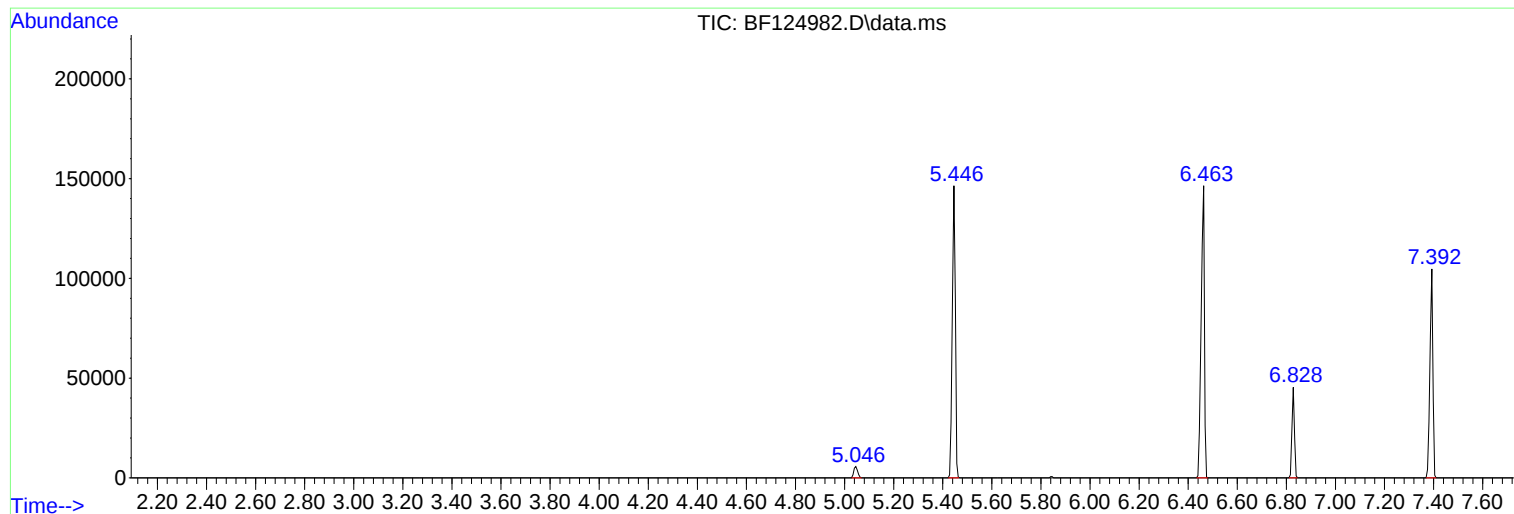

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080721\
Data File : BF124982.D
Acq On : 7 Aug 2021 19:31
Operator : JU/CG
Sample : M3305-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SA-01-080521









Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown5.046 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.046	3.96 ng	6336	1,4-Dichlorobenzene-d4	6.828

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Oxirane, [(1-methylethoxy)methyl]-	116	C6H12O2	004016-14-2	9
2			Diacetamide	101	C4H7NO2	000625-77-4	7
3			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	7
4			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	4
5			N-(n-Propyl)acetamide	101	C5H11NO	005331-48-6	3

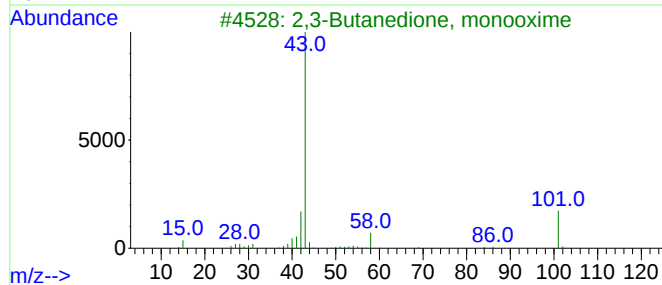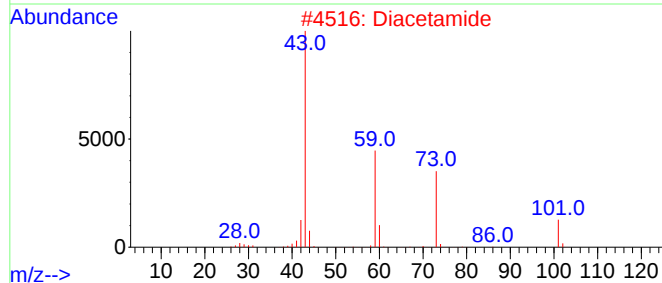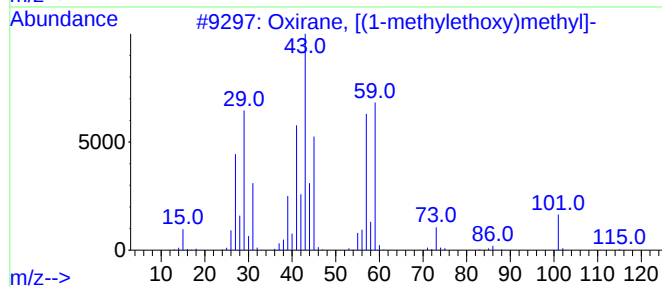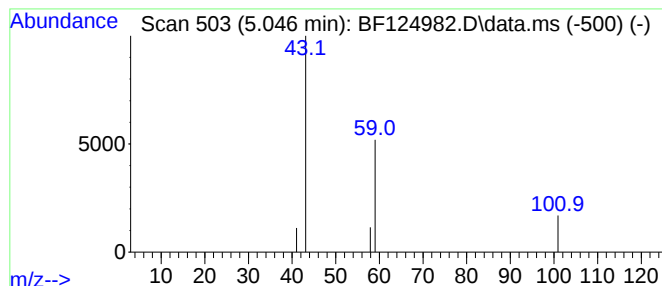

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080721\
Data File : BF124982.D
Acq On : 7 Aug 2021 19:31
Operator : JU/CG
Sample : M3305-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SA-01-080521










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown8.010 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.010	3.76 ng	8228	Naphthalene-d8	8.110

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Aziridine, 1-(methoxymethyl)-	87	C4H9NO	001497-83-2	7
2		1-Pentanamine	87	C5H13N	000110-58-7	5
3		2-Propanol, 1-amino-, (R)-	75	C3H9NO	002799-16-8	4
4		3-Buten-2-ol	72	C4H8O	000598-32-3	4
5		Methane, nitroso-	45	CH3NO	000865-40-7	4

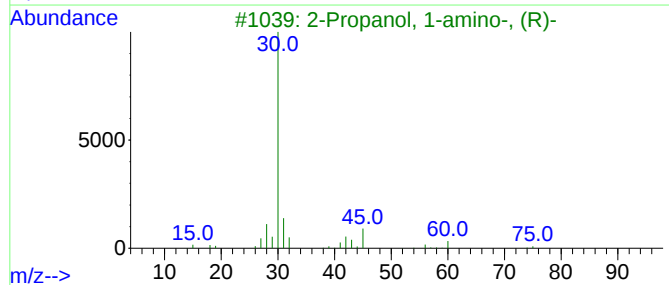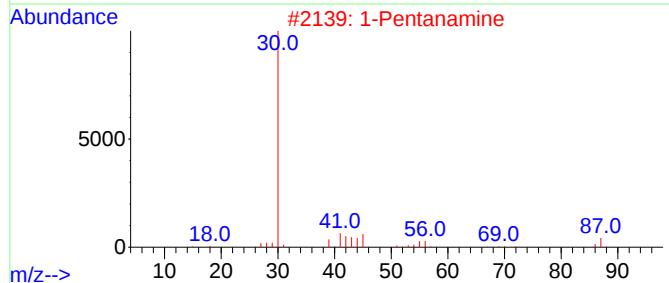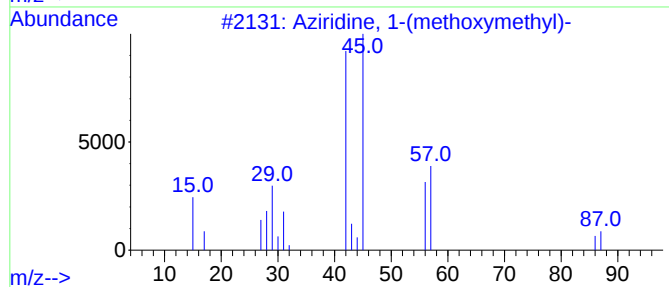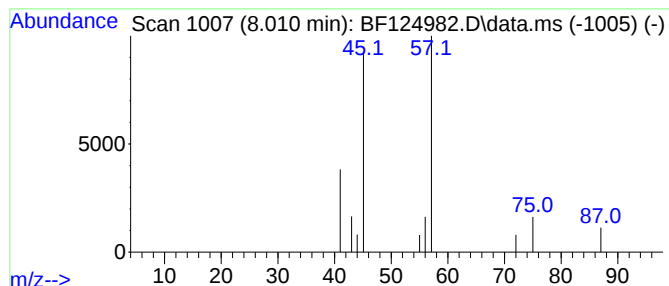

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080721\
Data File : BF124982.D
Acq On : 7 Aug 2021 19:31
Operator : JU/CG
Sample : M3305-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SA-01-080521

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.046	5.046	4.0	ng	6336	1	6.828	31979	20.0
unknown8.010	8.010	3.8	ng	8228	2	8.110	43768	20.0