


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080721\
 Data File : BF124965.D
 Acq On : 7 Aug 2021 9:25
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 09 11:03:44 2021

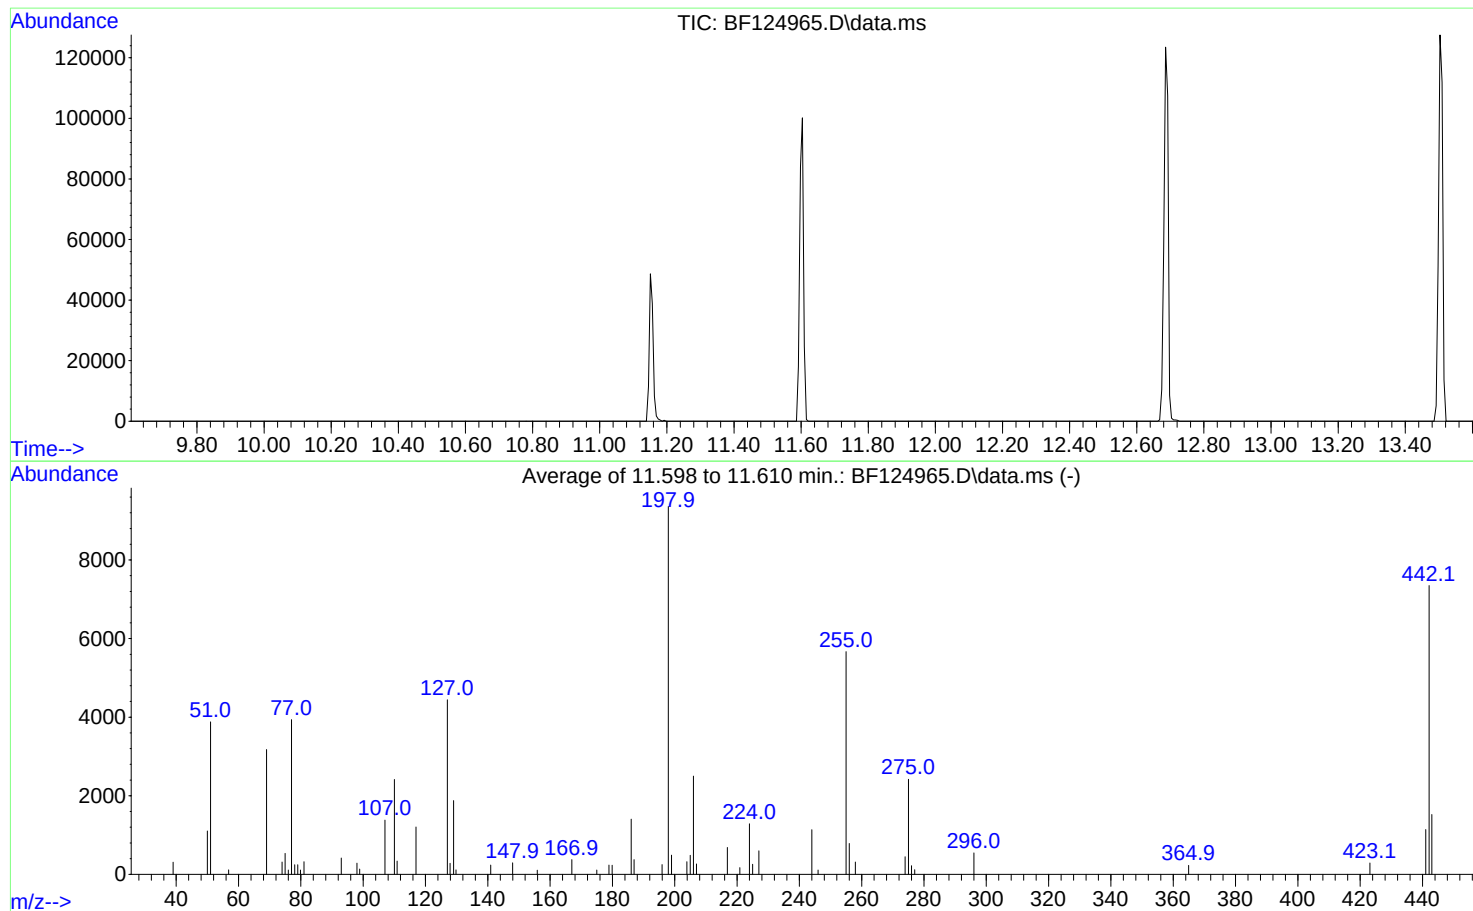




AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	3879	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.9	3176	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.4	4441	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	9360	PASS
199	198	5	9	5.2	488	PASS
275	198	10	60	25.9	2420	PASS
365	198	1	100	2.5	230	PASS
441	198	0.01	100	12.2	1139	PASS
442	442	50	100	100.0	7350	PASS
443	442	15	24	20.7	1523	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080721\
 Data File : BF124965.D
 Acq On : 7 Aug 2021 9:25
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 07 11:03:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 06 11:27:24 2021
 Response via : Initial Calibration

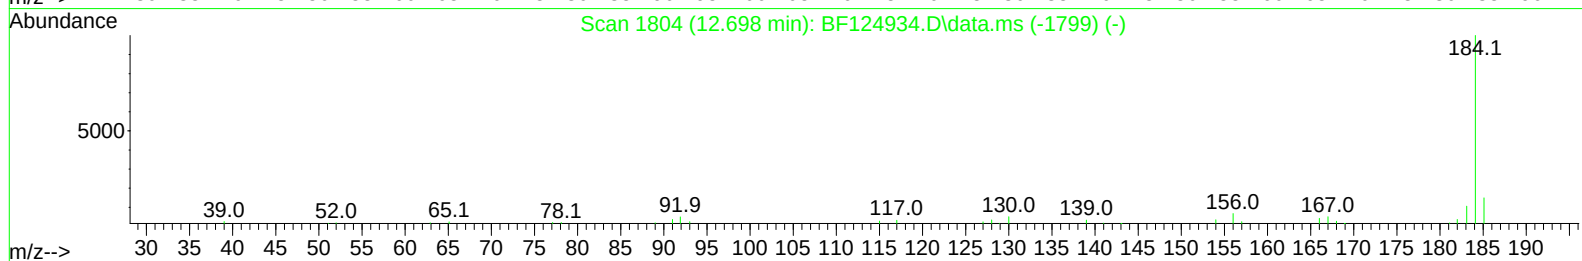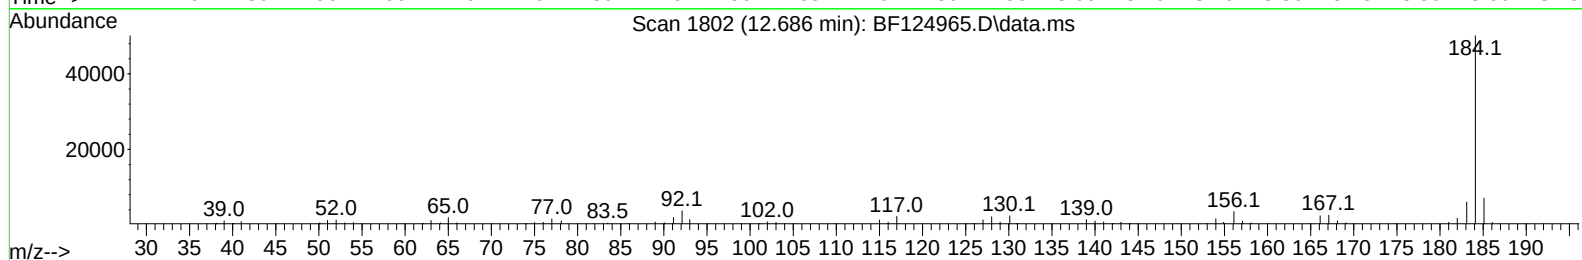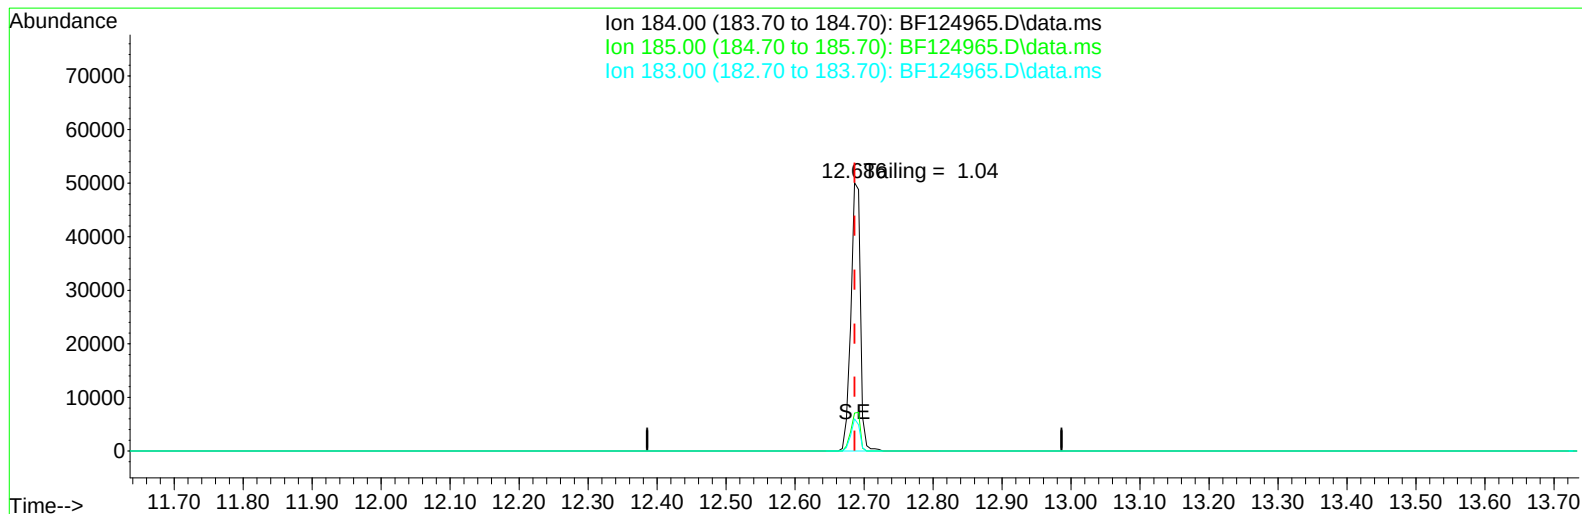

TIC: BF124965.D\data.ms

(77) Benzidine

12.686min (+ 0.000) 0.00 ng




response 48337

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.13
183.00	10.10	12.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080721\
Data File : BF124965.D
Acq On : 7 Aug 2021 9:25
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 07 11:03:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 06 11:27:24 2021
Response via : Initial Calibration

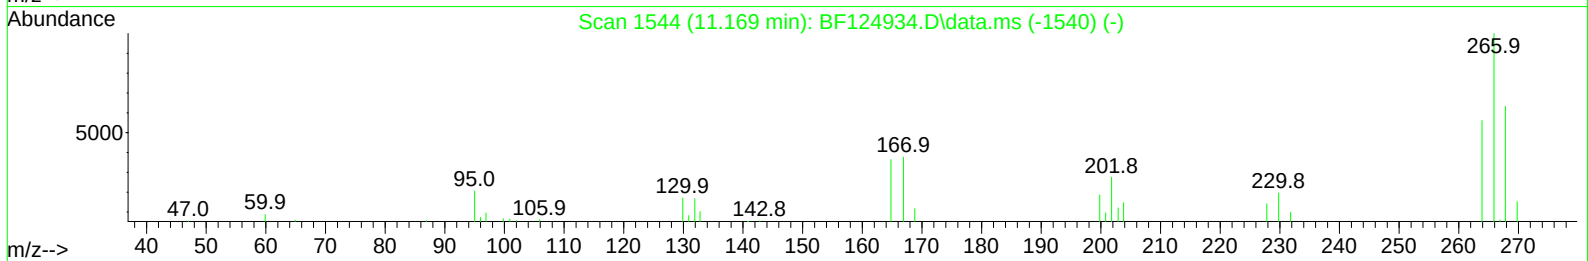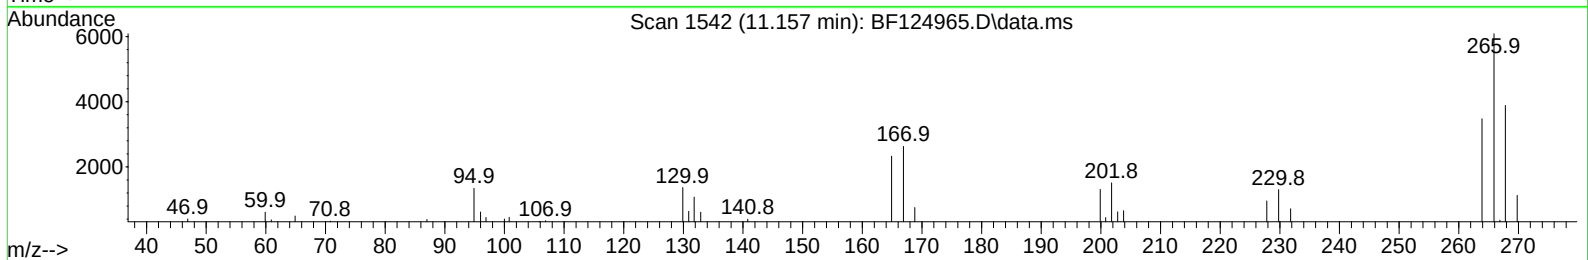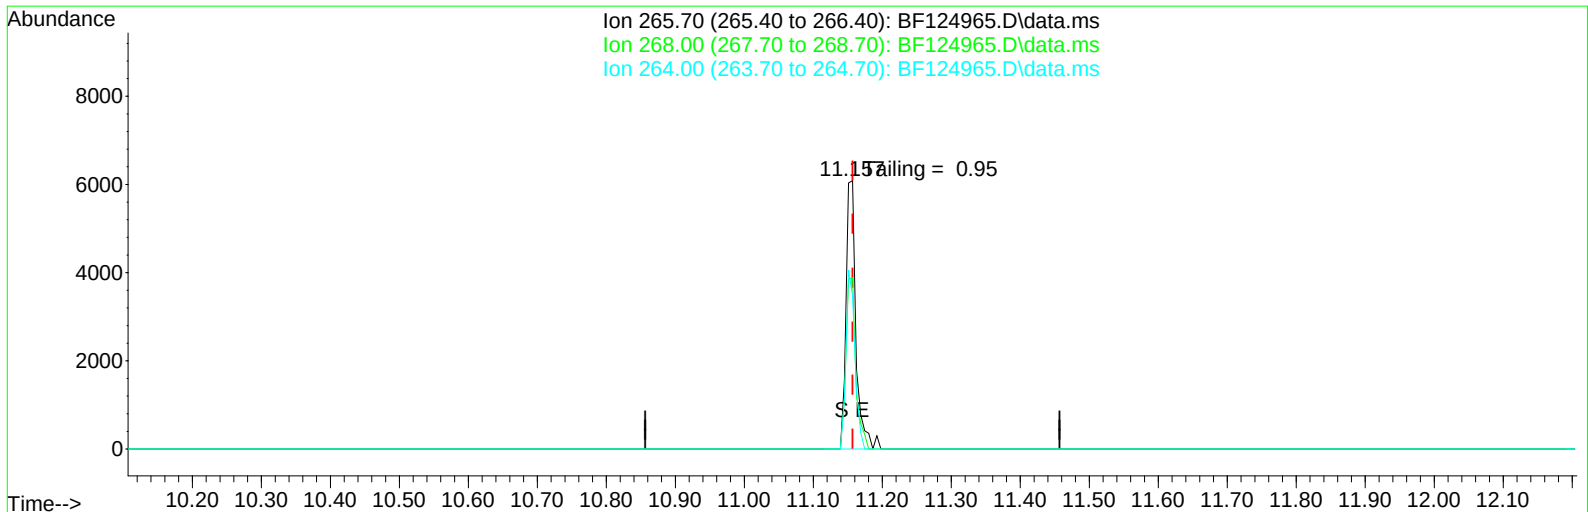

TIC: BF124965.D\data.ms

(70) Pentachlorophenol (C)

11.157min (+ 0.000) 0.00 ng

response 6115

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	63.86
264.00	69.90	57.17
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/7/2021	BNA_F	<u>BF124965.D</u>
Compound Name	Response	Retention Time
DDT	23073	13.51
DDD	0	13.3
DDE	0	12.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
0	23073	0.00

Instrument :
BNA_F
ClientSampleId :
DFTPP