
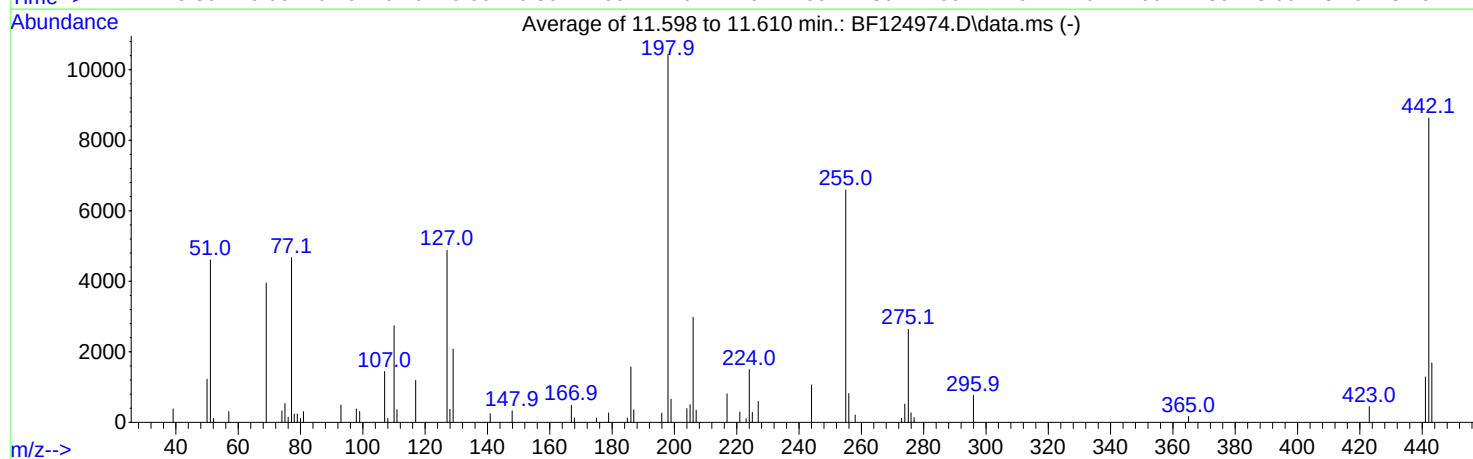


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080721\
 Data File : BF124974.D
 Acq On : 7 Aug 2021 14:49
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 09 11:03:44 2021

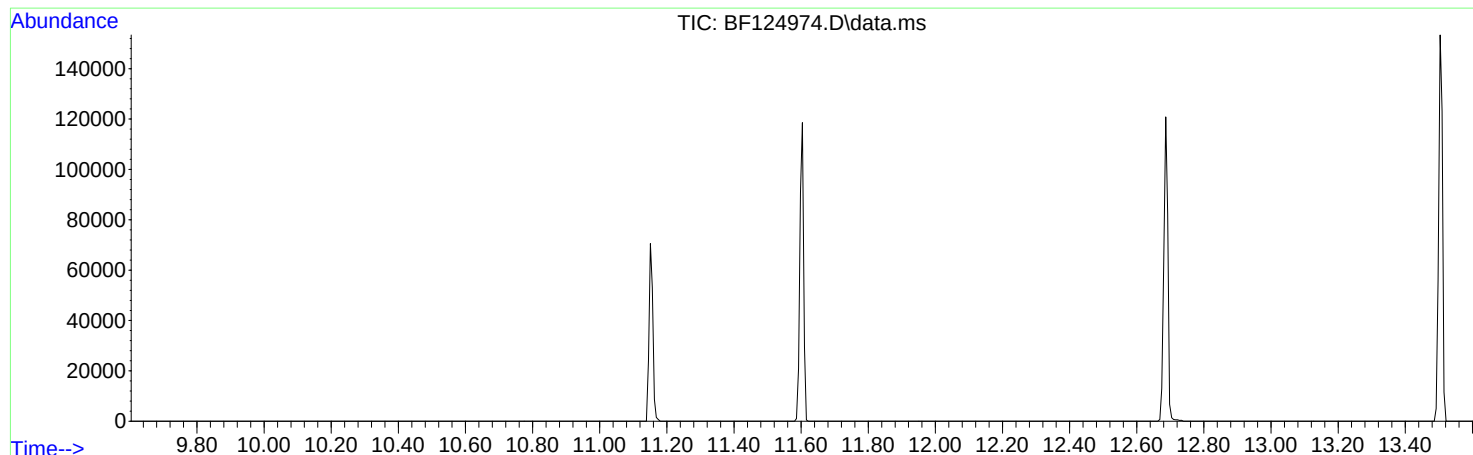




AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.2	4606	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.9	3954	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.8	4880	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	10430	PASS
199	198	5	9	6.3	656	PASS
275	198	10	60	25.3	2641	PASS
365	198	1	100	1.6	166	PASS
441	198	0.01	100	12.4	1290	PASS
442	442	50	100	100.0	8629	PASS
443	442	15	24	19.6	1689	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080721\
 Data File : BF124974.D
 Acq On : 7 Aug 2021 14:49
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 07 16:01:36 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 06 11:27:24 2021
 Response via : Initial Calibration

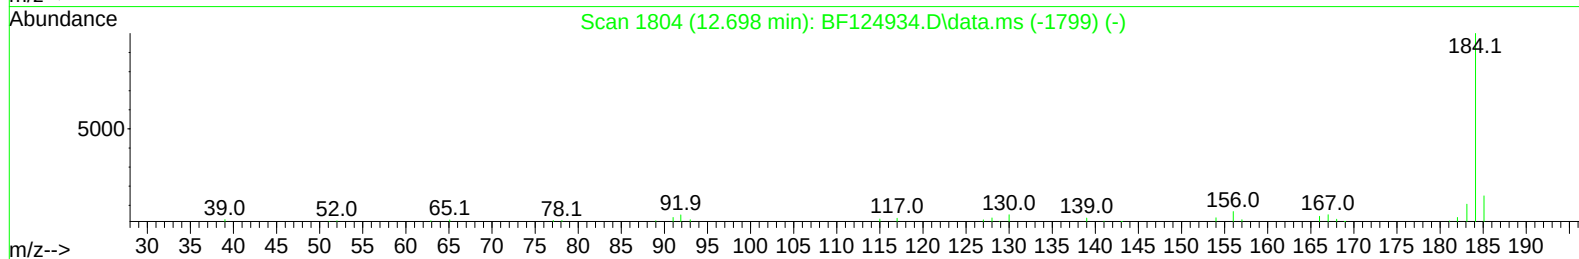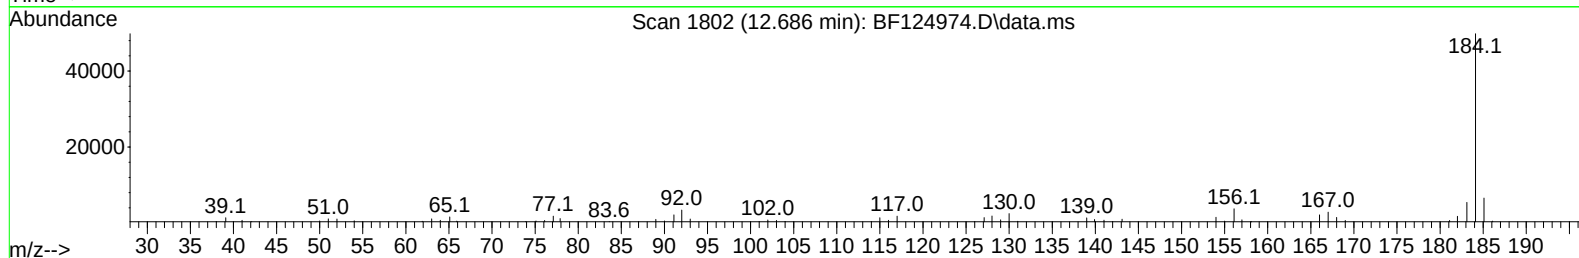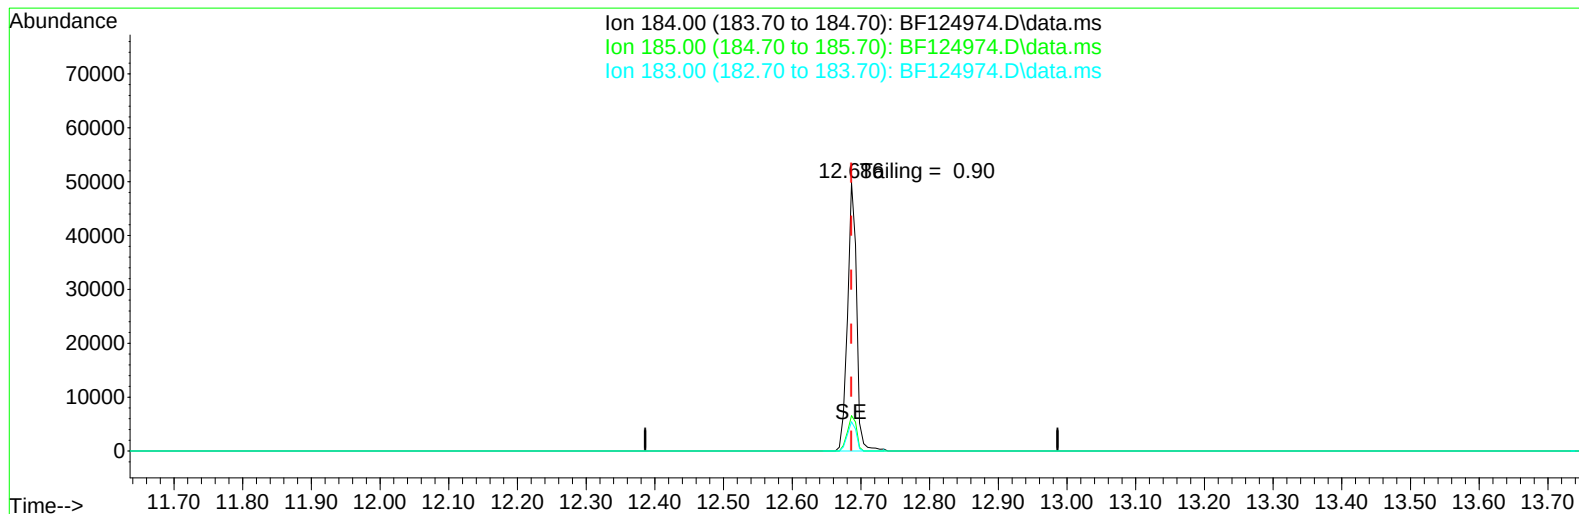

TIC: BF124974.D\data.ms

(77) Benzidine

12.686min (+ 0.000) 0.00 ng




response 45703

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.17
183.00	10.10	10.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080721\
 Data File : BF124974.D
 Acq On : 7 Aug 2021 14:49
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 07 16:01:36 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 06 11:27:24 2021
 Response via : Initial Calibration

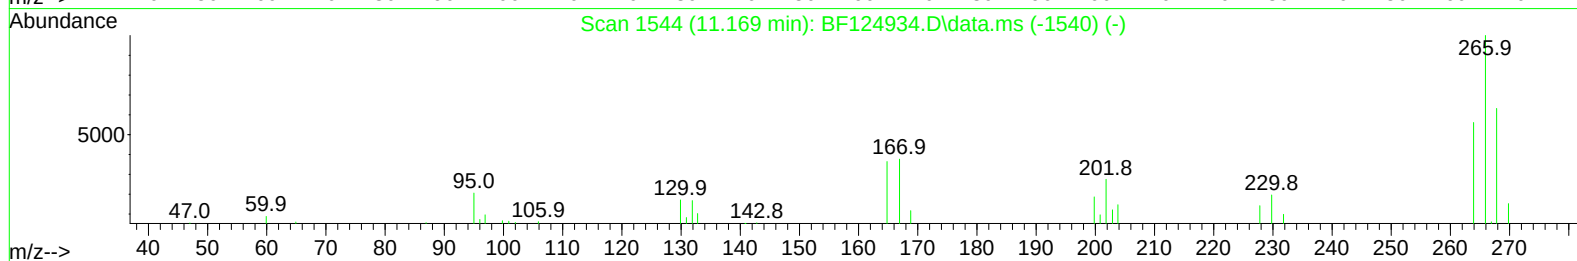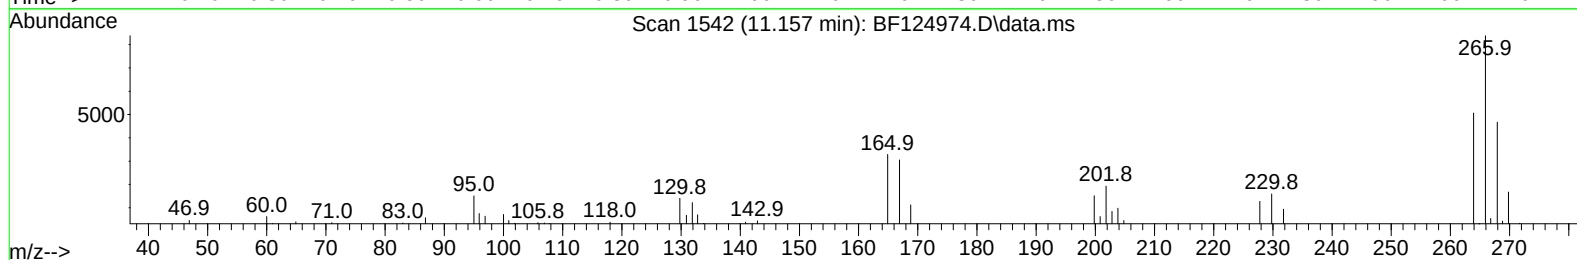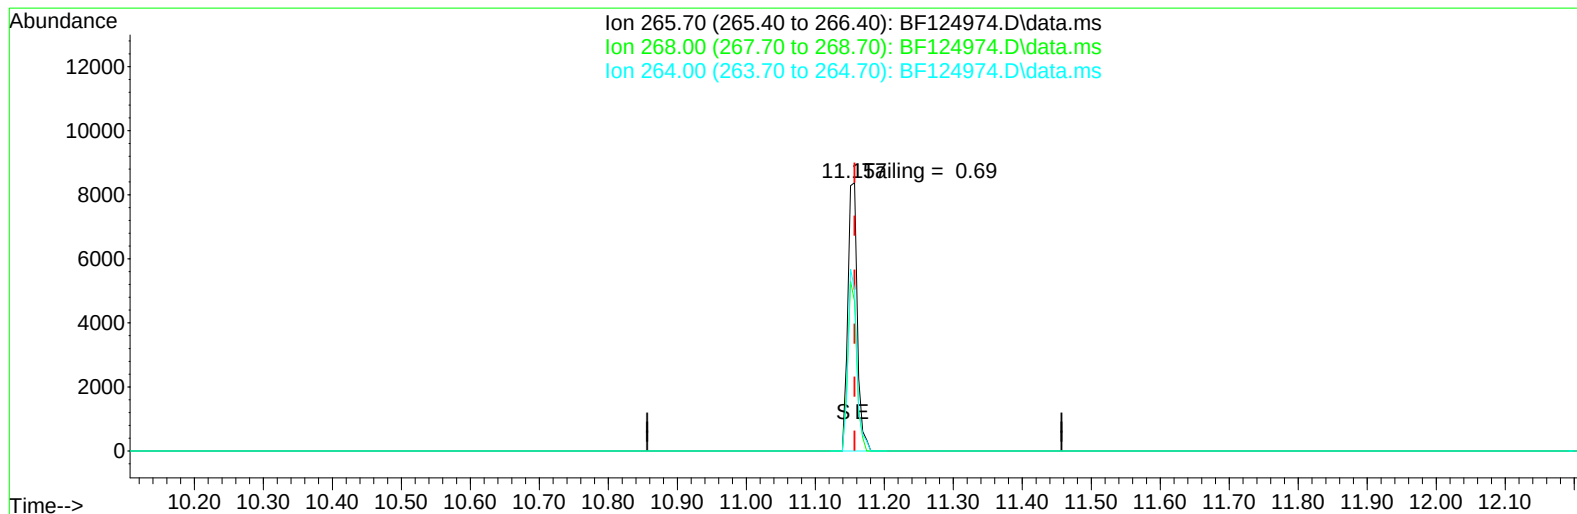

TIC: BF124974.D\data.ms

(70) Pentachlorophenol (C)

11.157min (+ 0.000) 0.00 ng

response 8043

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	55.75
264.00	69.90	60.41
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/7/2021	BNA_F	<u>BF124974.D</u>
Compound Name	Response	Retention Time
DDT	25605	13.51
DDD	0	13.25
DDE	0	12.7
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
0	25605	0.00

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP