

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080724\
Data File : BF138842.D
Acq On : 07 Aug 2024 15:04
Operator : RC/JU
Sample : P3450-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
923-K1-WP0-0.25-080124

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138842.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.134	3	7	16	rVB	1394080	2063758	100.00%	21.122%
2	5.057	500	504	518	rVB	21937	31933	1.55%	0.327%
3	5.469	569	574	593	rBV	432198	573720	27.80%	5.872%
4	6.481	741	746	766	rVB	266469	367062	17.79%	3.757%
5	6.839	802	807	812	rBV	226319	278269	13.48%	2.848%
6	7.404	897	903	908	rBV	672311	897914	43.51%	9.190%
7	8.116	1019	1024	1038	rBV	286253	373094	18.08%	3.818%
8	8.434	1073	1078	1088	rBV	33325	52731	2.56%	0.540%
9	9.192	1201	1207	1212	rBV	1288837	1645918	79.75%	16.845%
10	9.869	1317	1322	1331	rVB	335192	416932	20.20%	4.267%
11	10.251	1383	1387	1391	rBV	22982	29243	1.42%	0.299%
12	10.663	1452	1457	1472	rBV	689427	895893	43.41%	9.169%
13	11.357	1570	1575	1580	rBV	316242	386268	18.72%	3.953%
14	12.939	1838	1844	1849	rBV	990772	1250427	60.59%	12.798%
15	13.468	1926	1934	1942	rBV	22600	33058	1.60%	0.338%
16	13.845	1993	1998	2011	rBV2	13465	34560	1.67%	0.354%
17	13.998	2019	2024	2030	rVB	164465	213873	10.36%	2.189%
18	15.457	2266	2272	2280	rBV	149566	226054	10.95%	2.314%




Sum of corrected areas: 9770707

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080724\
Data File : BF138842.D
Acq On : 07 Aug 2024 15:04
Operator : RC/JU
Sample : P3450-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
923-K1-WP0-0.25-080124

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

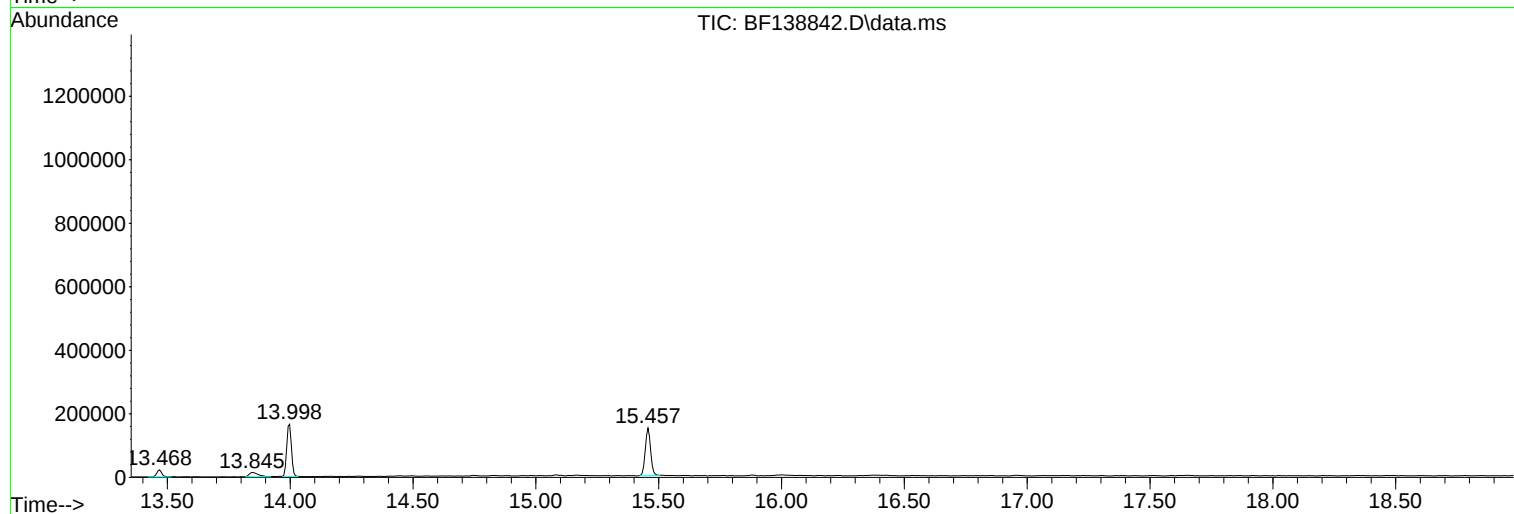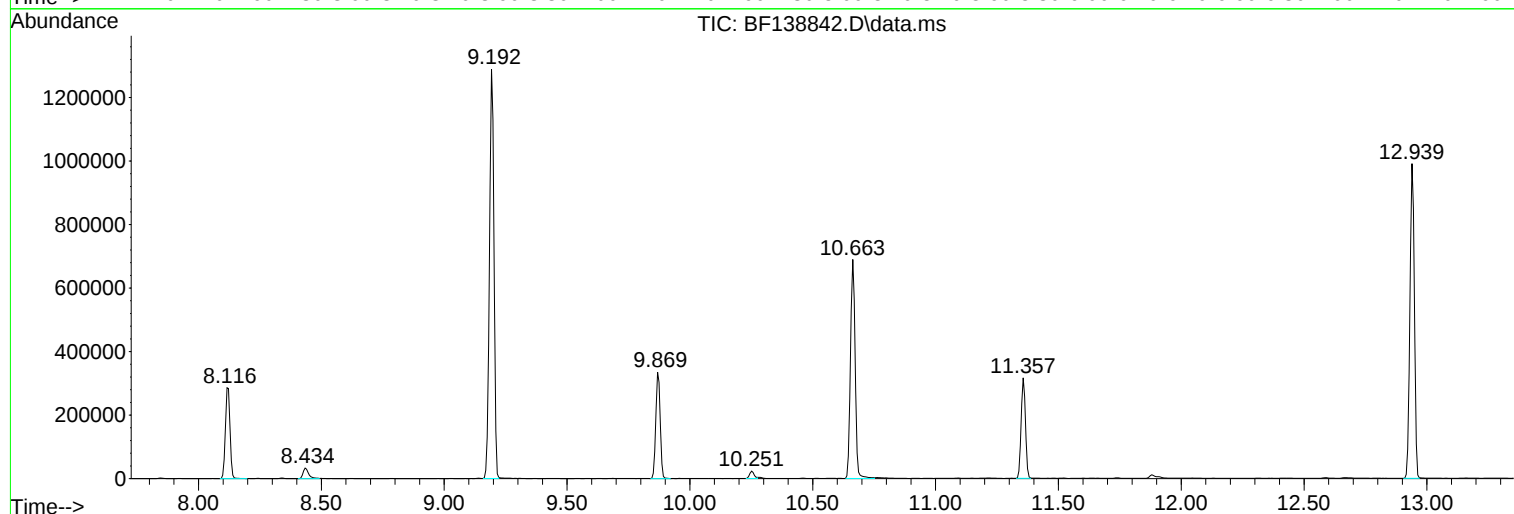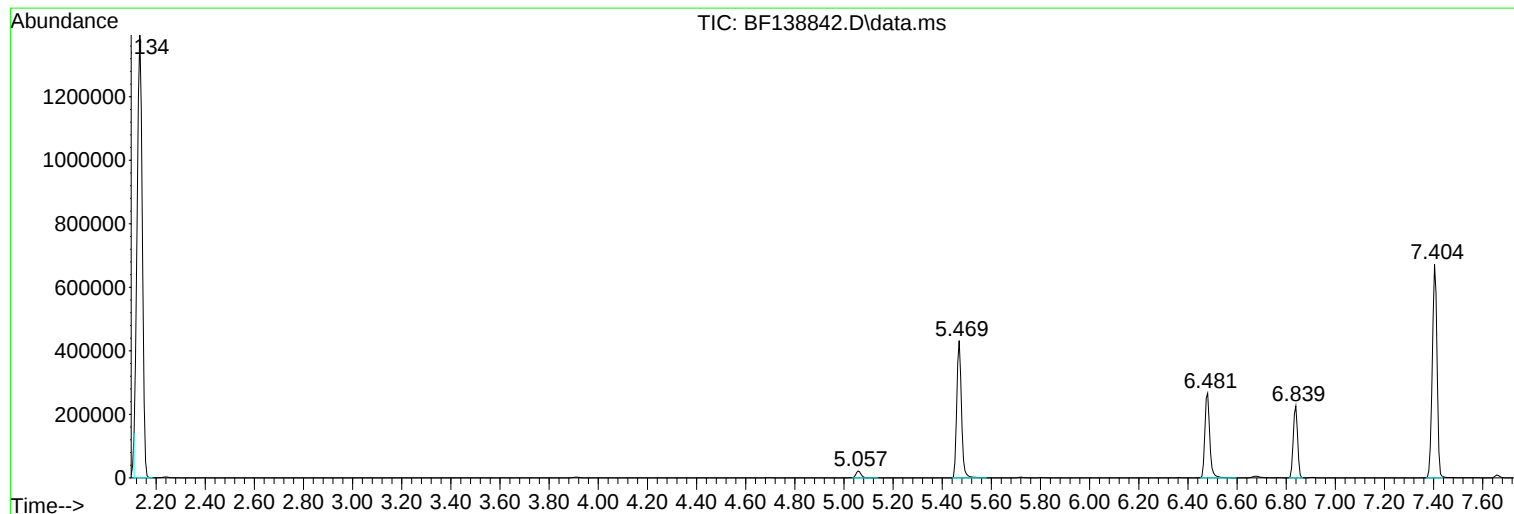

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080724\
Data File : BF138842.D
Acq On : 07 Aug 2024 15:04
Operator : RC/JU
Sample : P3450-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
923-K1-WP0-0.25-080124

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080724\
Data File : BF138842.D
Acq On : 07 Aug 2024 15:04
Operator : RC/JU
Sample : P3450-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
923-K1-WP0-0.25-080124

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------