
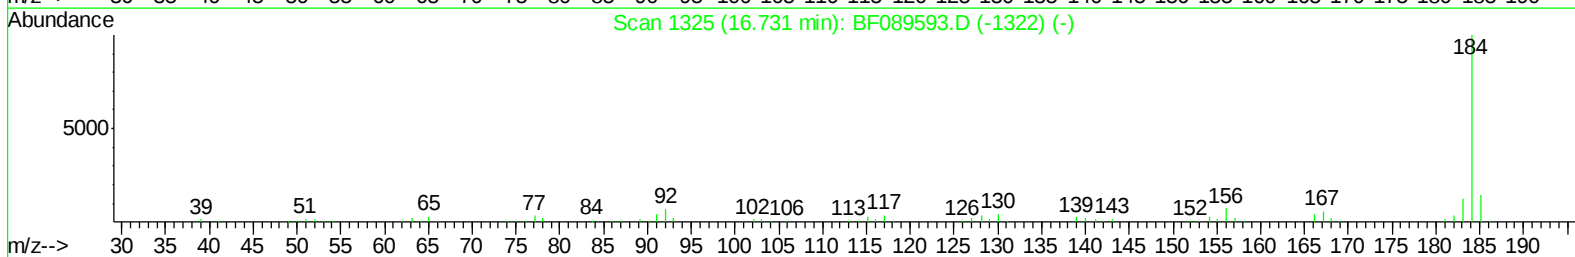
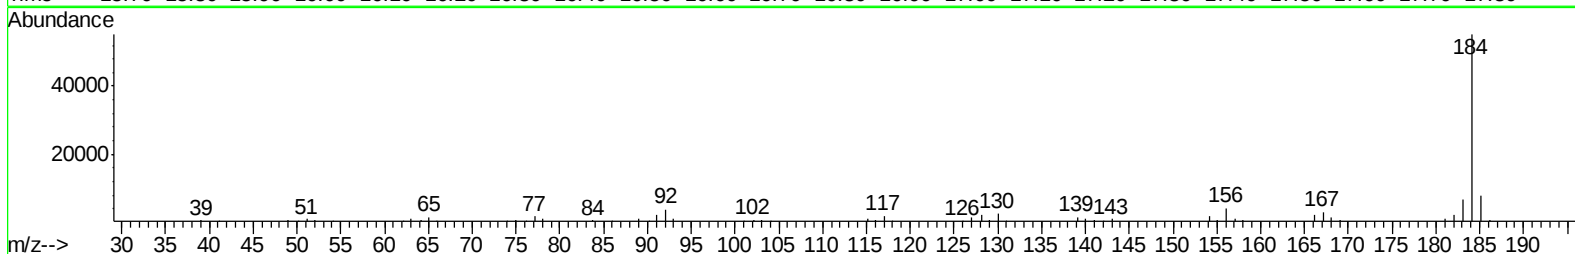


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080816\
Data File : BF089658.D
Acq On : 8 Aug 2016 12:37
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 08:09:07 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 05 01:39:23 2016
Response via : Initial Calibration

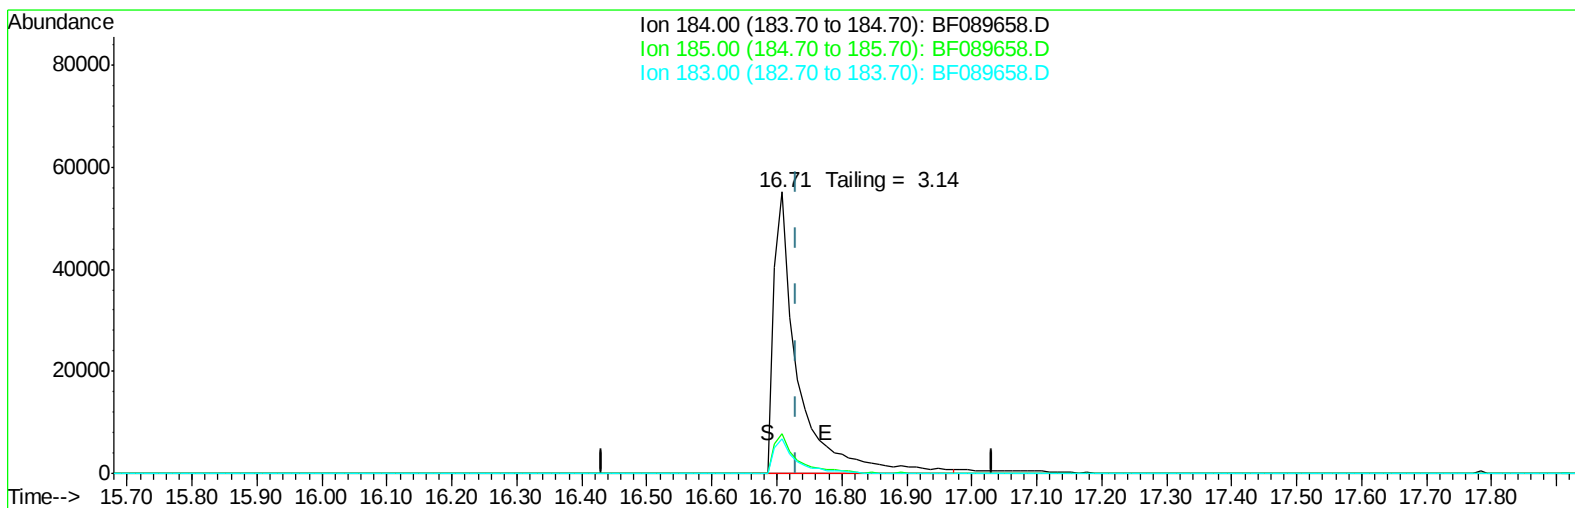

TIC: BF089658.D

(76) Benzidine




16.708min (-0.023) 0.00ng

response 141162

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.14
183.00	12.30	12.17
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080816\
Data File : BF089658.D
Acq On : 8 Aug 2016 12:37
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 08:09:07 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 05 01:39:23 2016
Response via : Initial Calibration

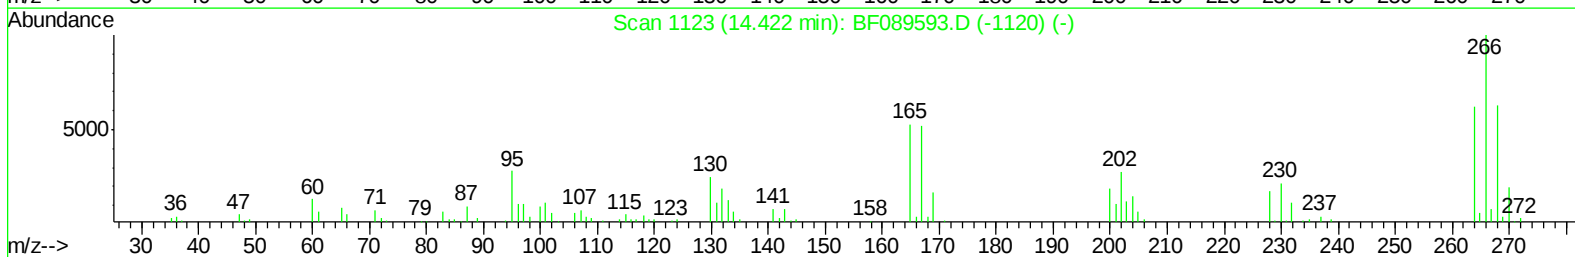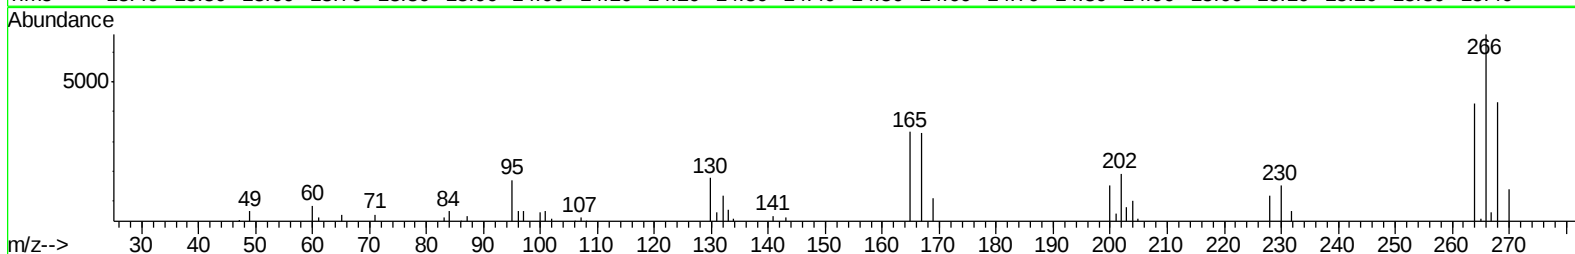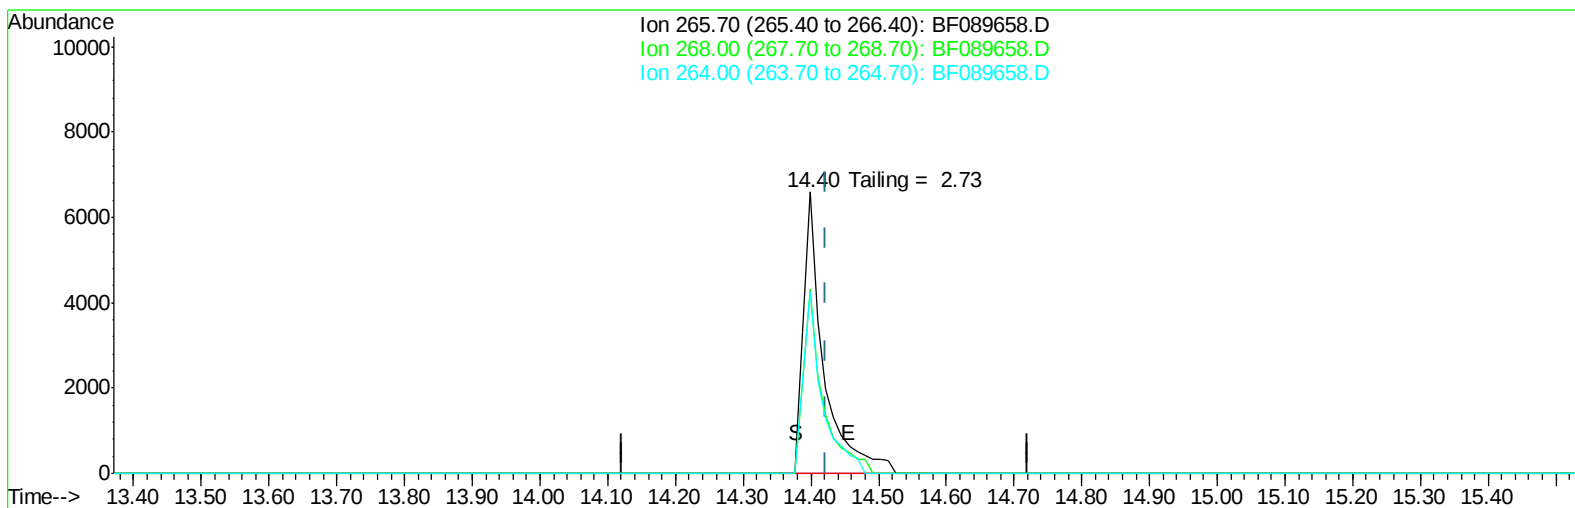

TIC: BF089658.D

(69) Pentachlorophenol (C)

14.399min (-0.023) 0.00ng m

response 13848

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	65.29
264.00	61.90	64.75
0.00	0.00	0.00