

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080816\
 Data File : BF089677.D
 Acq On : 9 Aug 2016 00:04
 Operator : UM/SJ
 Sample : H4331-11 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC1-GRAB

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.604	262	264	271	rBV	6970	15156	4.34%	0.661%
2	5.324	325	327	339	rBV	9605	38335	10.99%	1.672%
3	6.982	469	472	478	rBV	15422	44762	12.83%	1.953%
4	7.073	478	480	492	rVB	35177	82391	23.62%	3.594%
5	7.416	508	510	524	rBV	150813	225885	64.75%	9.854%
6	7.656	529	531	540	rVV	41653	65431	18.76%	2.854%
7	8.342	589	591	604	rBV	9389	32504	9.32%	1.418%
8	9.450	685	688	698	rBV	223939	321787	92.24%	14.038%
9	11.222	841	843	855	rBB	76099	92499	26.52%	4.035%
10	11.919	902	904	910	rBB	18655	23060	6.61%	1.006%
11	12.262	932	934	943	rBB	226196	348845	100.00%	15.218%
12	13.554	1046	1047	1052	rBB	15197	25228	7.23%	1.101%
13	14.422	1121	1123	1126	rBB	4866	6449	1.85%	0.281%
14	14.662	1141	1144	1152	rVB	181897	273865	78.51%	11.947%
15	15.051	1174	1178	1180	rBV2	1734	4567	1.31%	0.199%
16	15.131	1182	1185	1188	rVV2	2338	5191	1.49%	0.226%
17	15.668	1230	1232	1237	rBV4	6537	15531	4.45%	0.678%
18	15.748	1237	1239	1241	rVV2	3236	4118	1.18%	0.180%
19	16.217	1278	1280	1283	rBV4	2463	4149	1.19%	0.181%
20	16.320	1287	1289	1291	rVB3	3565	5736	1.64%	0.250%
21	16.468	1300	1302	1305	rBV4	5296	6623	1.90%	0.289%
22	16.777	1326	1329	1332	rBV	10971	21996	6.31%	0.960%
23	17.028	1348	1351	1353	rBV	52212	71459	20.48%	3.117%
24	18.366	1465	1468	1474	rBV	177161	281760	80.77%	12.292%
25	20.023	1611	1613	1620	rVB	201801	274959	78.82%	11.995%


Sum of corrected areas: 2292286

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080816\
Data File : BF089677.D
Acq On : 9 Aug 2016 00:04
Operator : UM/SJ
Sample : H4331-11 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC1-GRAB

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

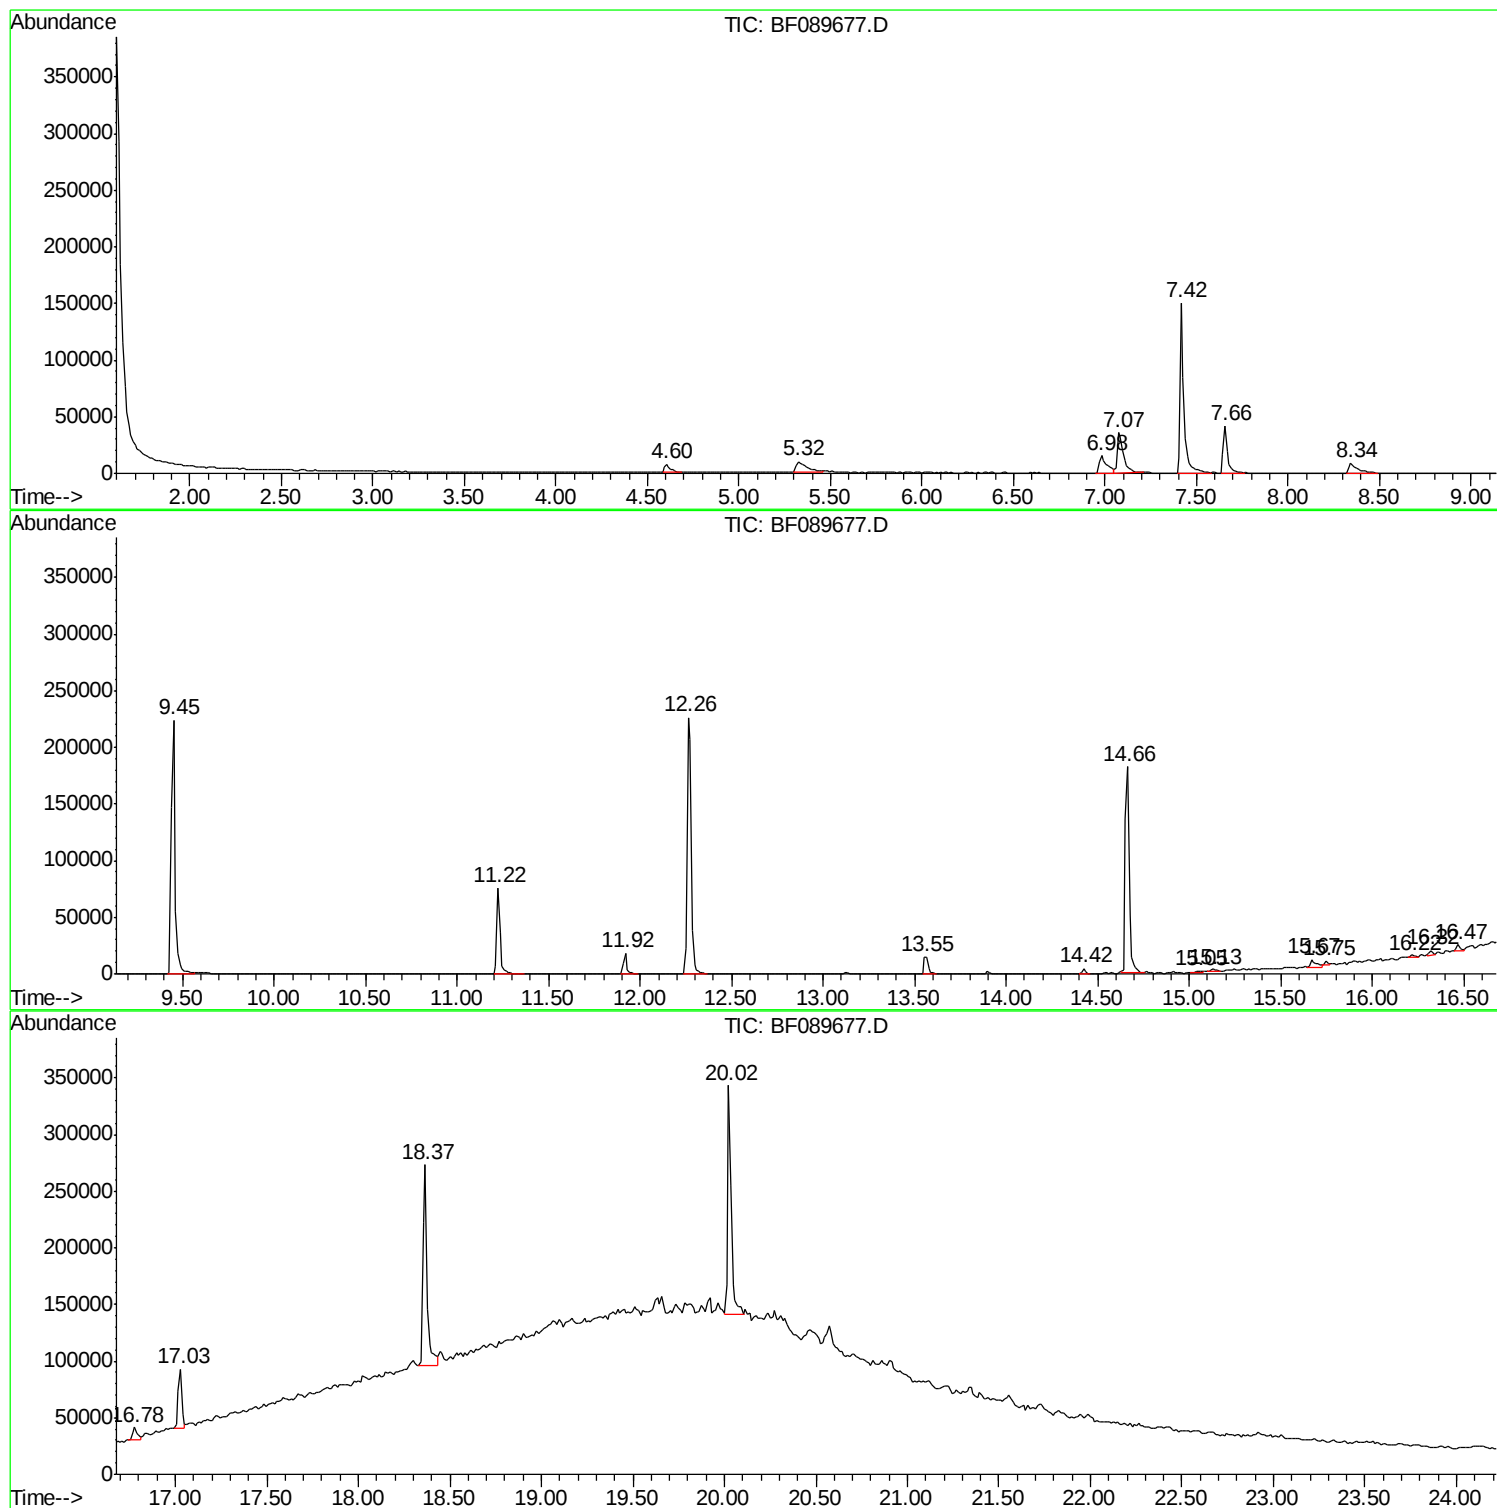

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080816\
Data File : BF089677.D
Acq On : 9 Aug 2016 00:04
Operator : UM/SJ
Sample : H4331-11 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC1-GRAB










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.07 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.07	7.29 ng	82391	1,4-Dichlorobenzene-d4	7.42

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
2		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
3		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	9

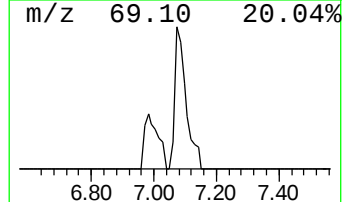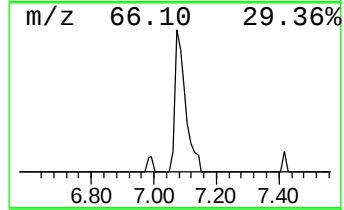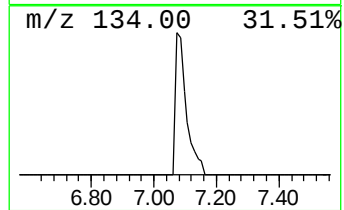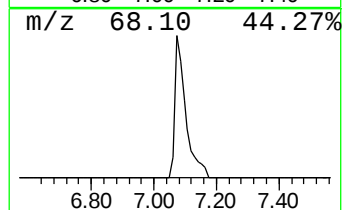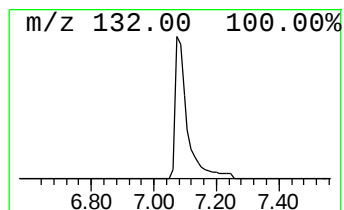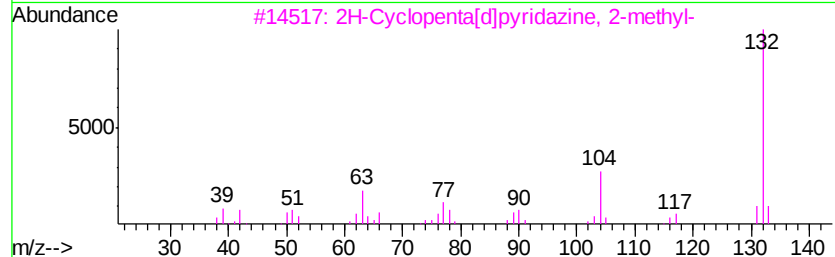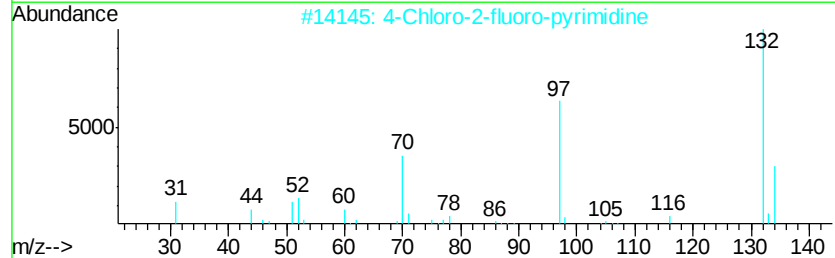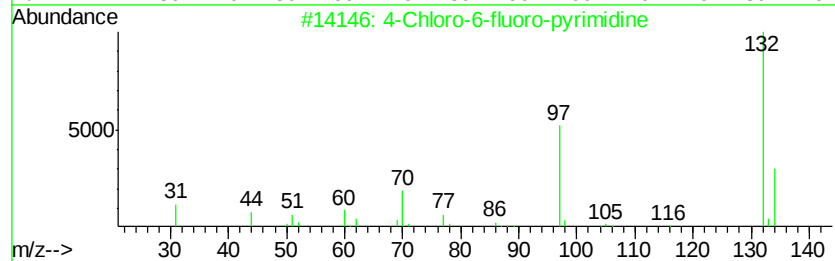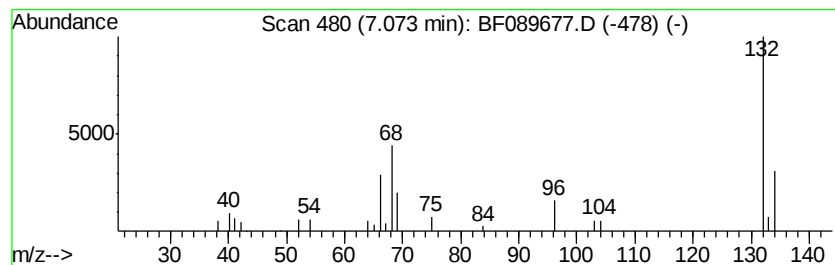

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080816\
Data File : BF089677.D
Acq On : 9 Aug 2016 00:04
Operator : UM/SJ
Sample : H4331-11 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC1-GRAB

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.07	7.07	7.3	ng	82391	1	7.42	225885	20.0