


Data Path : Z:\HPCHEM1\BNA_F\Data\BF080816\
Data File : BF089658.D
Acq On : 8 Aug 2016 12:37
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080416.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 05 01:39:23 2016

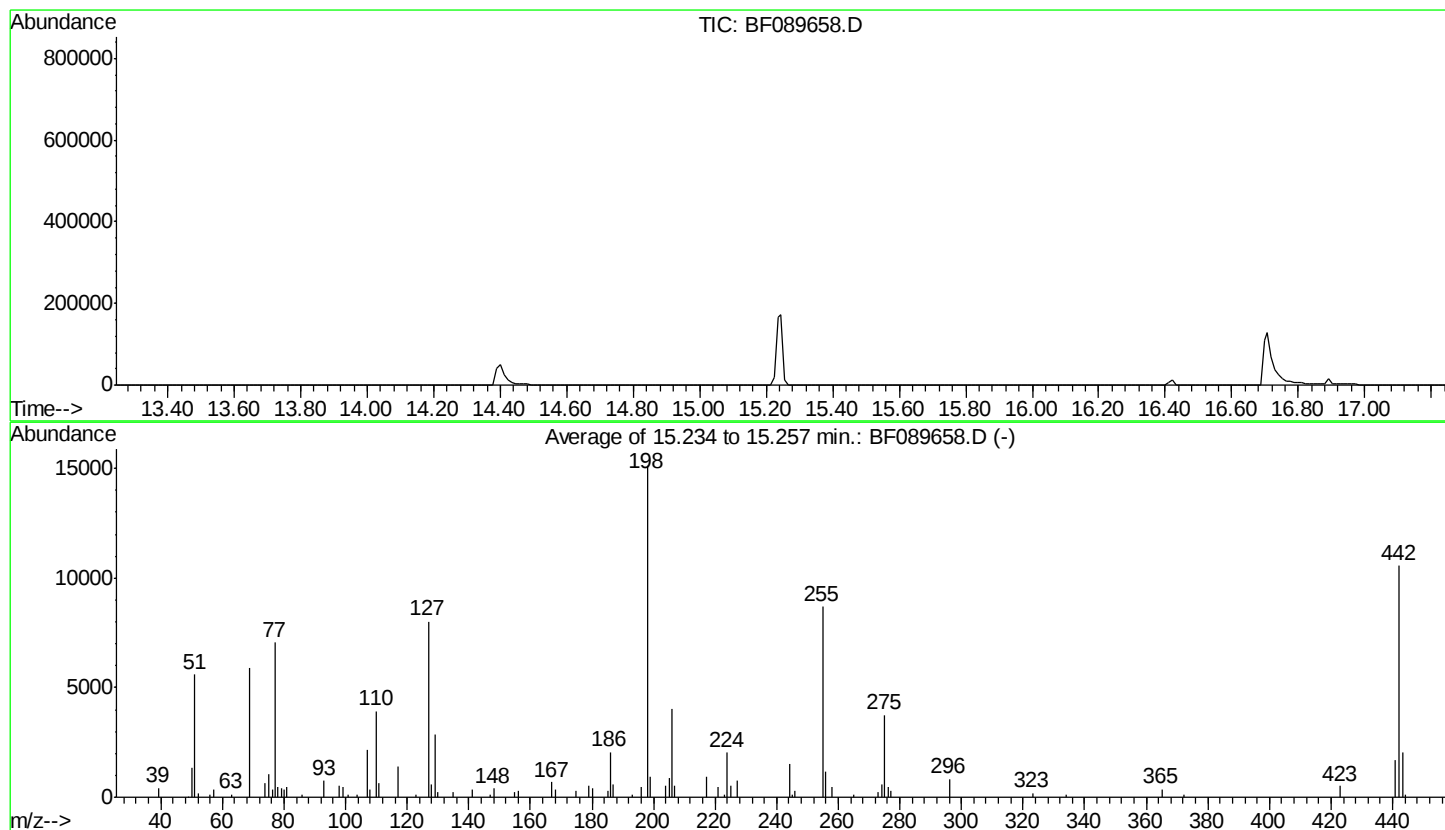

AutoFind: Scans 1194, 1195, 1196; Background Corrected with Scan 1190

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	5599	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.0	5893	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.9	8001	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	15127	PASS
199	198	5	9	6.3	954	PASS
275	198	10	60	24.8	3750	PASS
365	198	1	100	2.4	366	PASS
441	442	0.01	24	16.0	1685	PASS
442	198	50	100	69.8	10563	PASS
443	442	15	24	19.1	2020	PASS