


Data Path : Z:\HPCHEM1\BNA_F\Data\BF080816\
 Data File : BF089678.D
 Acq On : 9 Aug 2016 2:19
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 05 01:39:23 2016

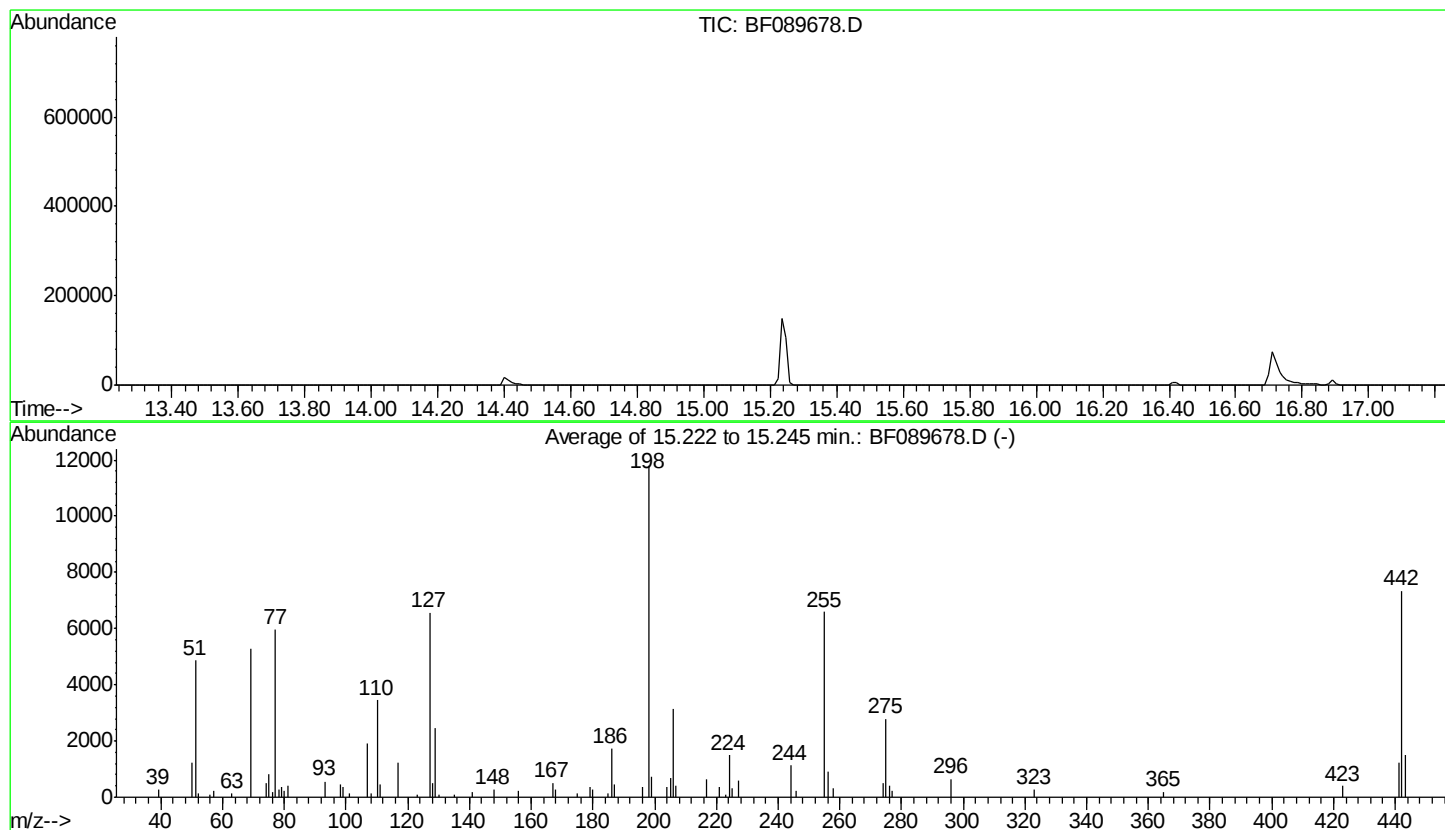

AutoFind: Scans 1193, 1194, 1195; Background Corrected with Scan 1190

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	4855	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	44.7	5273	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.6	6564	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	11796	PASS
199	198	5	9	6.2	732	PASS
275	198	10	60	23.6	2779	PASS
365	198	1	100	1.7	196	PASS
441	442	0.01	24	16.8	1232	PASS
442	198	50	100	62.3	7354	PASS
443	442	15	24	20.2	1483	PASS