

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080817\
 Data File : BF097494.D
 Acq On : 9 Aug 2017 3:15
 Operator : SJ/JU
 Sample : I4652-02 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP8N-WC1

Quant Time: Aug 09 04:49:47 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 07 16:02:51 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.40	152	75794	20.00	ng	0.00
21) Naphthalene-d8	7.69	136	290504	20.00	ng	-0.01
38) Acenaphthene-d10	9.43	164	106853	20.00	ng	0.00
63) Phenanthrene-d10	10.90	188	171518	20.00	ng	-0.01
75) Chrysene-d12	13.53	240	175634	20.00	ng	0.00
86) Perylene-d12	14.87	264	123249	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.01	112	82446	16.40	ng	0.00
7) Phenol-d6	6.09	99	96538	16.82	ng	0.00
23) Nitrobenzene-d5	6.99	82	44492	8.98	ng	0.00
41) 2,4,6-Tribromophenol	10.23	330	13223	15.66	ng	0.00
44) 2-Fluorobiphenyl	8.77	172	74807	11.88	ng	0.00
78) Terphenyl-d14	12.49	244	54841	6.37	ng	-0.01
Target Compounds						
25) Isophorone	6.99	82	44492	4.59	ng	# 67
49) Dimethylphthalate	9.17	163	19307	2.38	ng	98
50) 2,6-Dinitrotoluene	9.43	165	12952	7.53	ng	# 33
56) 2,4-Dinitrotoluene	9.43	165	12952	6.55	ng	# 32

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080817\
Data File : BF097494.D
Acq On : 9 Aug 2017 3:15
Operator : SJ/JU
Sample : I4652-02 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP8N-WC1

Quant Time: Aug 09 04:49:47 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 07 16:02:51 2017
Response via : Initial Calibration

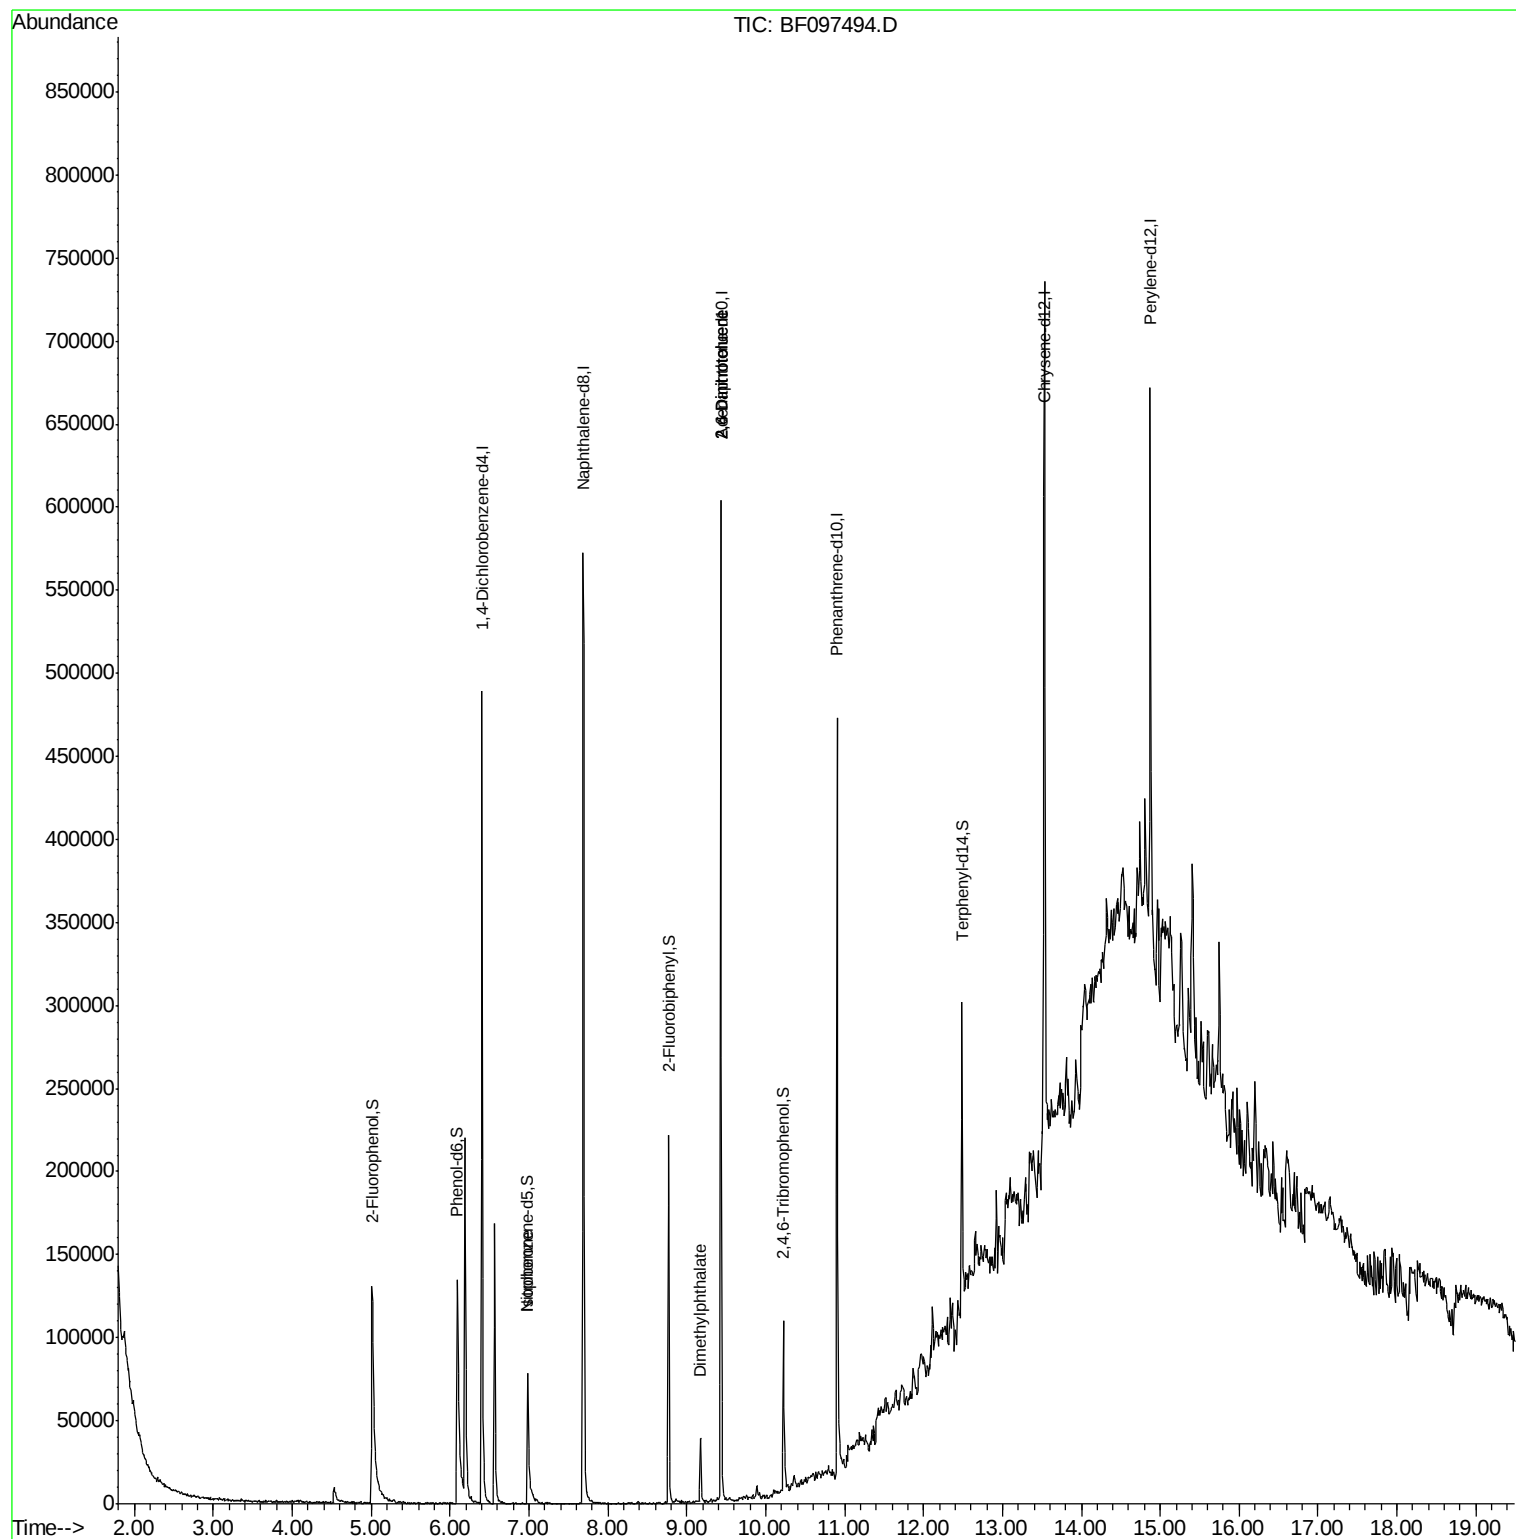







#1

1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.40 min Scan# 785
 Delta R.T. -0.01 min
 Lab File: BF097494.D
 Acq: 9 Aug 2017 3:15

Instrument :
 BNA_F
 ClientSampleId :
 TP8N-WC1




Tot Ion:152 Resp: 75794
 Ion Ratio Lower Upper
 152 100
 150 155.5 126.2 189.2
 115 64.8 52.2 78.2

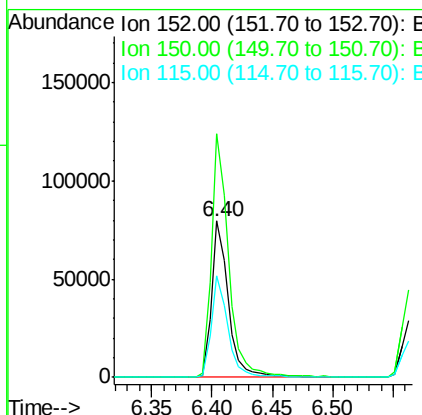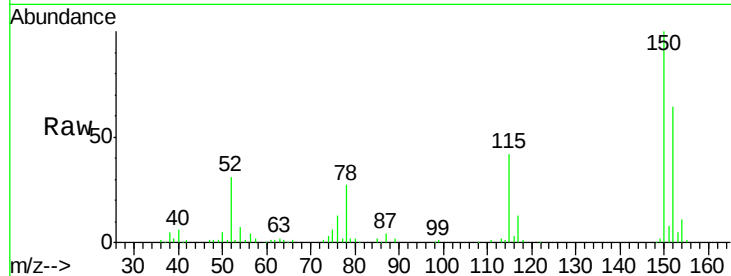


#5

2-Fluorophenol
 Concen: 16.40 ng
 RT: 5.01 min Scan# 548
 Delta R.T. 0.01 min
 Lab File: BF097494.D
 Acq: 9 Aug 2017 3:15

Tgt Ion:112 Resp: 82446
 Ion Ratio Lower Upper
 112 100
 64 63.4 46.0 69.0
 63 32.0 23.4 35.0

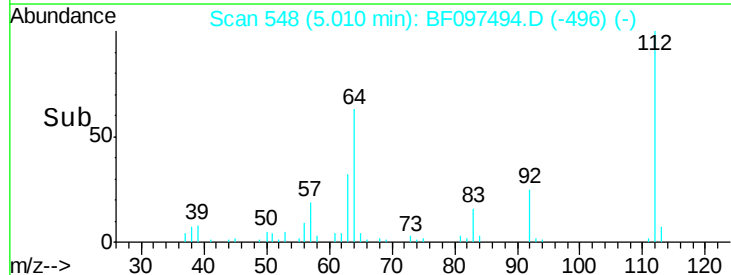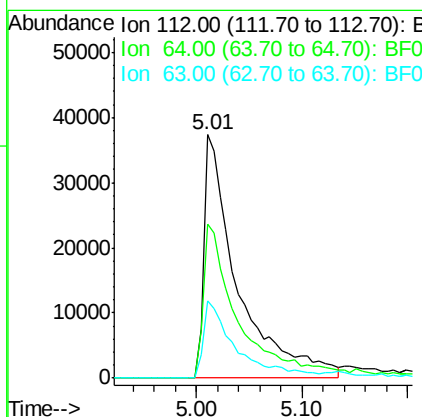

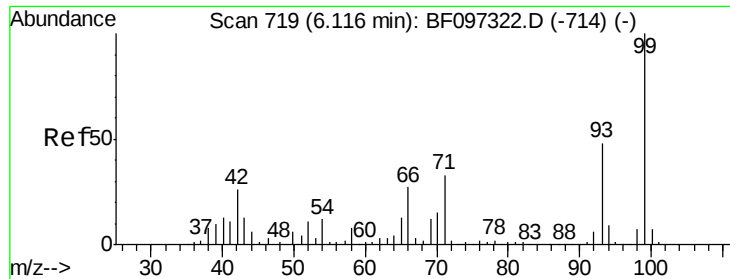

#7

Phenol-d6

Concen: 16.82 ng

RT: 6.09 min Scan# 732

Delta R.T. 0.01 min

Lab File: BF097494.D

Acq: 9 Aug 2017 3:15

Instrument :

BNA_F

ClientSampleId :

TP8N-WC1


Tot Ion: 99 Resp: 96538

Ion Ratio Lower Upper

99 100

42 23.6 13.5 20.3#




71 30.5 24.5 36.7

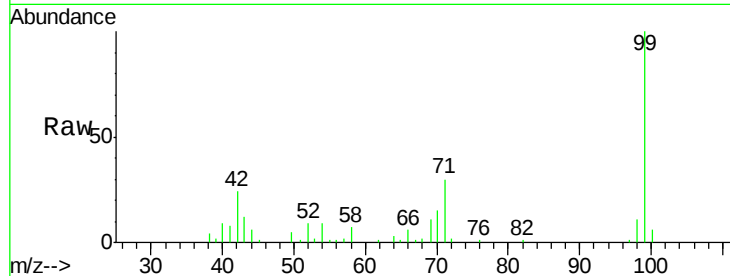

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

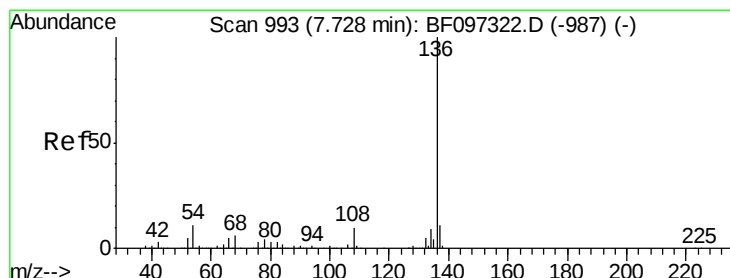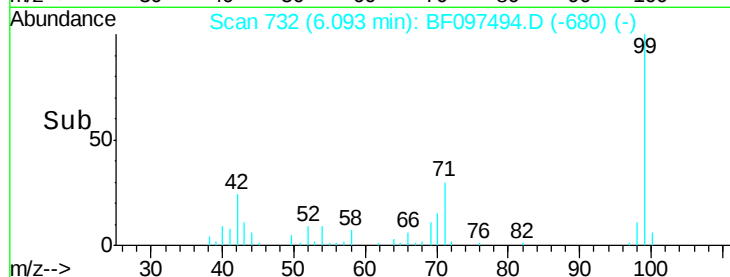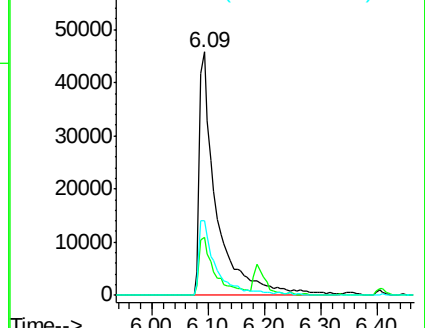

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.69 min Scan# 1003

Delta R.T. -0.01 min

Lab File: BF097494.D

Acq: 9 Aug 2017 3:15

Tgt Ion: 136 Resp: 290504


Ion Ratio Lower Upper

136 100

137 10.6 8.5 12.7

54 11.3 4.9 7.3#

68 6.0 4.1 6.1


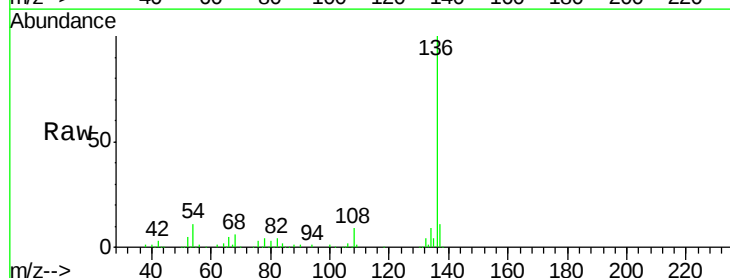



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



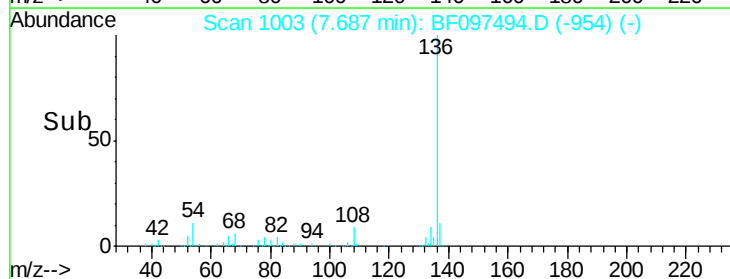
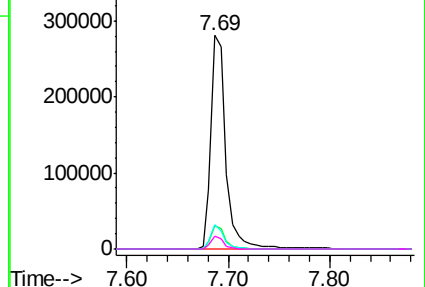


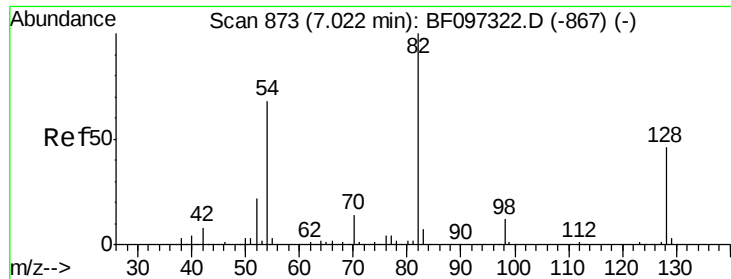

#23
 Nitrobenzene-d5
 Concen: 8.98 ng
 RT: 6.99 min Scan# 884
 Delta R.T. -0.01 min
 Lab File: BF097494.D
 Acq: 9 Aug 2017 3:15




Instrument :
 BNA_F
 ClientSampleId :
 TP8N-WC1


Tot Ion: 82 Resp: 44492
 Ion Ratio Lower Upper
 82 100
 128 44.8 34.0 51.0
 54 64.8 42.2 63.2#

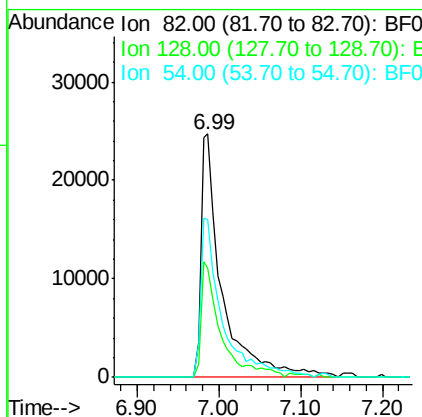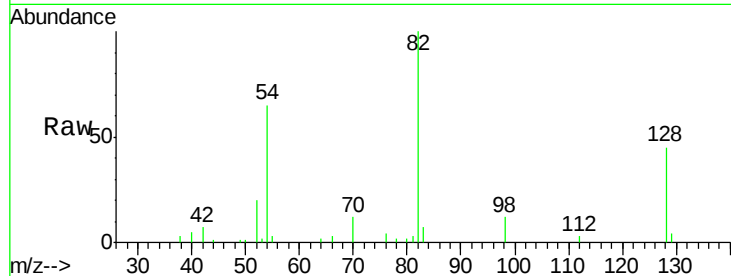

#25
 Isophorone
 Concen: 4.59 ng
 RT: 6.99 min Scan# 884
 Delta R.T. -0.26 min
 Lab File: BF097494.D
 Acq: 9 Aug 2017 3:15

Tgt Ion: 82 Resp: 44492
 Ion Ratio Lower Upper
 82 100
 95 0.0 5.3 7.9#
 138 0.0 13.1 19.7#



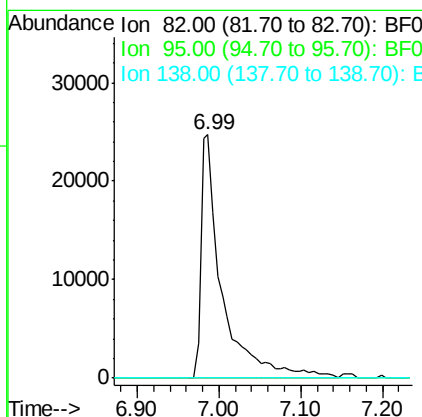



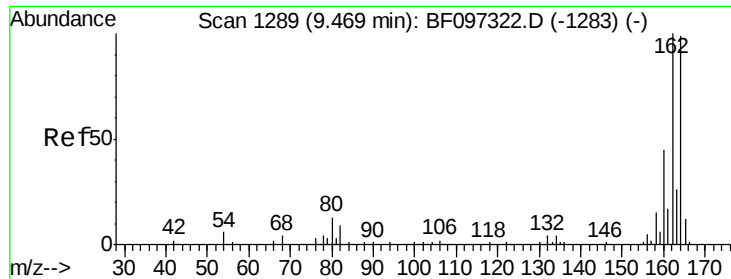

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.43 min Scan# 1300
 Delta R.T. -0.01 min
 Lab File: BF097494.D
 Acq: 9 Aug 2017 3:15




Instrument :
 BNA_F
 ClientSampleId :
 TP8N-WC1


Tot Ion:164 Resp: 106853
 Ion Ratio Lower Upper
 164 100
 162 100.9 82.6 123.8
 160 45.8 36.2 54.2

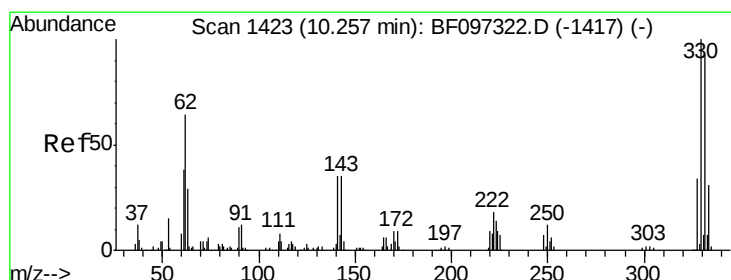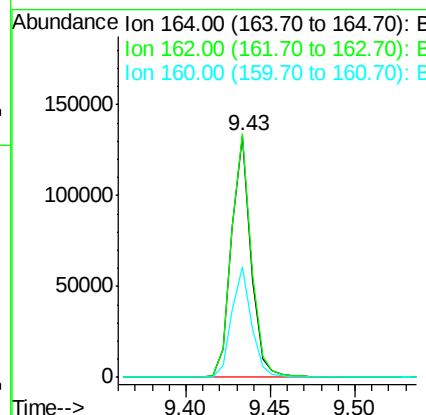

#41
 2,4,6-Tribromophenol
 Concen: 15.66 ng
 RT: 10.23 min Scan# 1435
 Delta R.T. -0.01 min
 Lab File: BF097494.D
 Acq: 9 Aug 2017 3:15

Tgt Ion:330 Resp: 13223
 Ion Ratio Lower Upper
 330 100
 332 97.2 76.6 115.0
 141 44.1 31.4 47.2

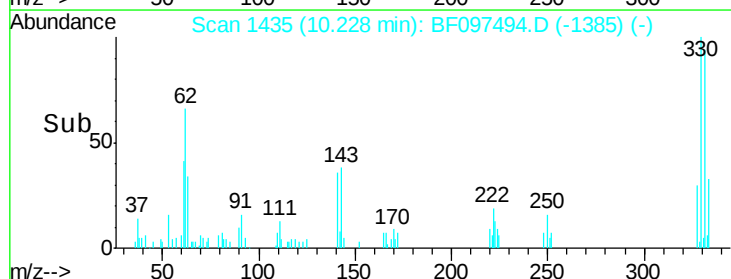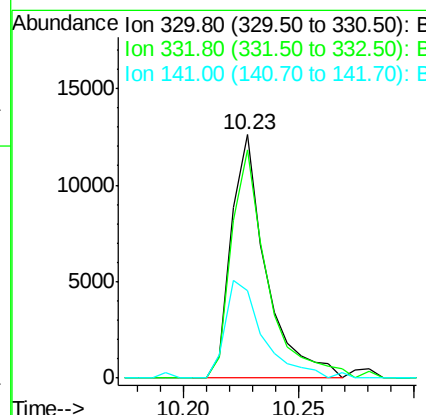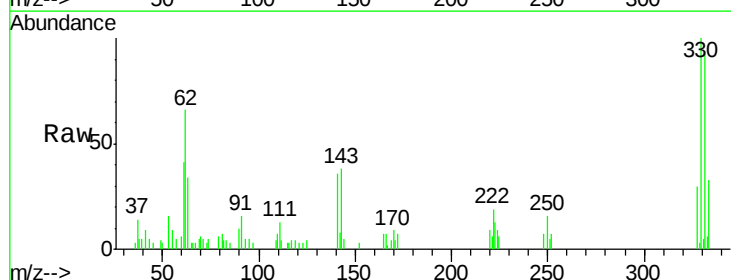

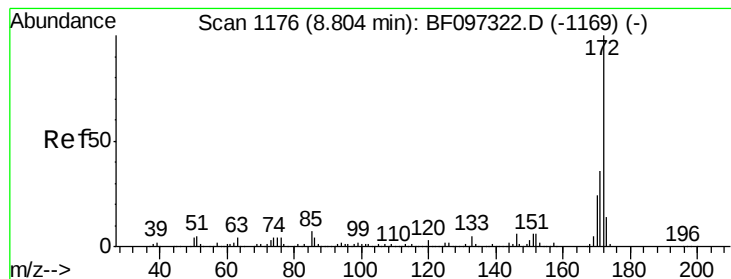

#44

2-Fluorobiphenyl

Concen: 11.88 ng

RT: 8.77 min Scan# 1187

Delta R.T. -0.01 min

Lab File: BF097494.D

Acq: 9 Aug 2017 3:15

Instrument :

BNA_F

ClientSampled :

TP8N-WC1


Tot Ion:172 Resp: 74807

Ion Ratio Lower Upper

172 100

171 33.2 29.6 44.4




170 22.9 19.8 29.8



Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

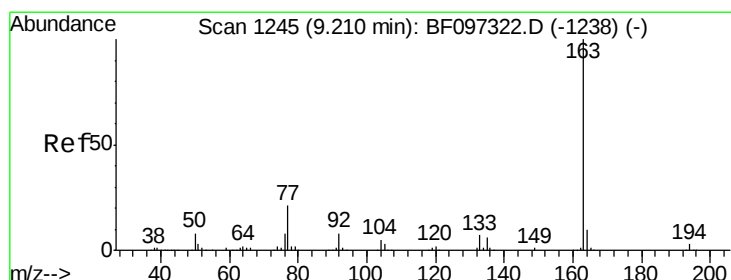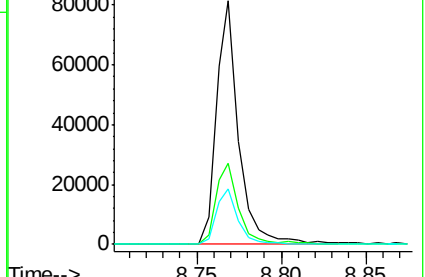

#49

Dimethylphthalate

Concen: 2.38 ng

RT: 9.17 min Scan# 1256

Delta R.T. -0.01 min

Lab File: BF097494.D

Acq: 9 Aug 2017 3:15


Tgt Ion:163 Resp: 19307

Ion Ratio Lower Upper

163 100

194 3.2 2.6 4.0



164 9.6 8.4 12.6




Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E




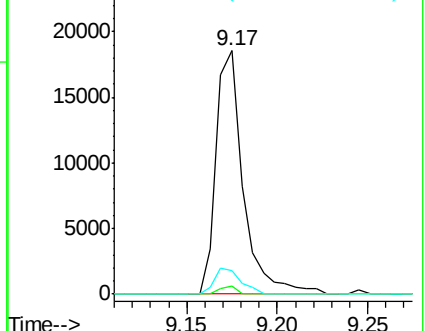


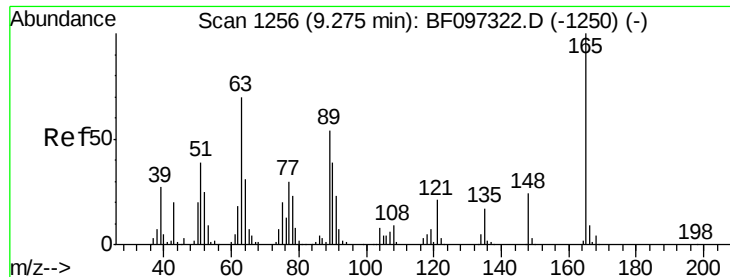

#50
 2,6-Dinitrotoluene
 Concen: 7.53 ng
 RT: 9.43 min Scan# 1300
 Delta R.T. 0.18 min
 Lab File: BF097494.D
 Acq: 9 Aug 2017 3:15




Instrument :
 BNA_F
 ClientSampleId :
 TP8N-WC1


Tot Ion	Ratio	Lower	Upper
165	100		
63	2.3	34.3	51.5#
89	0.0	37.1	55.7#

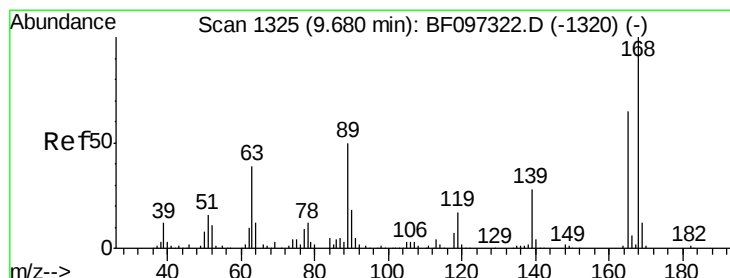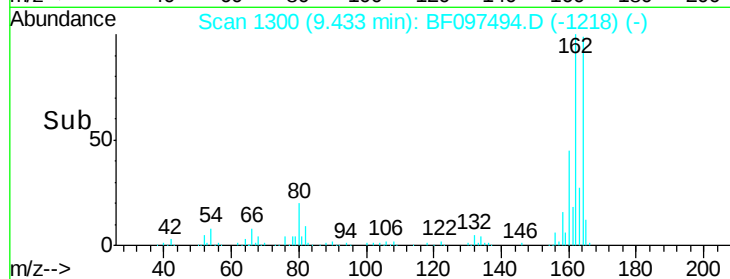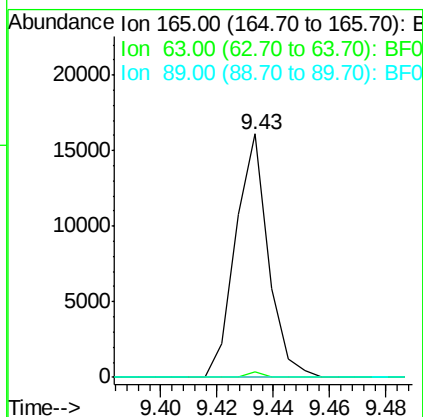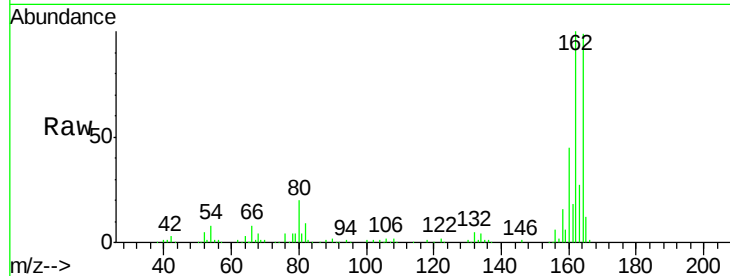

#56
 2,4-Dinitrotoluene
 Concen: 6.55 ng
 RT: 9.43 min Scan# 1300
 Delta R.T. -0.23 min
 Lab File: BF097494.D
 Acq: 9 Aug 2017 3:15

Tgt Ion	Ratio	Lower	Upper
165	100		
63	2.3	25.4	38.0#
89	0.0	46.4	69.6#
182	0.0	1.8	2.6#

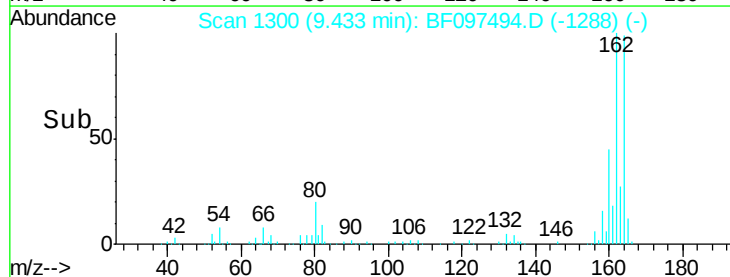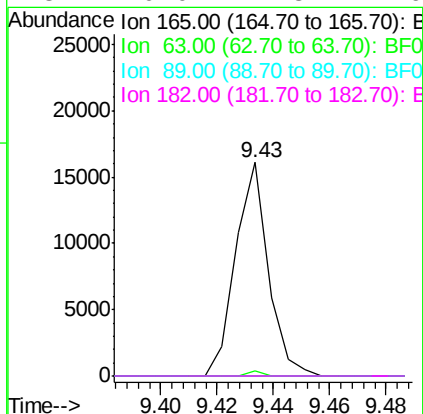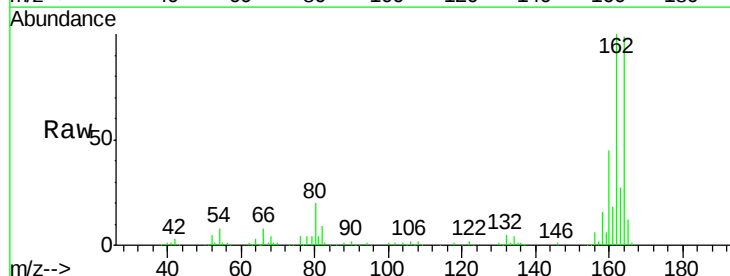


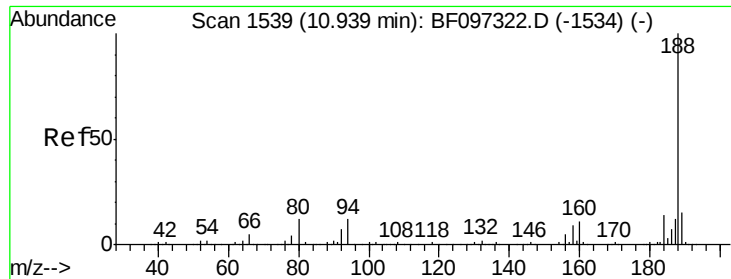




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 10.90 min Scan# 1550
Delta R.T. -0.01 min
Lab File: BF097494.D
Acq: 9 Aug 2017 3:15

Instrument :
BNA_F
ClientSampleId :
TP8N-WC1

Tot Ion:188 Resp: 171518
Ion Ratio Lower Upper
188 100
94 11.5 9.4 14.2
80 11.9 10.2 15.2




Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

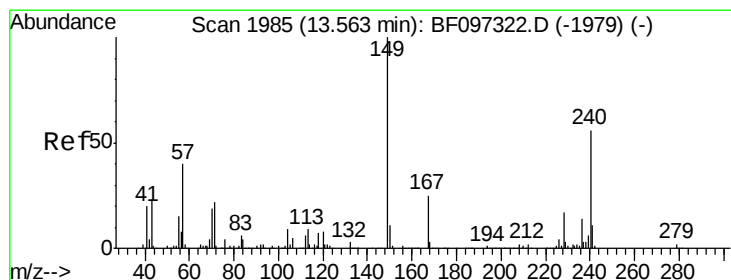
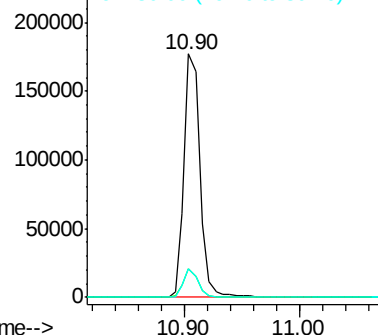



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.53 min Scan# 1997
Delta R.T. -0.01 min
Lab File: BF097494.D
Acq: 9 Aug 2017 3:15

Tgt Ion:240 Resp: 175634
Ion Ratio Lower Upper
240 100
120 15.1 5.8 8.8#
236 24.7 20.5 30.7

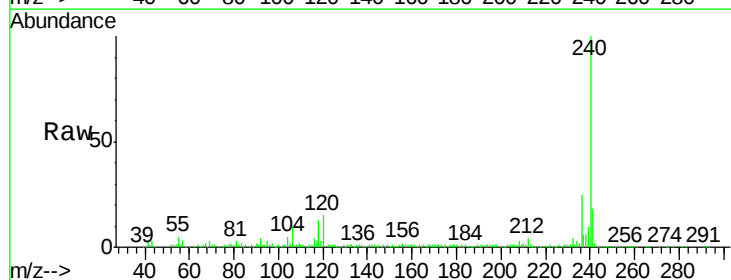

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E




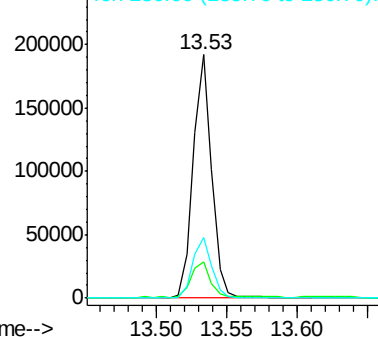




#78
 Terphenyl-d14
 Concen: 6.37 ng
 RT: 12.49 min Scan# 1819
 Delta R.T. -0.01 min
 Lab File: BF097494.D
 Acq: 9 Aug 2017 3:15

Instrument :
 BNA_F
 ClientSampleId :
 TP8N-WC1

Tot Ion:244 Resp: 54841
 Ion Ratio Lower Upper
 244 100
 212 6.8 6.0 9.0
 122 13.7 10.3 15.5

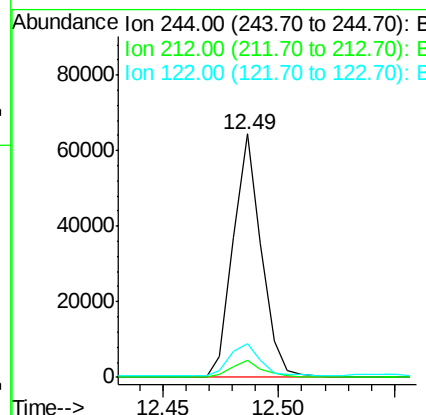

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 14.87 min Scan# 2225
 Delta R.T. 0.01 min
 Lab File: BF097494.D
 Acq: 9 Aug 2017 3:15

Tgt Ion:264 Resp: 123249
 Ion Ratio Lower Upper
 264 100
 260 23.7 19.5 29.3
 265 21.9 17.2 25.8

