
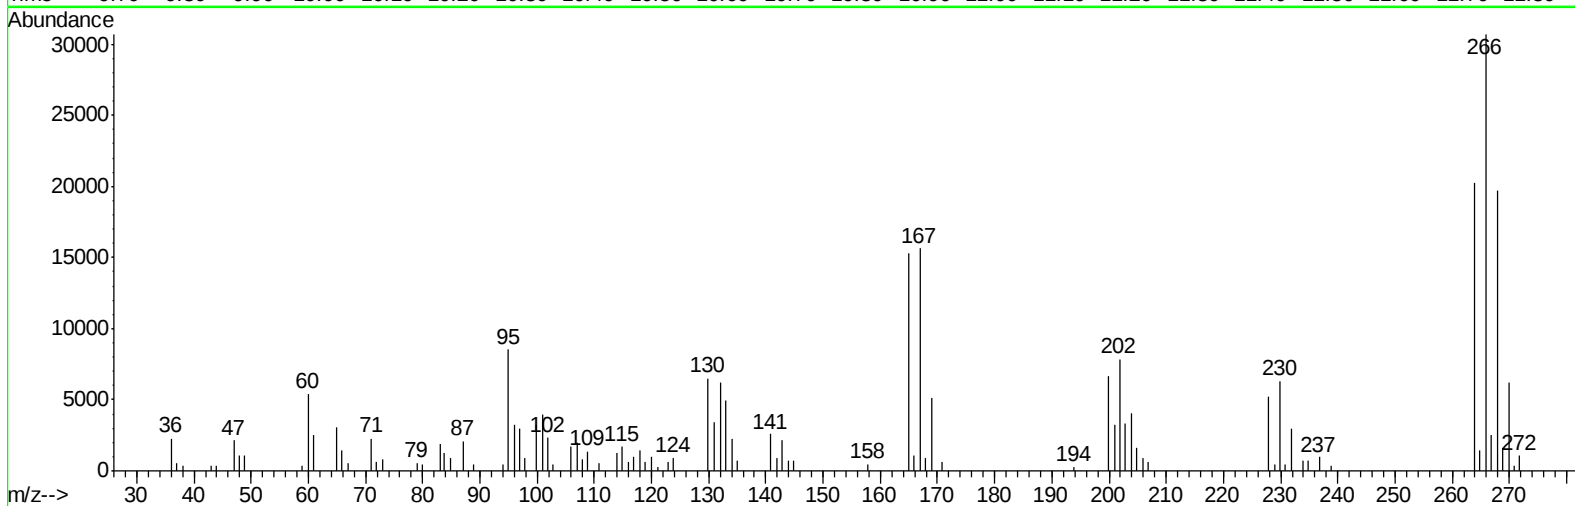


Data Path : Z:\HPCHEM1\BNA F\DATA\BF080817\
Data File : BF097475.D
Acq On : 8 Aug 2017 18:22
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 06:50:00 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 07 16:02:51 2017
Response via : Initial Calibration

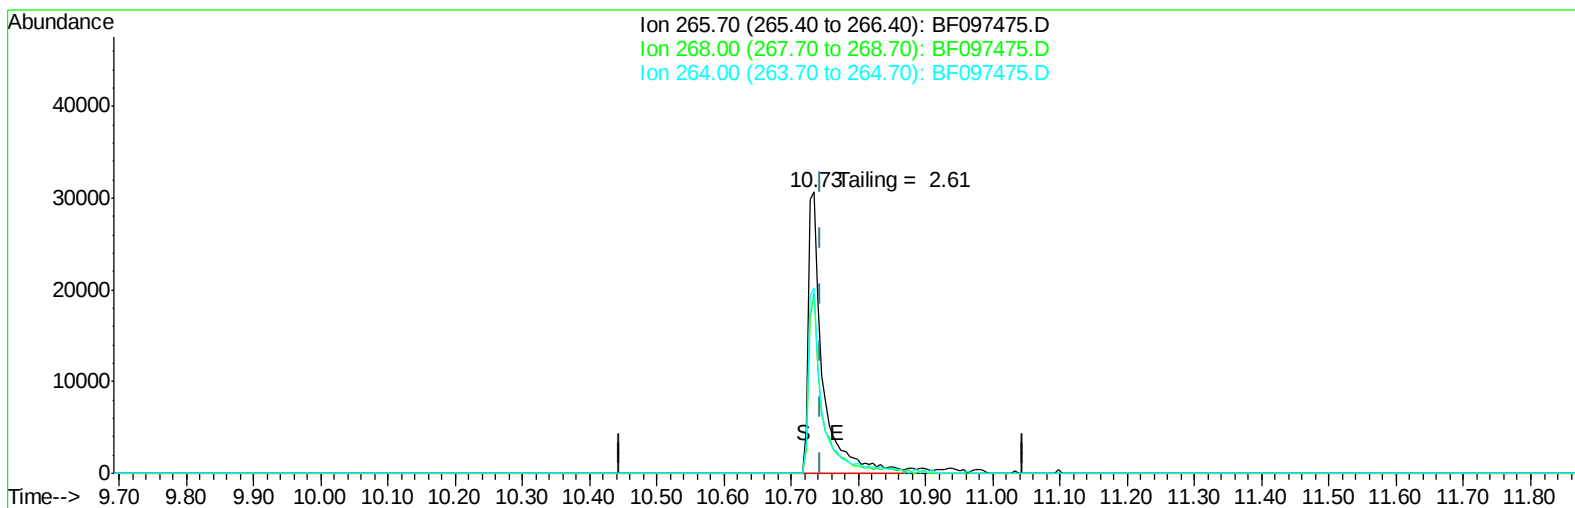

TIC: BF097475.D

(69) Pentachlorophenol (C)



10.733min (-0.012) 87444.60ng

response 47374

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.28
264.00	64.60	66.10
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080817\
Data File : BF097475.D
Acq On : 8 Aug 2017 18:22
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 06:50:00 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 07 16:02:51 2017
Response via : Initial Calibration

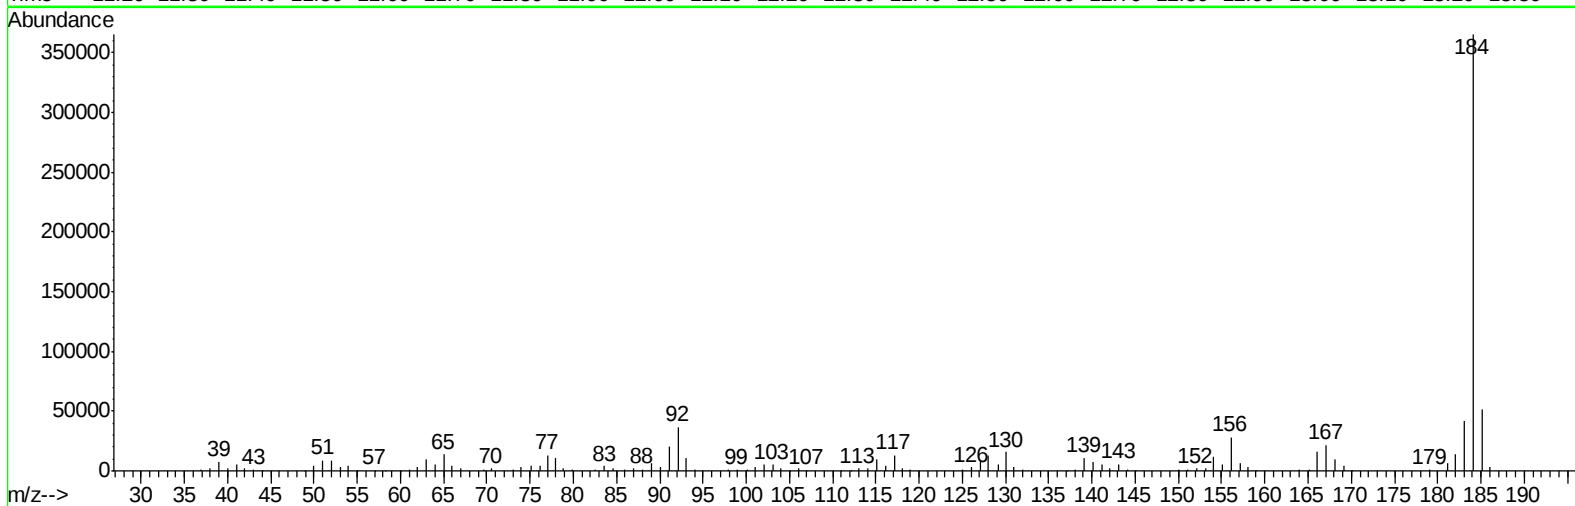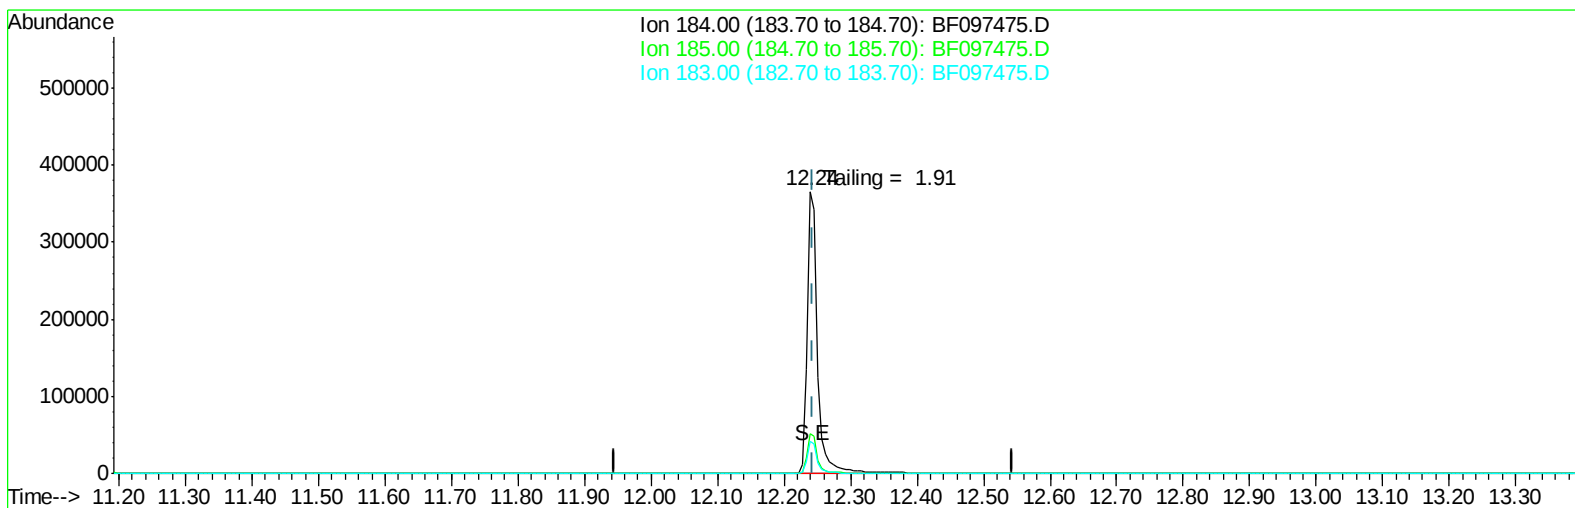

TIC: BF097475.D

(76) Benzidine

12.239min (-0.006) 0.00ng

response 397777

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.09#
183.00	12.20	11.55
0.00	0.00	0.00