

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080817\
 Data File : BF097500.D
 Acq On : 9 Aug 2017 6:02
 Operator : SJ/JU
 Sample : I4604-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-5A-080217

Quant Time: Aug 09 06:43:49 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 07 16:02:51 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.40	152	98825	20.00	ng	0.00
21) Naphthalene-d8	7.69	136	343222	20.00	ng	-0.01
38) Acenaphthene-d10	9.43	164	136485	20.00	ng	0.00
63) Phenanthrene-d10	10.90	188	212933	20.00	ng	-0.01
75) Chrysene-d12	13.53	240	157471	20.00	ng	0.00
86) Perylene-d12	14.87	264	122918	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.00	112	445851	68.01	ng	0.00
7) Phenol-d6	6.08	99	365415	48.83	ng	0.00
23) Nitrobenzene-d5	6.98	82	621054	106.15	ng	-0.01
41) 2,4,6-Tribromophenol	10.22	330	134582	124.80	ng	-0.01
44) 2-Fluorobiphenyl	8.77	172	839788	104.42	ng	0.00
78) Terphenyl-d14	12.49	244	539101	69.80	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.17	163	44414	4.285	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080817\
Data File : BF097500.D
Acq On : 9 Aug 2017 6:02
Operator : SJ/JU
Sample : I4604-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-5A-080217

Quant Time: Aug 09 06:43:49 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 07 16:02:51 2017
Response via : Initial Calibration

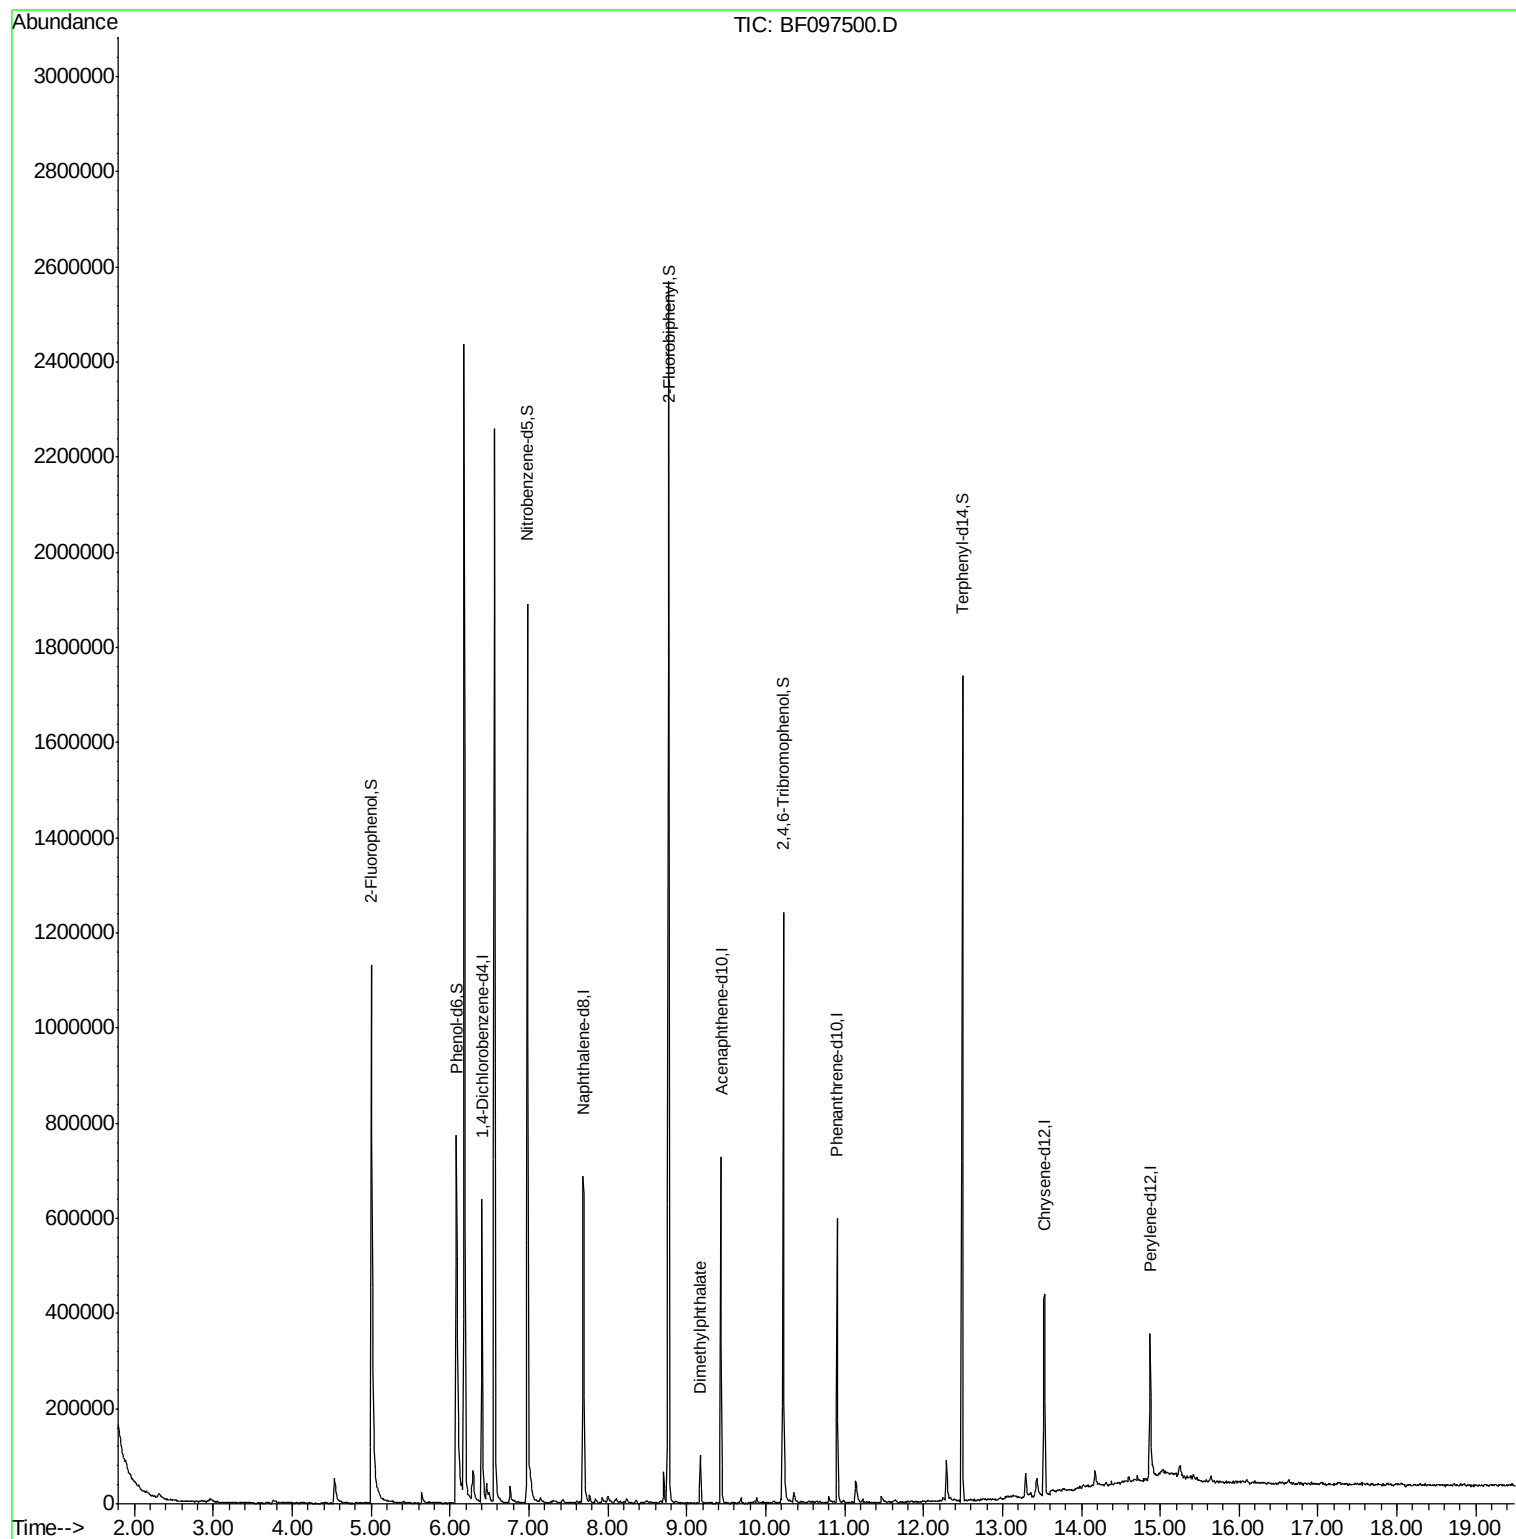

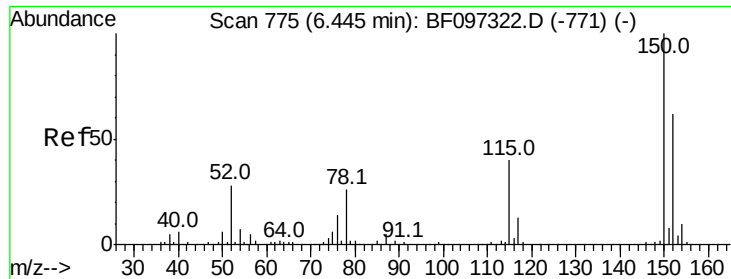


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.40 min Scan# 785
Delta R.T. -0.01 min
Lab File: BF097500.D
Acq: 9 Aug 2017 6:02

Instrument :
BNA_F
ClientSampleId :
MW-5A-080217

Tot Ion:152 Resp: 98825
Ion Ratio Lower Upper
152 100
150 158.3 126.2 189.2
115 65.7 52.2 78.2

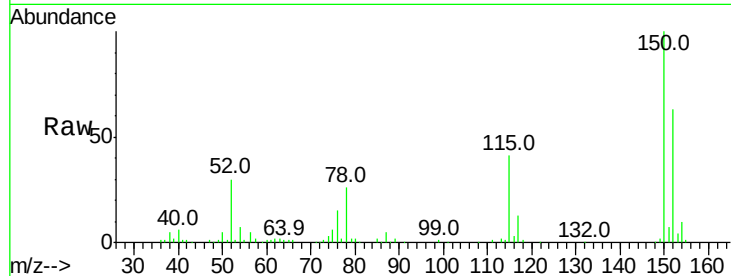


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

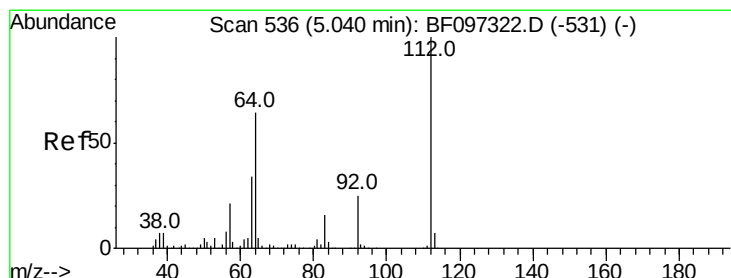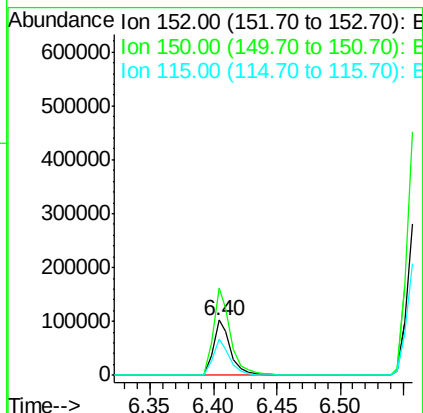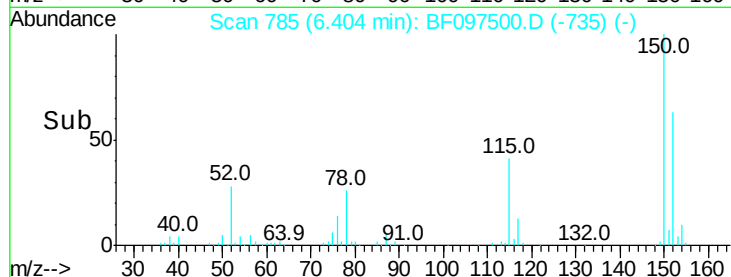



#5


2-Fluorophenol
Concen: 68.011 ng
RT: 5.00 min Scan# 547
Delta R.T. 0.00 min
Lab File: BF097500.D
Acq: 9 Aug 2017 6:02

Tgt Ion:112 Resp: 445851
Ion Ratio Lower Upper
112 100
64 65.2 46.0 69.0
63 33.0 23.4 35.0

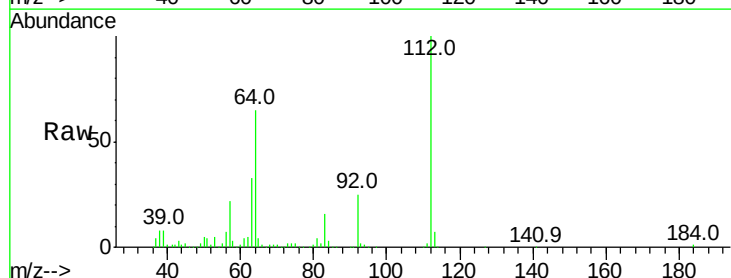

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

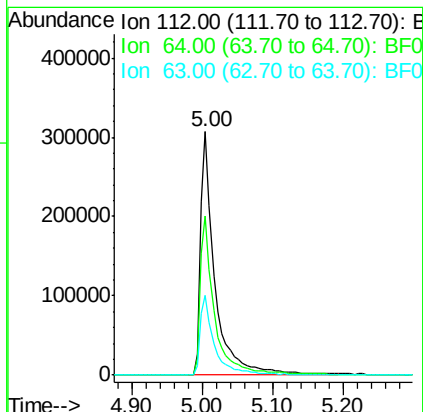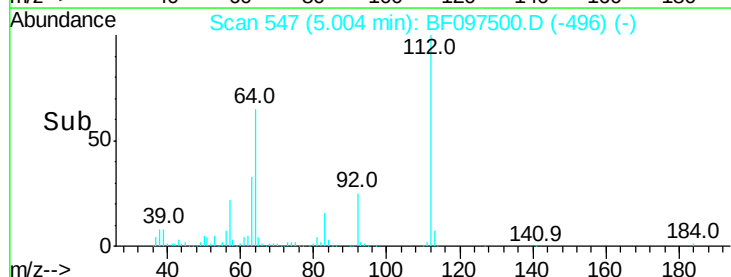

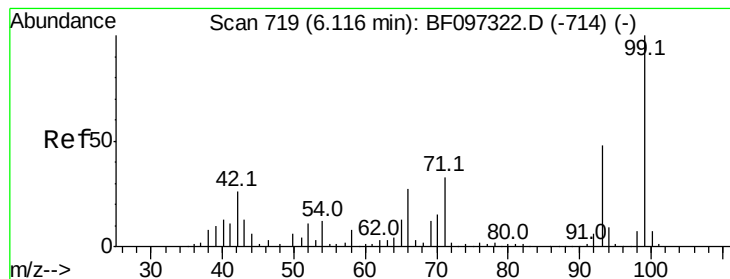

#7

Phenol-d6

Concen: 48.826 ng

RT: 6.08 min Scan# 730

Delta R.T. -0.01 min

Lab File: BF097500.D

Acq: 9 Aug 2017 6:02

Instrument :

BNA_F

ClientSampleId :

MW-5A-080217


Tot Ion: 99 Resp: 365415

Ion Ratio Lower Upper

99 100

42 24.0 13.5 20.3#




71 31.4 24.5 36.7

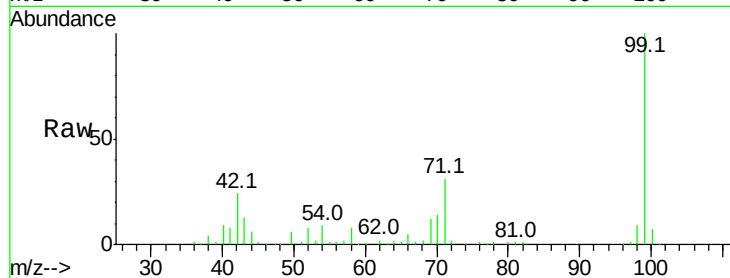

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

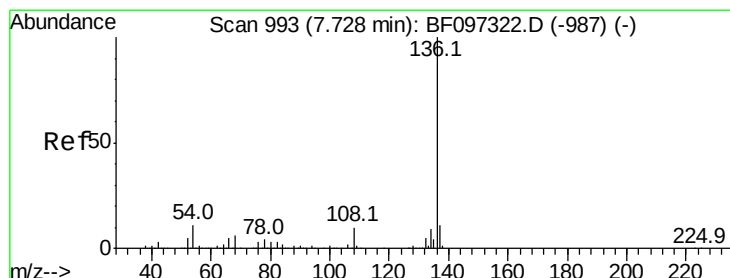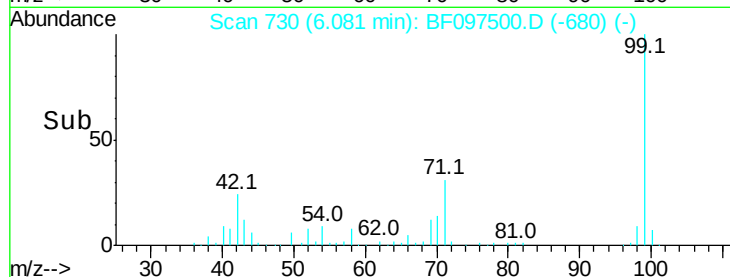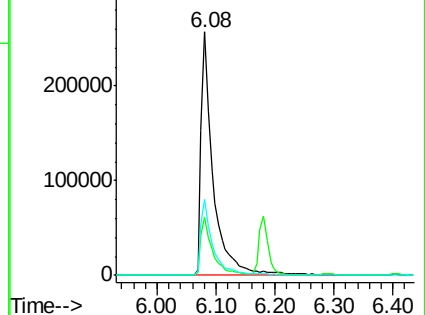

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.69 min Scan# 1003

Delta R.T. -0.01 min

Lab File: BF097500.D

Acq: 9 Aug 2017 6:02

Tgt Ion: 136 Resp: 343222


Ion Ratio Lower Upper

136 100

137 11.1 8.5 12.7

54 12.1 4.9 7.3#

68 6.1 4.1 6.1


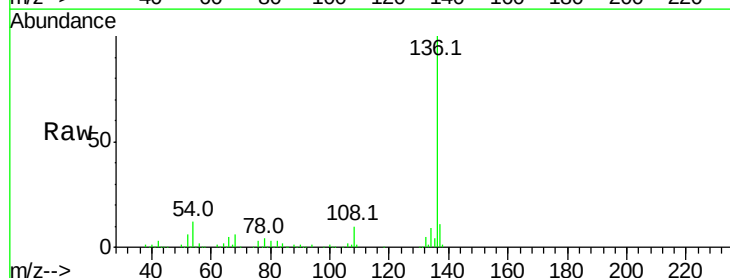



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



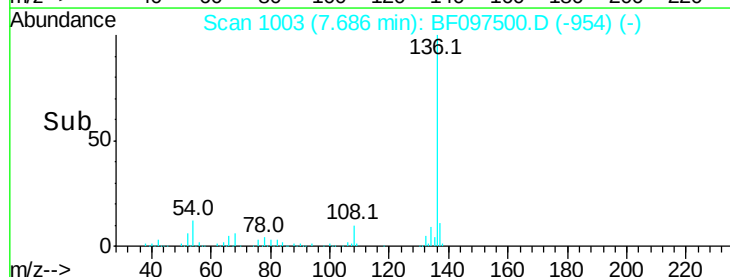
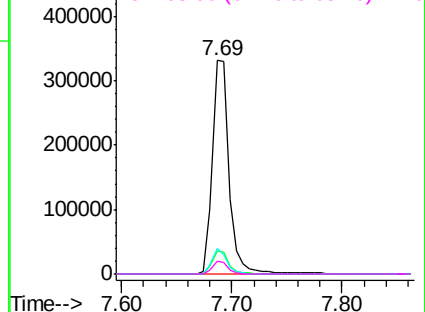


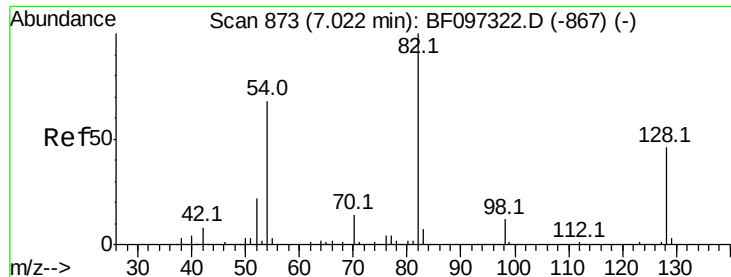

#23
 Nitrobenzene-d5
 Concen: 106.151 ng
 RT: 6.98 min Scan# 883
 Delta R.T. -0.01 min
 Lab File: BF097500.D
 Acq: 9 Aug 2017 6:02




Instrument :
 BNA_F
 ClientSampleId :
 MW-5A-080217


Tot Ion: 82 Resp: 621054
 Ion Ratio Lower Upper
 82 100
 128 44.7 34.0 51.0
 54 68.8 42.2 63.2#

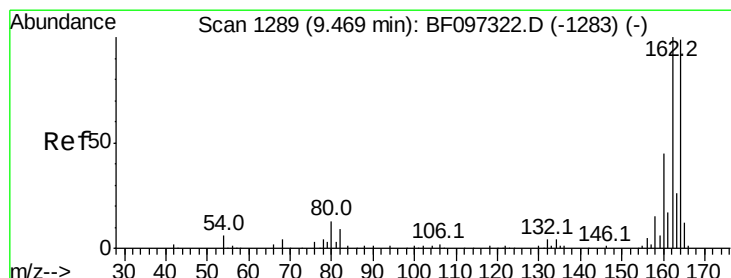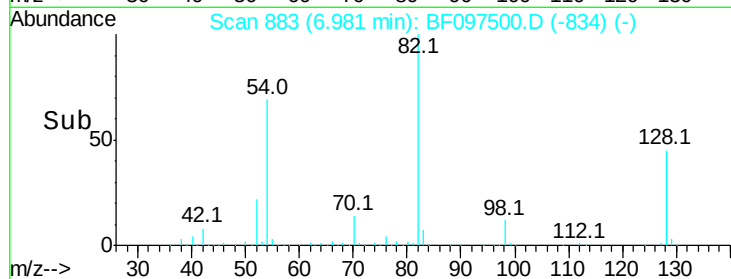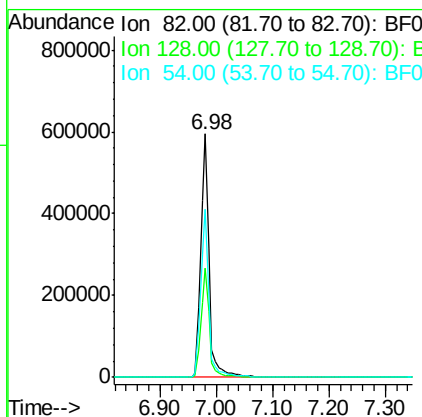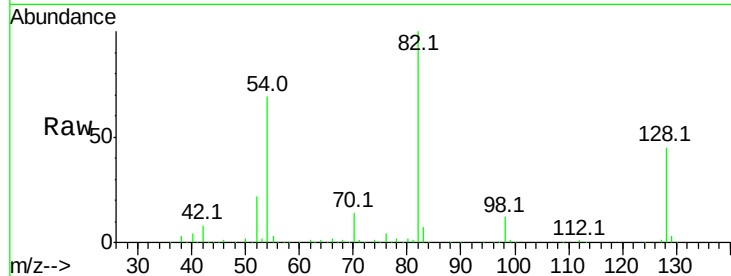

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.43 min Scan# 1300
 Delta R.T. -0.01 min
 Lab File: BF097500.D
 Acq: 9 Aug 2017 6:02

Tgt Ion:164 Resp: 136485
 Ion Ratio Lower Upper
 164 100
 162 103.0 82.6 123.8
 160 45.2 36.2 54.2


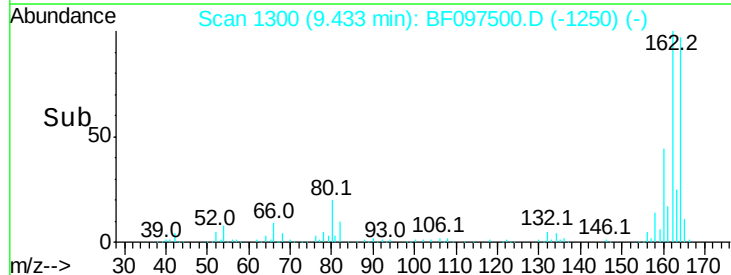
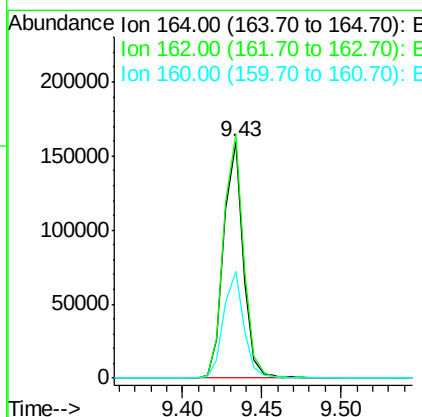
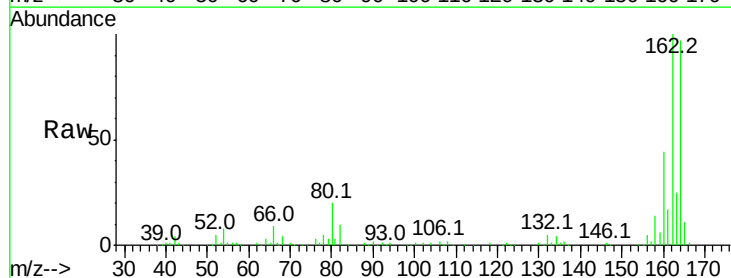


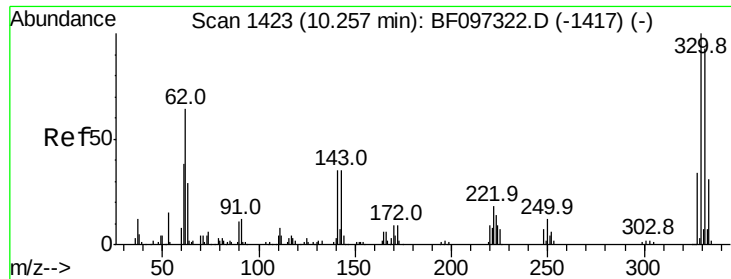

#41
 2,4,6-Tribromophenol
 Concen: 124.802 ng
 RT: 10.22 min Scan# 1434
 Delta R.T. -0.01 min
 Lab File: BF097500.D
 Acq: 9 Aug 2017 6:02




Instrument :
 BNA_F
 ClientSampleId :
 MW-5A-080217


Tot Ion	Ratio	Lower	Upper
330	100		
332	97.7	76.6	115.0
141	40.8	31.4	47.2

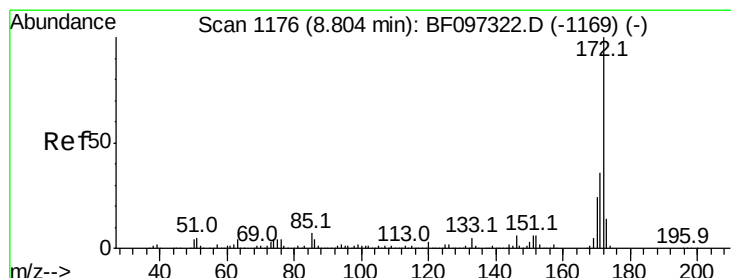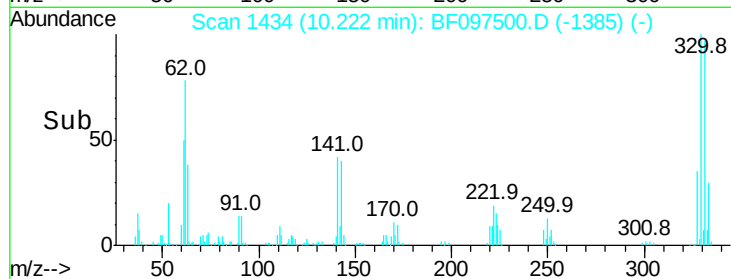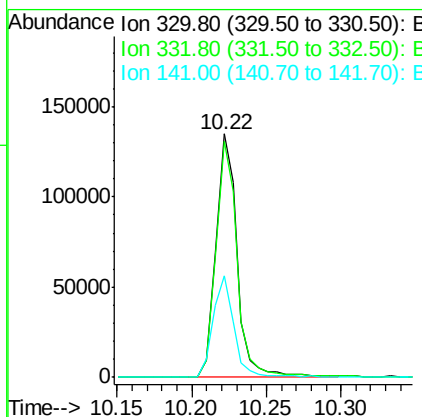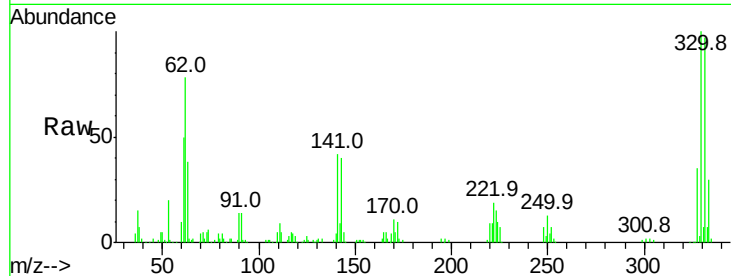

#44
 2-Fluorobiphenyl
 Concen: 104.422 ng
 RT: 8.77 min Scan# 1187
 Delta R.T. -0.01 min
 Lab File: BF097500.D
 Acq: 9 Aug 2017 6:02

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.4	29.6	44.4
170	24.2	19.8	29.8

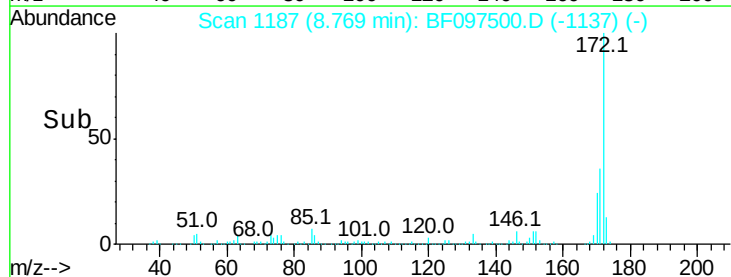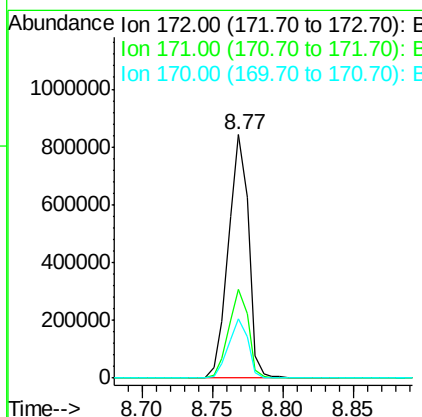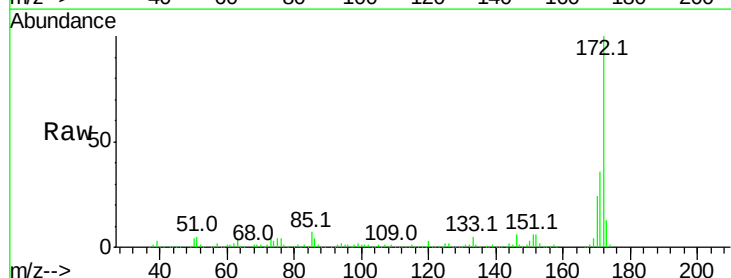


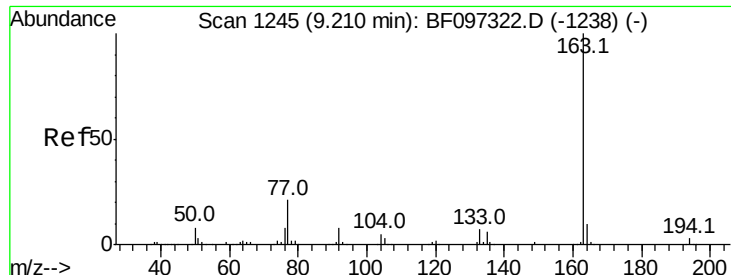




#49
Dimethylphthalate
Concen: 4.285 ng
RT: 9.17 min Scan# 1255
Delta R.T. -0.02 min
Lab File: BF097500.D
Acq: 9 Aug 2017 6:02

Instrument :
BNA_F
ClientSampleId :
MW-5A-080217

Tot Ion:163 Resp: 44414
Ion Ratio Lower Upper
163 100
194 3.0 2.6 4.0
164 10.2 8.4 12.6

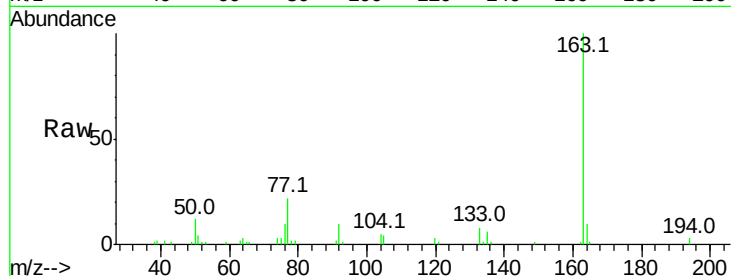


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

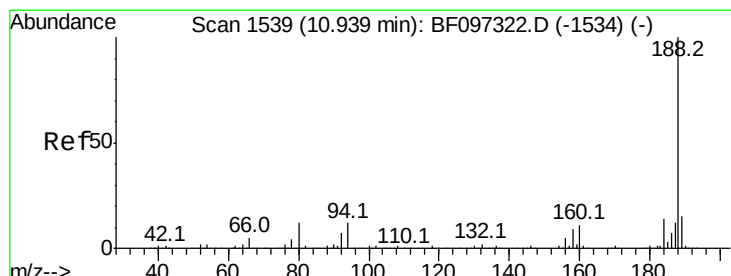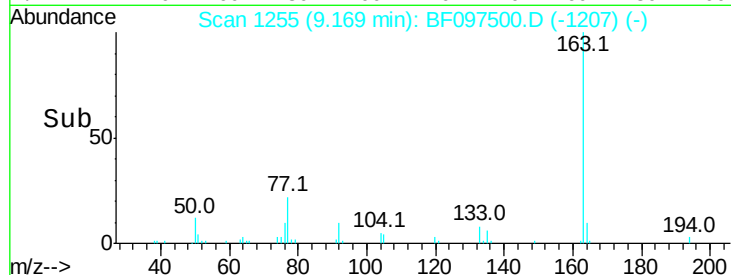
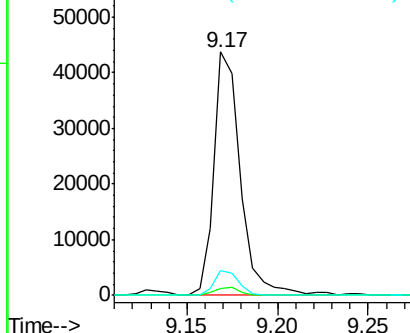



#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 10.90 min Scan# 1550
Delta R.T. -0.01 min
Lab File: BF097500.D
Acq: 9 Aug 2017 6:02

Tgt Ion:188 Resp: 212933
Ion Ratio Lower Upper
188 100
94 14.4 9.4 14.2#
80 13.9 10.2 15.2

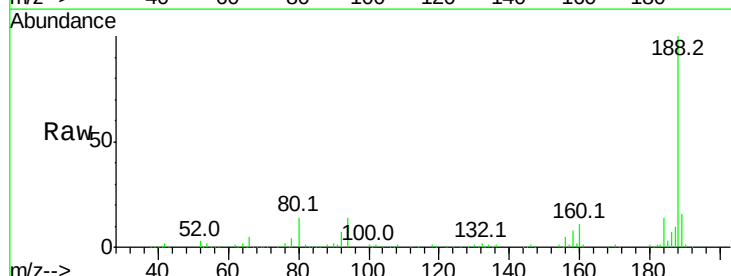

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

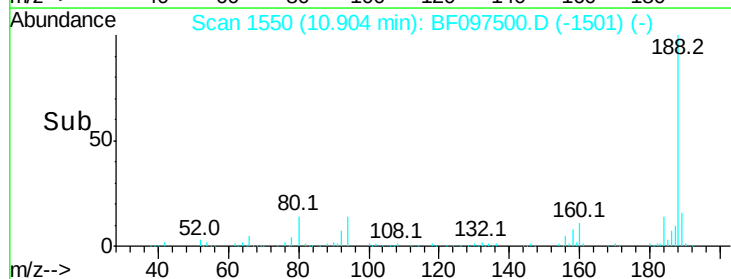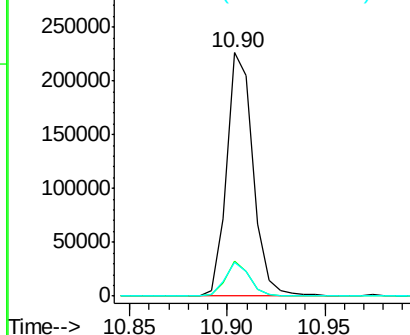

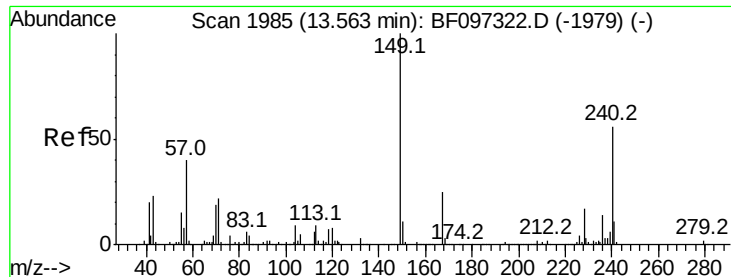

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.53 min Scan# 1997

Delta R.T. -0.01 min

Lab File: BF097500.D

Acq: 9 Aug 2017 6:02

Instrument :

BNA_F

ClientSampleId :

MW-5A-080217


Tot Ion:240 Resp: 157471

Ion Ratio Lower Upper

240 100

120 12.5 5.8 8.8#




236 25.6 20.5 30.7

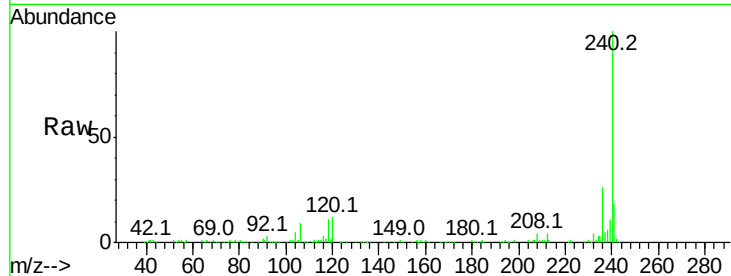

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

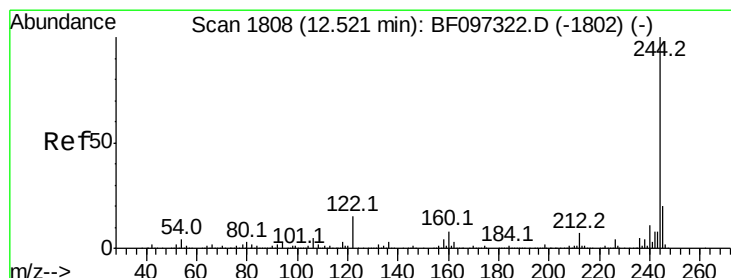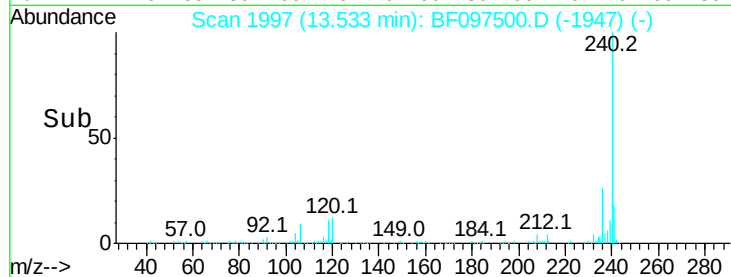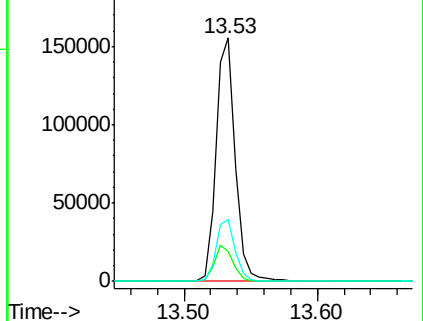

#78

Terphenyl-d14

Concen: 69.800 ng

RT: 12.49 min Scan# 1820

Delta R.T. -0.01 min

Lab File: BF097500.D

Acq: 9 Aug 2017 6:02


Tgt Ion:244 Resp: 539101

Ion Ratio Lower Upper

244 100

212 6.6 6.0 9.0



122 14.4 10.3 15.5

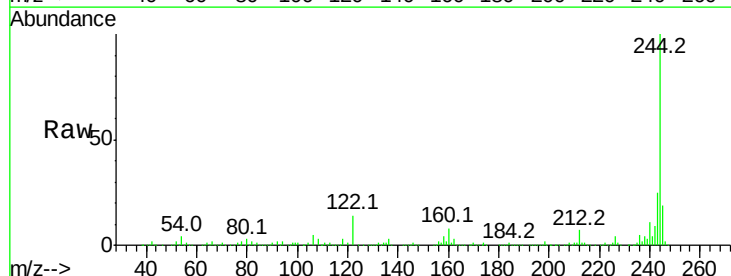


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

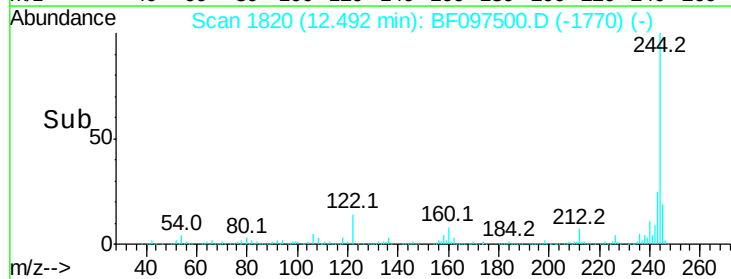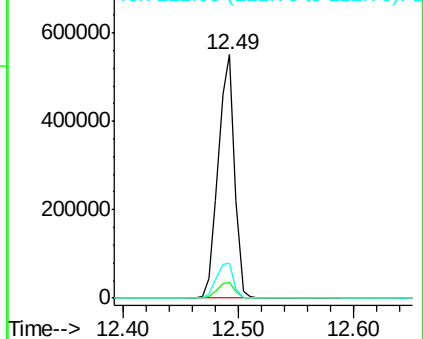


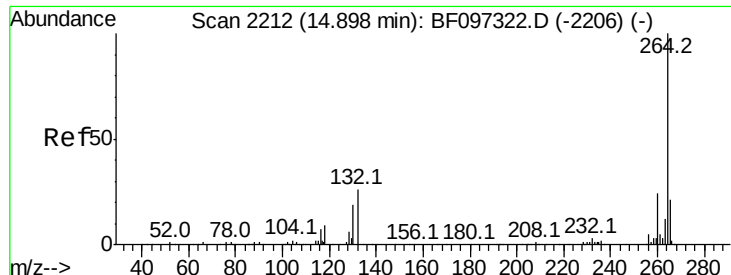

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 14.87 min Scan# 2225
 Delta R.T. 0.01 min
 Lab File: BF097500.D
 Acq: 9 Aug 2017 6:02

Instrument :
 BNA_F
 ClientSampleId :
 MW-5A-080217

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.0	19.5	29.3
265	21.3	17.2	25.8

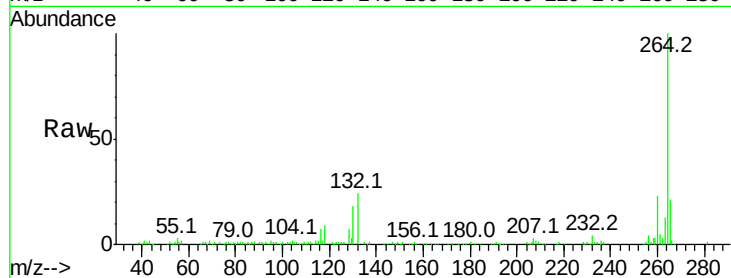

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

