


Data Path : Z:\HPCHEM1\BNA F\Data\BF080817\
Data File : BF097462.D
Acq On : 8 Aug 2017 11:20
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 07 16:02:51 2017

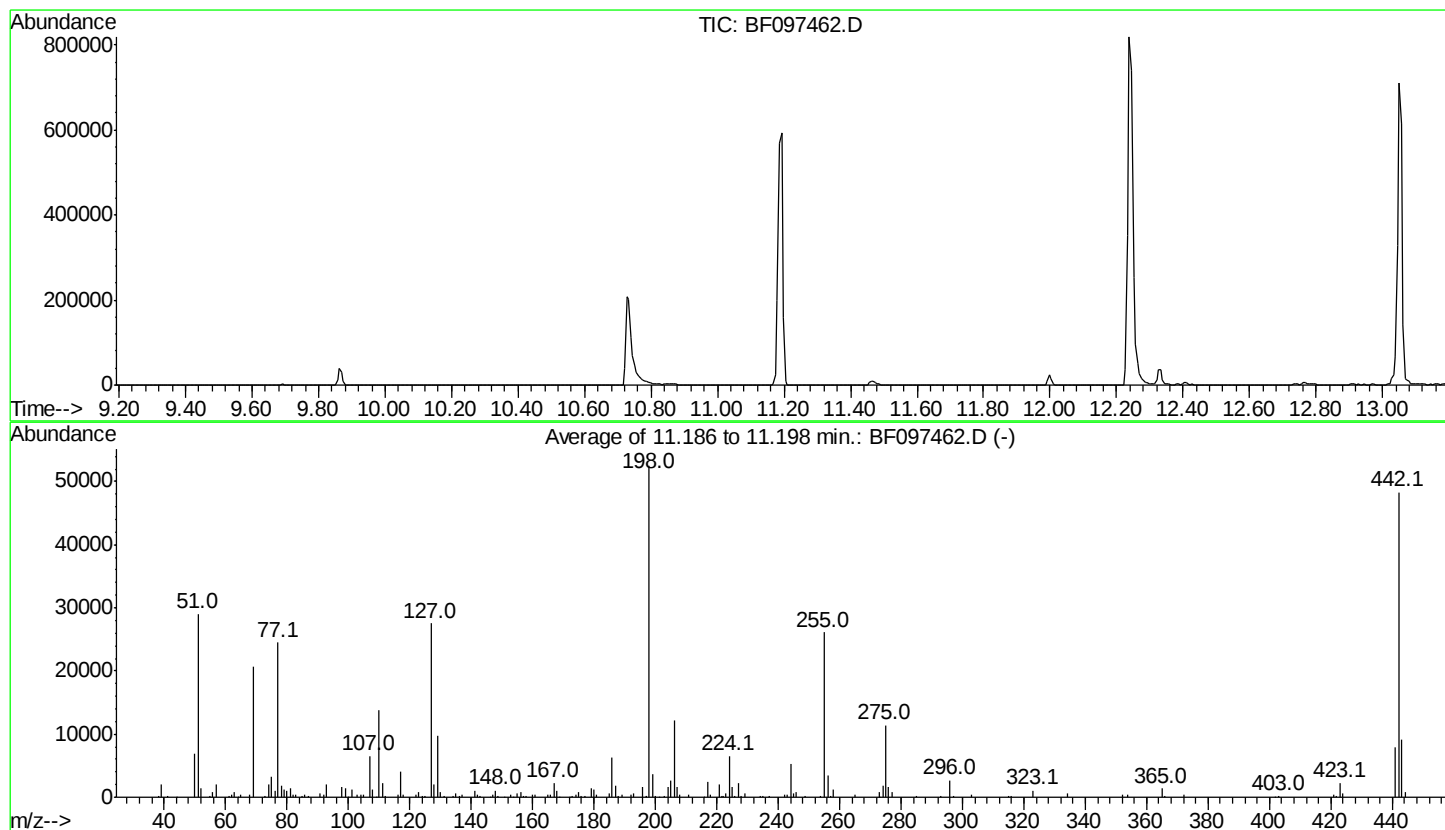

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.4	29091	PASS
68	69	0.00	2	1.7	352	PASS
69	198	0.00	100	39.5	20752	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.5	27563	PASS
197	198	0.00	2	0.5	287	PASS
198	198	100	100	100.0	52522	PASS
199	198	5	9	6.9	3649	PASS
275	198	10	60	21.8	11453	PASS
365	198	1	100	2.6	1379	PASS
441	442	0.01	24	16.2	7825	PASS
442	198	50	100	92.0	48306	PASS
443	442	15	24	19.1	9230	PASS