


Data Path : Z:\HPCHEM1\BNA F\Data\BF080817\
Data File : BF097475.D
Acq On : 8 Aug 2017 18:22
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 07 16:02:51 2017

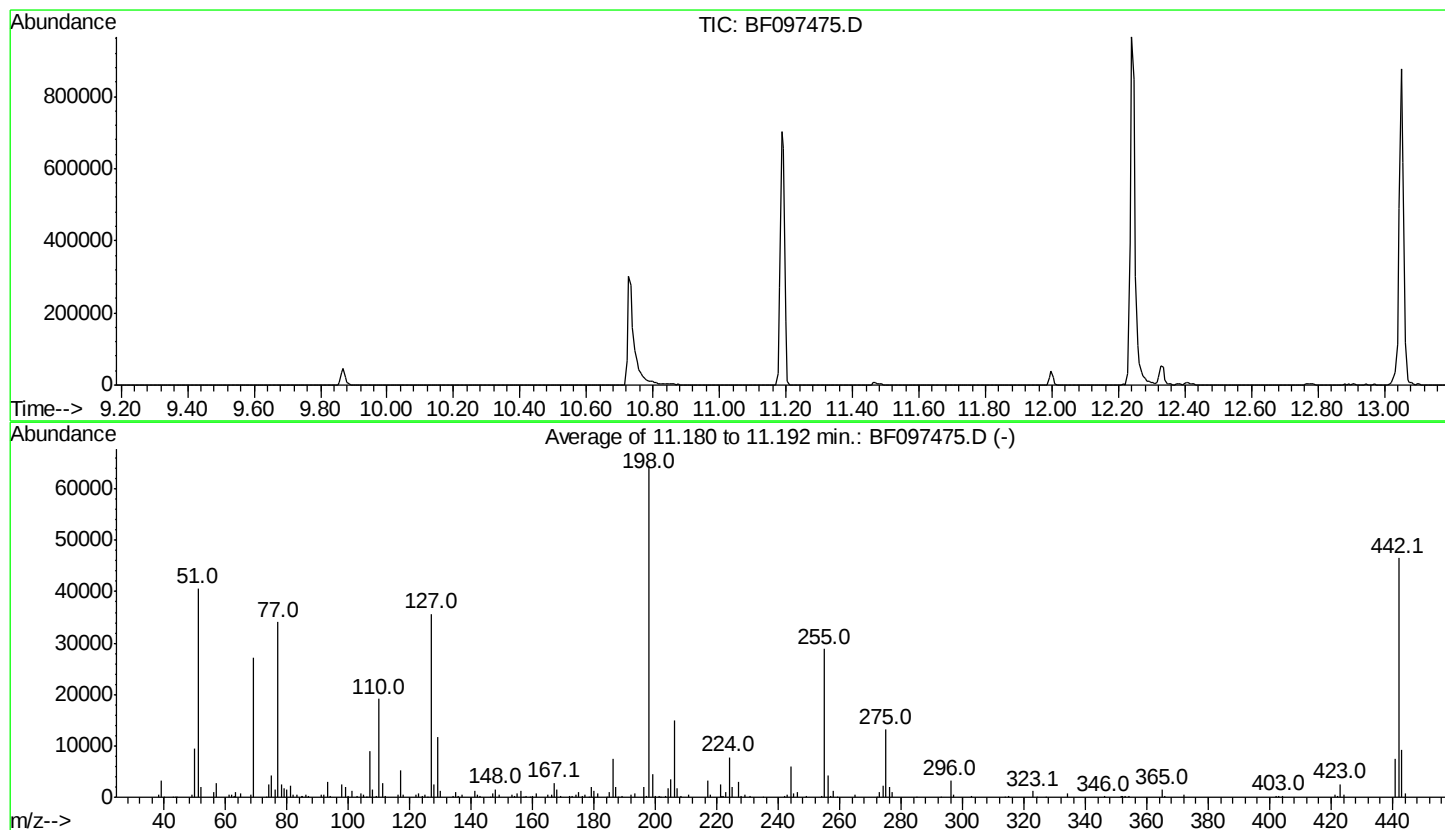

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.8	40514	PASS
68	69	0.00	2	1.8	494	PASS
69	198	0.00	100	42.0	27082	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.4	35744	PASS
197	198	0.00	2	0.4	274	PASS
198	198	100	100	100.0	64533	PASS
199	198	5	9	7.1	4550	PASS
275	198	10	60	20.4	13149	PASS
365	198	1	100	2.2	1429	PASS
441	442	0.01	24	16.1	7482	PASS
442	198	50	100	72.2	46576	PASS
443	442	15	24	20.1	9341	PASS