


Data Path : Z:\HPCHEM1\BNA F\DATA\BF080817\
 Data File : BF097501.D
 Acq On : 9 Aug 2017 6:57
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 07 16:02:51 2017

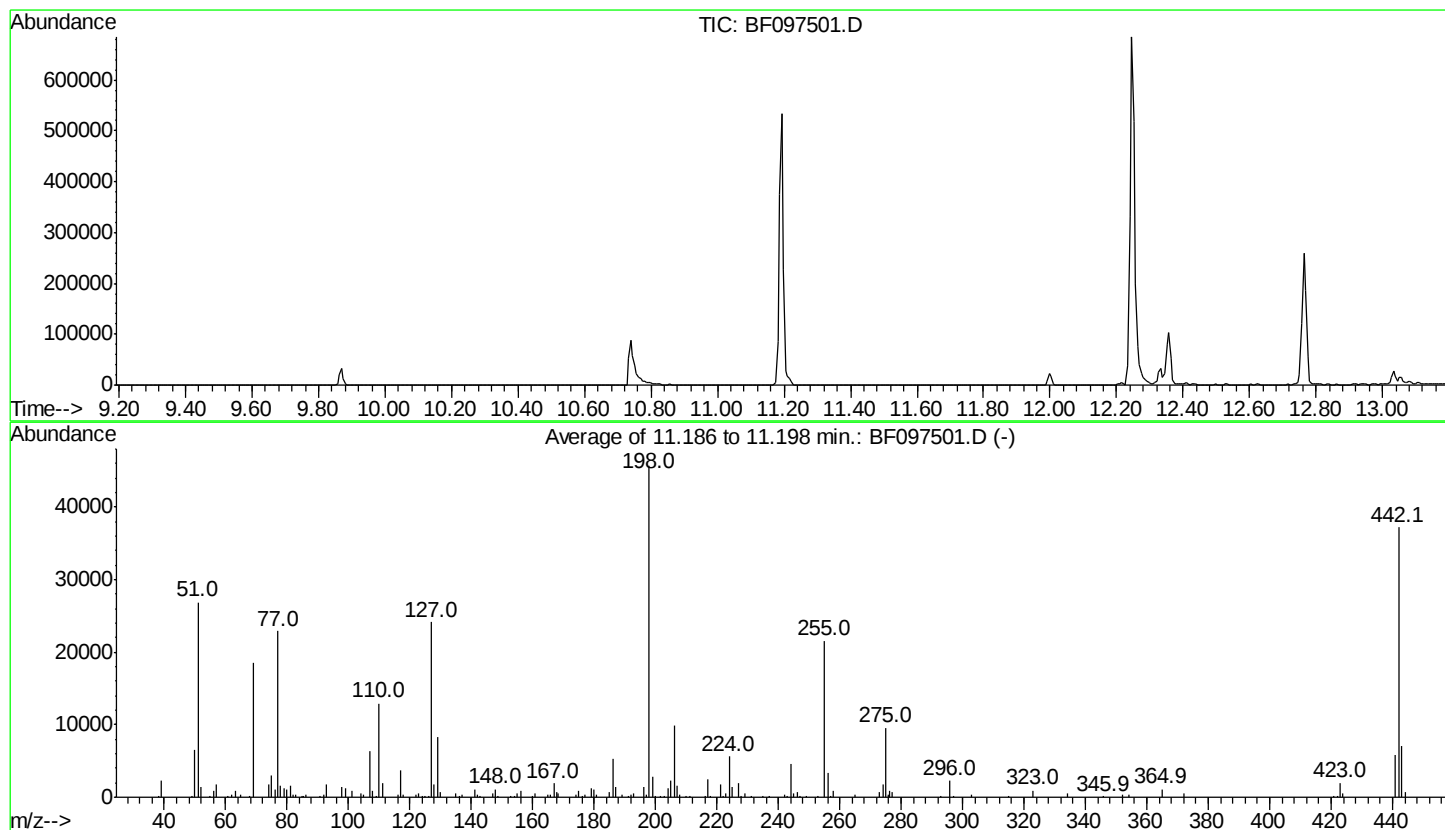

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.8	26899	PASS
68	69	0.00	2	0.8	140	PASS
69	198	0.00	100	40.5	18509	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.8	24139	PASS
197	198	0.00	2	0.7	306	PASS
198	198	100	100	100.0	45728	PASS
199	198	5	9	6.3	2891	PASS
275	198	10	60	20.9	9538	PASS
365	198	1	100	2.4	1093	PASS
441	442	0.01	24	15.7	5830	PASS
442	198	50	100	81.3	37194	PASS
443	442	15	24	19.1	7107	PASS