

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF080824\  
 Data File : BF138872.D  
 Acq On : 08 Aug 2024 18:31  
 Operator : RC/JU  
 Sample : P3488-03 5X  
 Misc :  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 HD-02-080624

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF073024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138872.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.045       | 497           | 502         | 510          | rBV      | 4346           | 7394          | 2.10%           | 0.333%        |
| 2         | 5.469       | 570           | 574         | 591          | rBB      | 44425          | 71695         | 20.38%          | 3.233%        |
| 3         | 6.487       | 742           | 747         | 759          | rBV      | 47076          | 77245         | 21.96%          | 3.484%        |
| 4         | 6.839       | 802           | 807         | 813          | rBV      | 222005         | 275384        | 78.29%          | 12.420%       |
| 5         | 7.404       | 899           | 903         | 911          | rVV      | 36056          | 55317         | 15.73%          | 2.495%        |
| 6         | 8.122       | 1017          | 1025        | 1030         | rBV      | 270119         | 351763        | 100.00%         | 15.865%       |
| 7         | 8.169       | 1030          | 1033        | 1037         | rVB      | 5794           | 7586          | 2.16%           | 0.342%        |
| 8         | 8.404       | 1067          | 1073        | 1078         | rBV4     | 3772           | 8042          | 2.29%           | 0.363%        |
| 9         | 8.533       | 1091          | 1095        | 1105         | rVB      | 7934           | 12876         | 3.66%           | 0.581%        |
| 10        | 8.763       | 1127          | 1134        | 1137         | rVV4     | 2247           | 4772          | 1.36%           | 0.215%        |
| 11        | 9.016       | 1174          | 1177        | 1182         | rVB4     | 2414           | 3688          | 1.05%           | 0.166%        |
| 12        | 9.128       | 1189          | 1196        | 1201         | rBV2     | 7237           | 11721         | 3.33%           | 0.529%        |
| 13        | 9.192       | 1201          | 1207        | 1216         | rBV      | 68001          | 88425         | 25.14%          | 3.988%        |
| 14        | 9.269       | 1216          | 1220        | 1224         | rBV3     | 4641           | 6827          | 1.94%           | 0.308%        |
| 15        | 9.533       | 1258          | 1265        | 1268         | rBV5     | 1766           | 4068          | 1.16%           | 0.183%        |
| 16        | 9.580       | 1268          | 1273        | 1277         | rVB6     | 8148           | 12019         | 3.42%           | 0.542%        |
| 17        | 9.792       | 1302          | 1309        | 1313         | rBV5     | 2907           | 7031          | 2.00%           | 0.317%        |
| 18        | 9.869       | 1317          | 1322        | 1332         | rVB      | 278149         | 343705        | 97.71%          | 15.501%       |
| 19        | 10.292      | 1388          | 1394        | 1398         | rBV4     | 3092           | 4607          | 1.31%           | 0.208%        |
| 20        | 10.510      | 1426          | 1431        | 1438         | rBV4     | 4646           | 6808          | 1.94%           | 0.307%        |
| 21        | 10.663      | 1453          | 1457        | 1466         | rVB      | 20375          | 27952         | 7.95%           | 1.261%        |
| 22        | 10.769      | 1466          | 1475        | 1484         | rBV2     | 7327           | 13538         | 3.85%           | 0.611%        |
| 23        | 11.210      | 1546          | 1550        | 1553         | rBV3     | 3422           | 4684          | 1.33%           | 0.211%        |
| 24        | 11.357      | 1570          | 1575        | 1584         | rBV      | 216499         | 272440        | 77.45%          | 12.287%       |
| 25        | 11.639      | 1618          | 1623        | 1627         | rVB      | 3418           | 4545          | 1.29%           | 0.205%        |
| 26        | 12.045      | 1688          | 1692        | 1696         | rVB2     | 3307           | 4363          | 1.24%           | 0.197%        |
| 27        | 12.433      | 1748          | 1758        | 1762         | rBV5     | 4152           | 8831          | 2.51%           | 0.398%        |
| 28        | 12.574      | 1778          | 1782        | 1787         | rBV      | 4609           | 6216          | 1.77%           | 0.280%        |
| 29        | 12.798      | 1815          | 1820        | 1825         | rBV      | 7457           | 11935         | 3.39%           | 0.538%        |
| 30        | 12.933      | 1837          | 1843        | 1850         | rBV      | 46759          | 58925         | 16.75%          | 2.658%        |
| 31        | 13.157      | 1878          | 1881        | 1890         | rBV8     | 4816           | 9435          | 2.68%           | 0.426%        |
| 32        | 13.468      | 1930          | 1934        | 1936         | rBV3     | 3987           | 5137          | 1.46%           | 0.232%        |
| 33        | 13.498      | 1937          | 1939        | 1943         | rVB5     | 4183           | 4665          | 1.33%           | 0.210%        |
| 34        | 13.992      | 2018          | 2023        | 2035         | rBV      | 167555         | 233349        | 66.34%          | 10.524%       |
| 35        | 15.457      | 2267          | 2272        | 2278         | rVB      | 125815         | 190277        | 54.09%          | 8.582%        |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF080824\  
Data File : BF138872.D  
Acq On : 08 Aug 2024 18:31  
Operator : RC/JU  
Sample : P3488-03 5X  
Misc :  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
HD-02-080624

Integration Parameters: rteint.p  
Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF073024.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 2217265

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF080824\  
Data File : BF138872.D  
Acq On : 08 Aug 2024 18:31  
Operator : RC/JU  
Sample : P3488-03 5X  
Misc :  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
HD-02-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF073024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

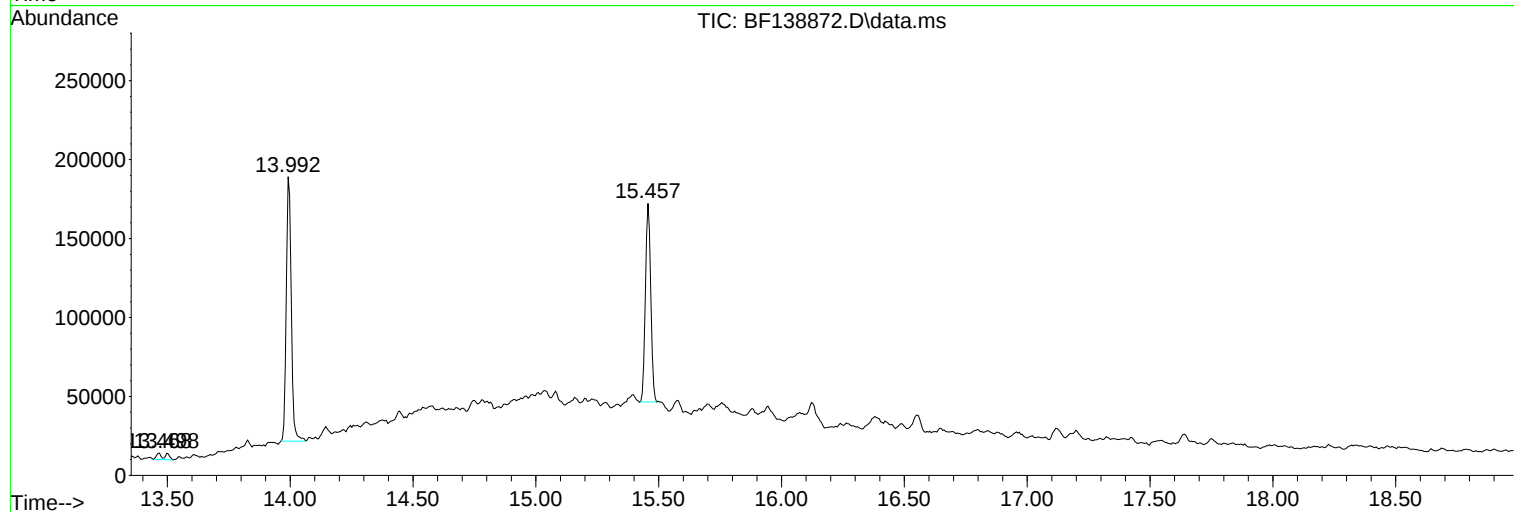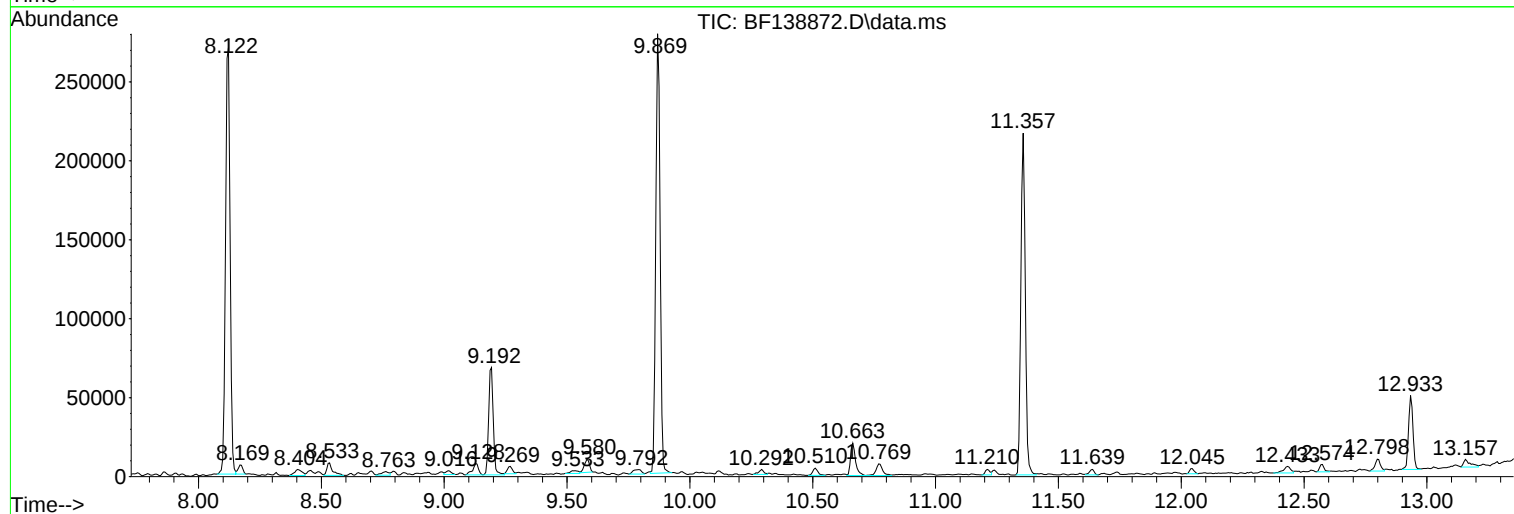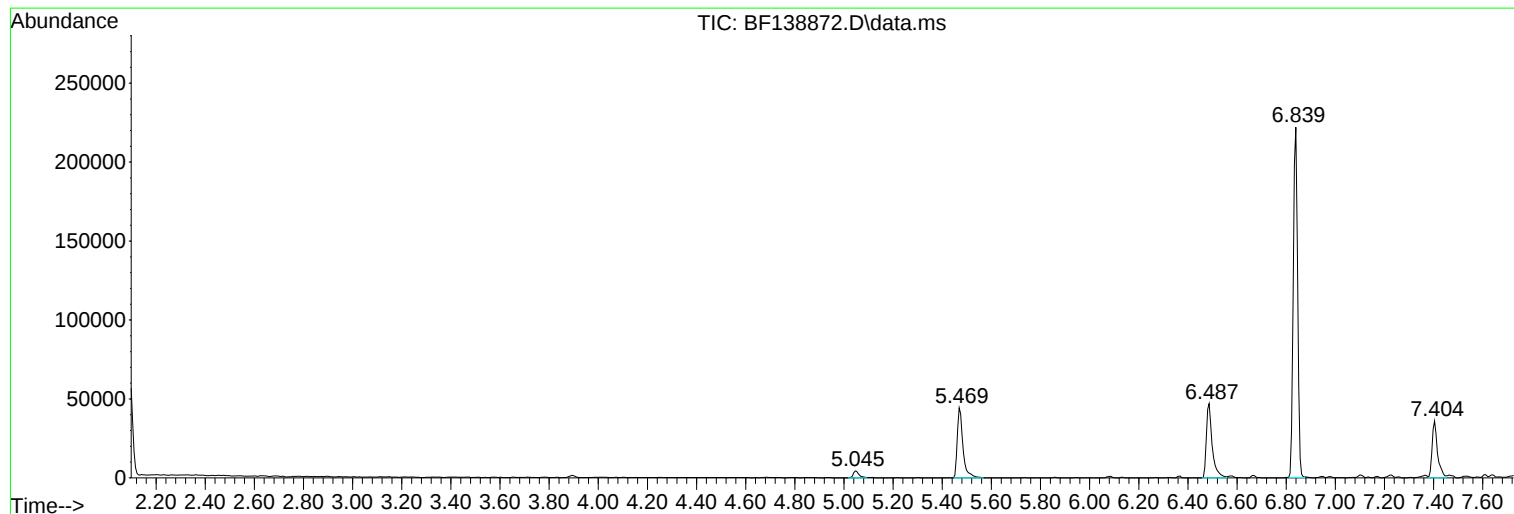

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF080824\  
Data File : BF138872.D  
Acq On : 08 Aug 2024 18:31  
Operator : RC/JU  
Sample : P3488-03 5X  
Misc :  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
HD-02-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF073024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF080824\  
Data File : BF138872.D  
Acq On : 08 Aug 2024 18:31  
Operator : RC/JU  
Sample : P3488-03 5X  
Misc :  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
HD-02-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF073024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|