


Data Path : Z:\HPCHEM1\BNA F\DATA\BF080916\
 Data File : BF089688.D
 Acq On : 9 Aug 2016 14:56
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 05 01:39:23 2016

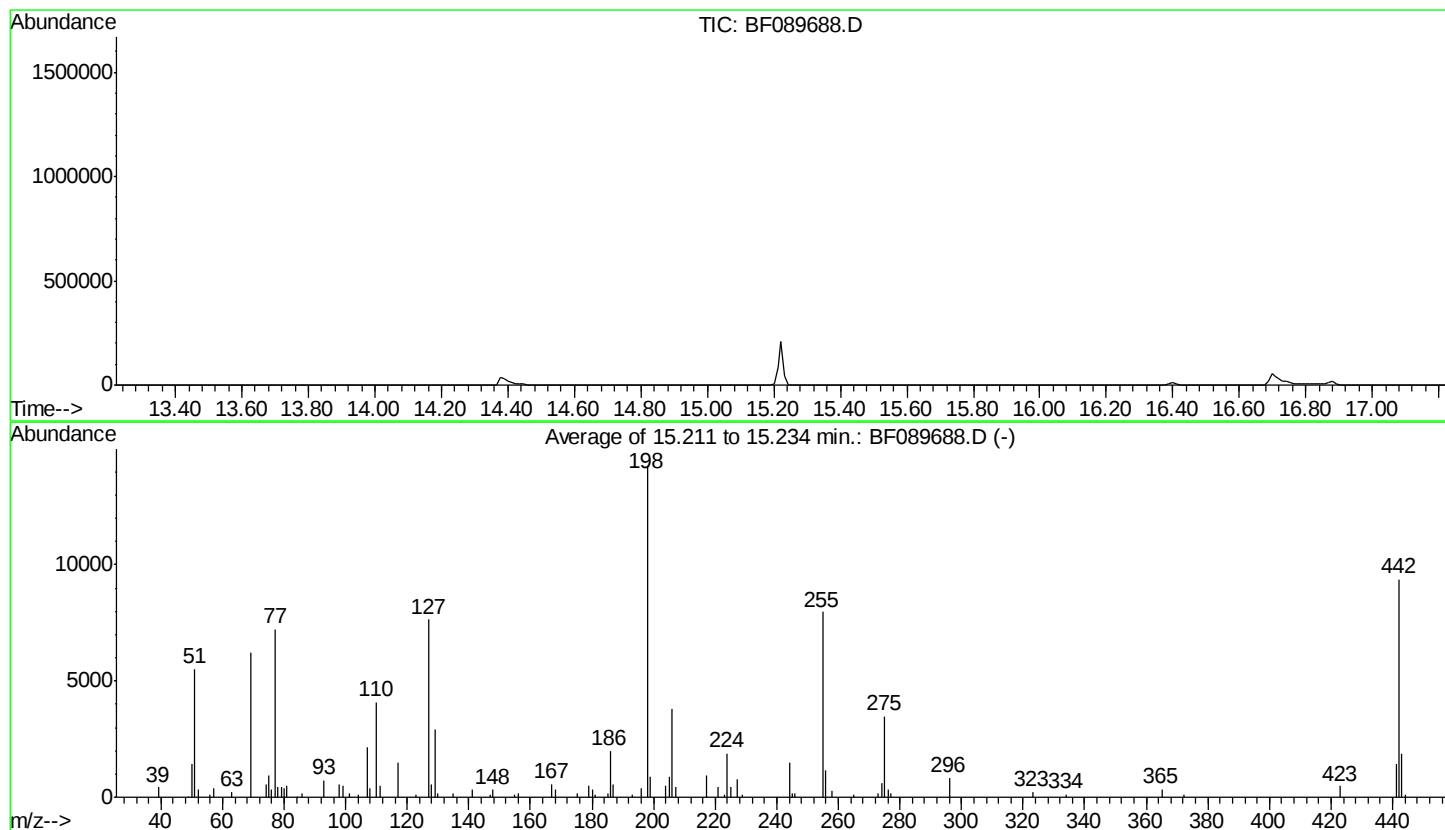

AutoFind: Scans 1192, 1193, 1194; Background Corrected with Scan 1189

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	5518	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.5	6204	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.5	7635	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14264	PASS
199	198	5	9	6.3	897	PASS
275	198	10	60	24.4	3486	PASS
365	198	1	100	2.4	345	PASS
441	442	0.01	24	15.3	1439	PASS
442	198	50	100	65.8	9383	PASS
443	442	15	24	19.8	1855	PASS