
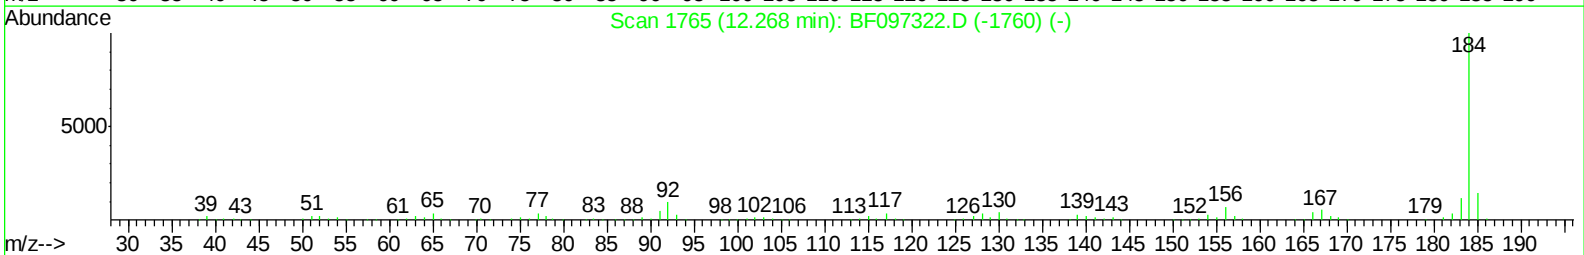
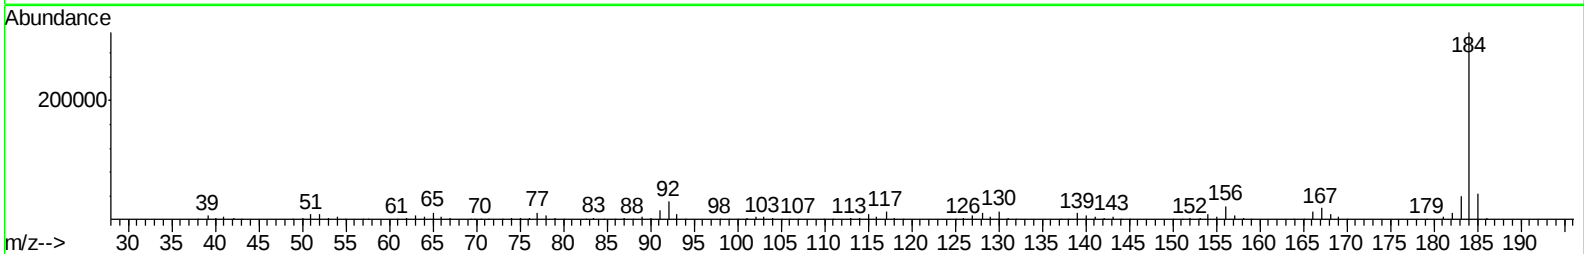


```
Data Path : Z:\HPCHEM1\BNA F\DATA\BF080917\  
Data File : BF097522.D  
Acq On    : 9 Aug 2017 18:19  
Operator   : SJ/JU  
Sample     : DFTPP  
Misc       :  
ALS Vial   : 1 Sample Multiplier: 1
```

Quant Time: Aug 10 08:29:31 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 07 16:02:51 2017
Response via : Initial Calibration



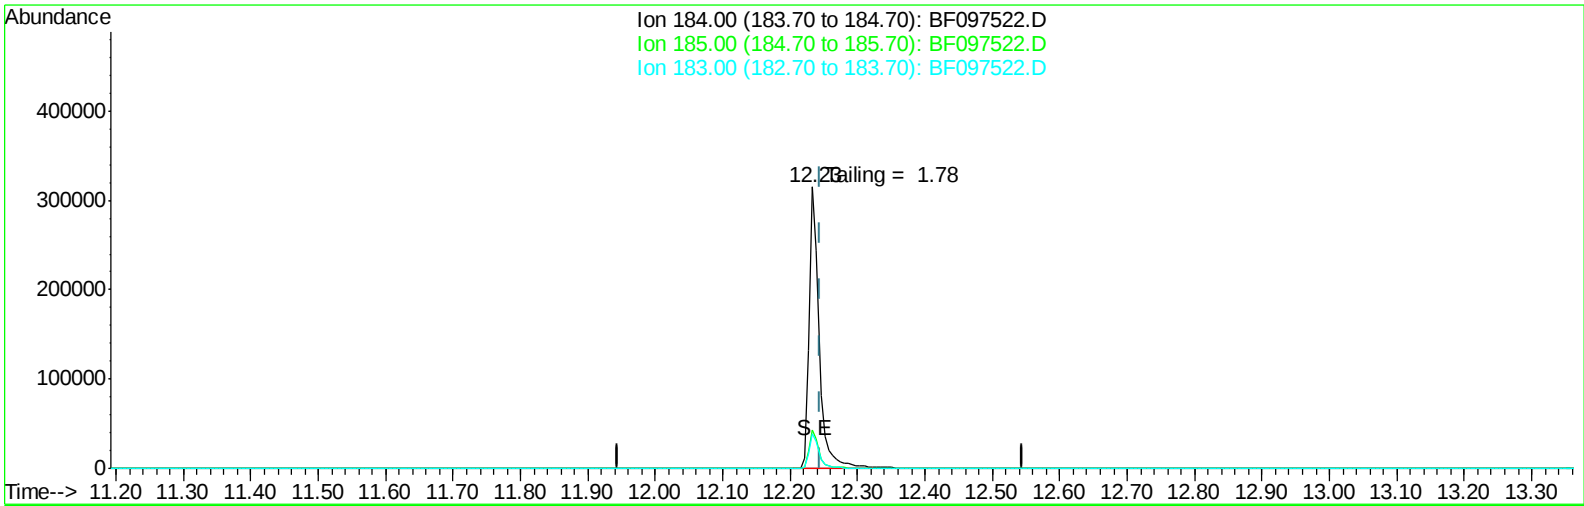


TIC: BF097522.D

(76) Benzidine		
12.233min (-0.012)	0.00ng	
response	320190	
Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.71#
183.00	12.20	12.13
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080917\
Data File : BF097522.D
Acq On : 9 Aug 2017 18:19
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 08:29:31 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 07 16:02:51 2017
Response via : Initial Calibration

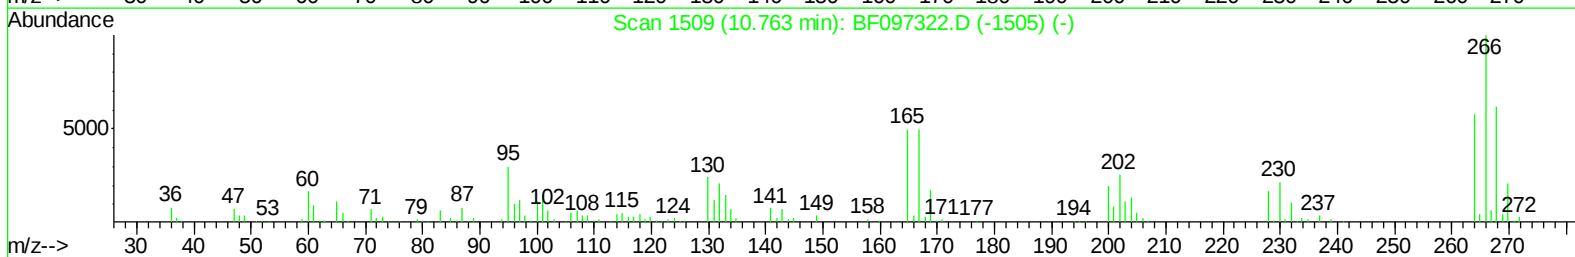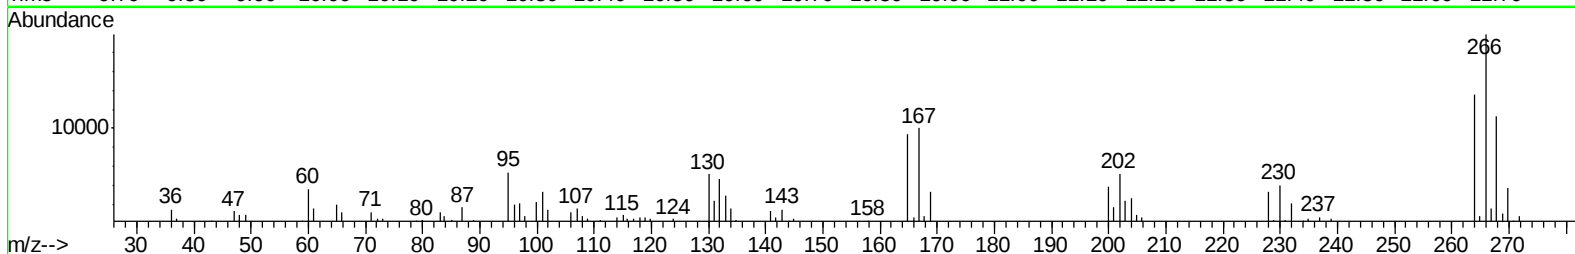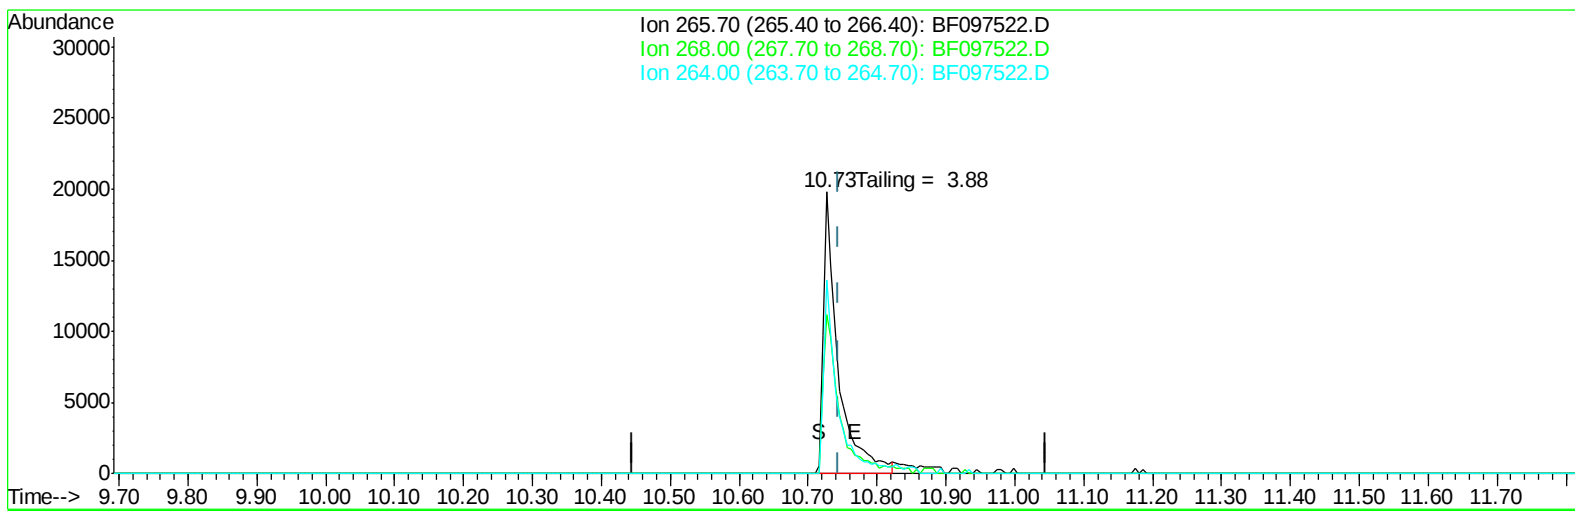

TIC: BF097522.D

(69) Pentachlorophenol (C)

10.728min (-0.017) 46313.61ng

response 28951

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	56.56
264.00	64.60	68.54
0.00	0.00	0.00