


Data Path : Z:\HPCHEM1\BNA F\Data\BF080917\
Data File : BF097516.D
Acq On : 9 Aug 2017 15:04
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 07 16:02:51 2017

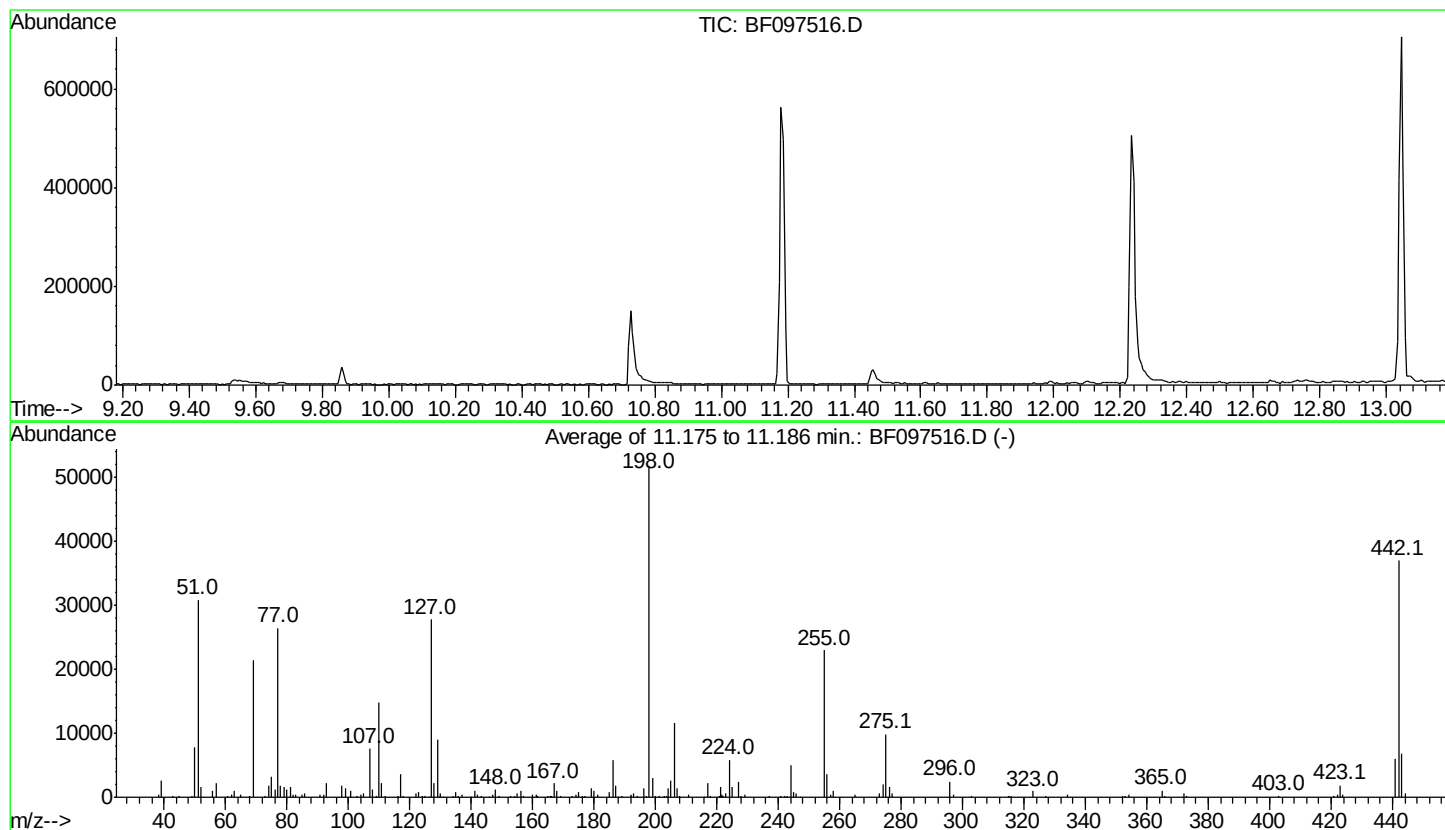

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.6	30842	PASS
68	69	0.00	2	0.8	181	PASS
69	198	0.00	100	41.4	21404	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.6	27740	PASS
197	198	0.00	2	0.4	188	PASS
198	198	100	100	100.0	51762	PASS
199	198	5	9	5.9	3063	PASS
275	198	10	60	19.1	9888	PASS
365	198	1	100	2.1	1094	PASS
441	442	0.01	24	16.0	5926	PASS
442	198	50	100	71.3	36932	PASS
443	442	15	24	18.6	6859	PASS