


Data Path : Z:\HPCHEM1\BNA F\Data\BF080917\
 Data File : BF097522.D
 Acq On : 9 Aug 2017 18:19
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 07 16:02:51 2017

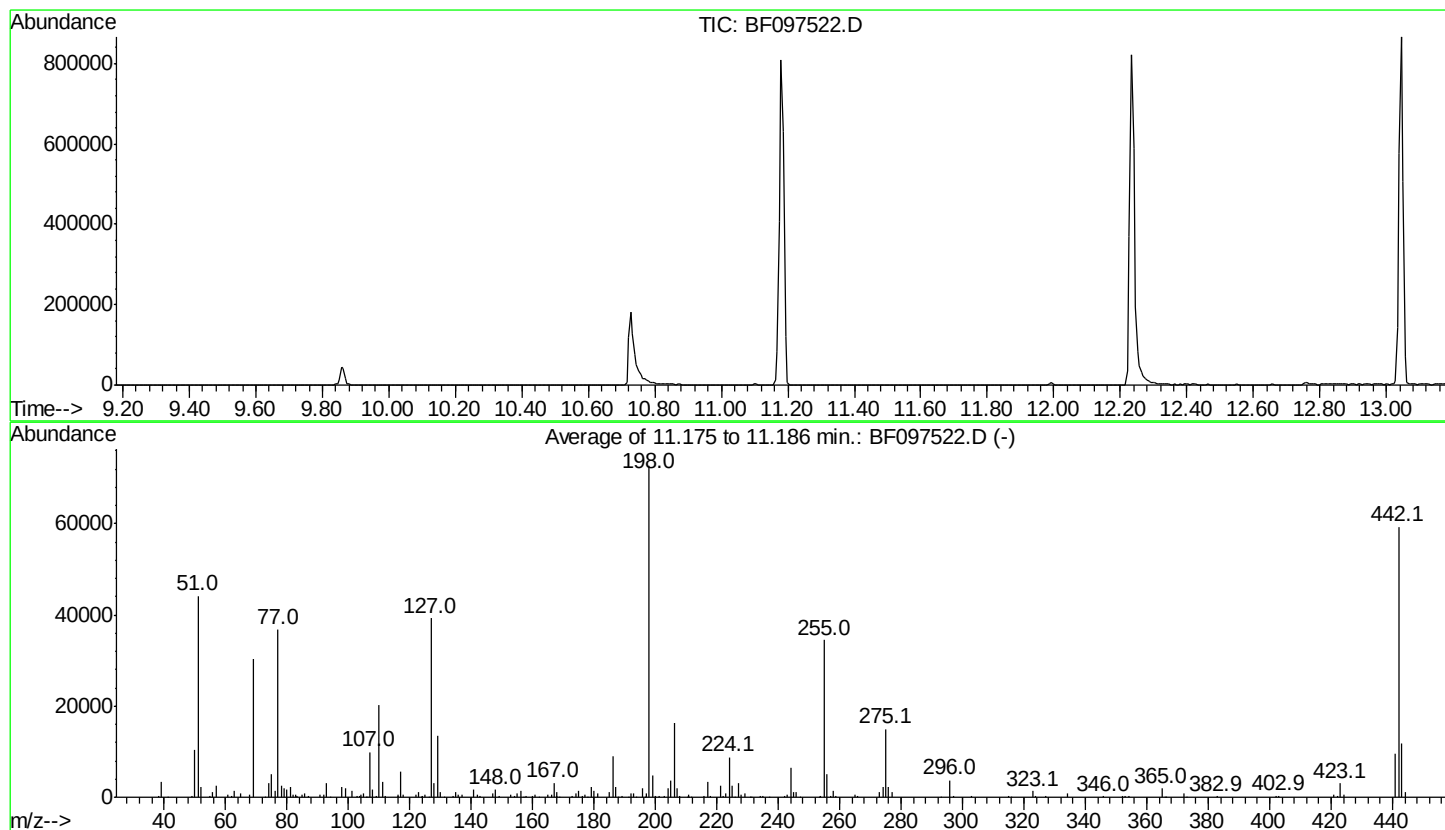

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.8	44184	PASS
68	69	0.00	2	1.6	489	PASS
69	198	0.00	100	41.8	30402	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.9	39178	PASS
197	198	0.00	2	1.0	747	PASS
198	198	100	100	100.0	72720	PASS
199	198	5	9	6.4	4667	PASS
275	198	10	60	20.6	14982	PASS
365	198	1	100	2.6	1876	PASS
441	442	0.01	24	16.0	9481	PASS
442	198	50	100	81.5	59293	PASS
443	442	15	24	19.7	11676	PASS