


Data Path : Z:\HPCHEM1\BNA F\Data\BF080917\
 Data File : BF097547.D
 Acq On : 10 Aug 2017 7:57
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 07 16:02:51 2017

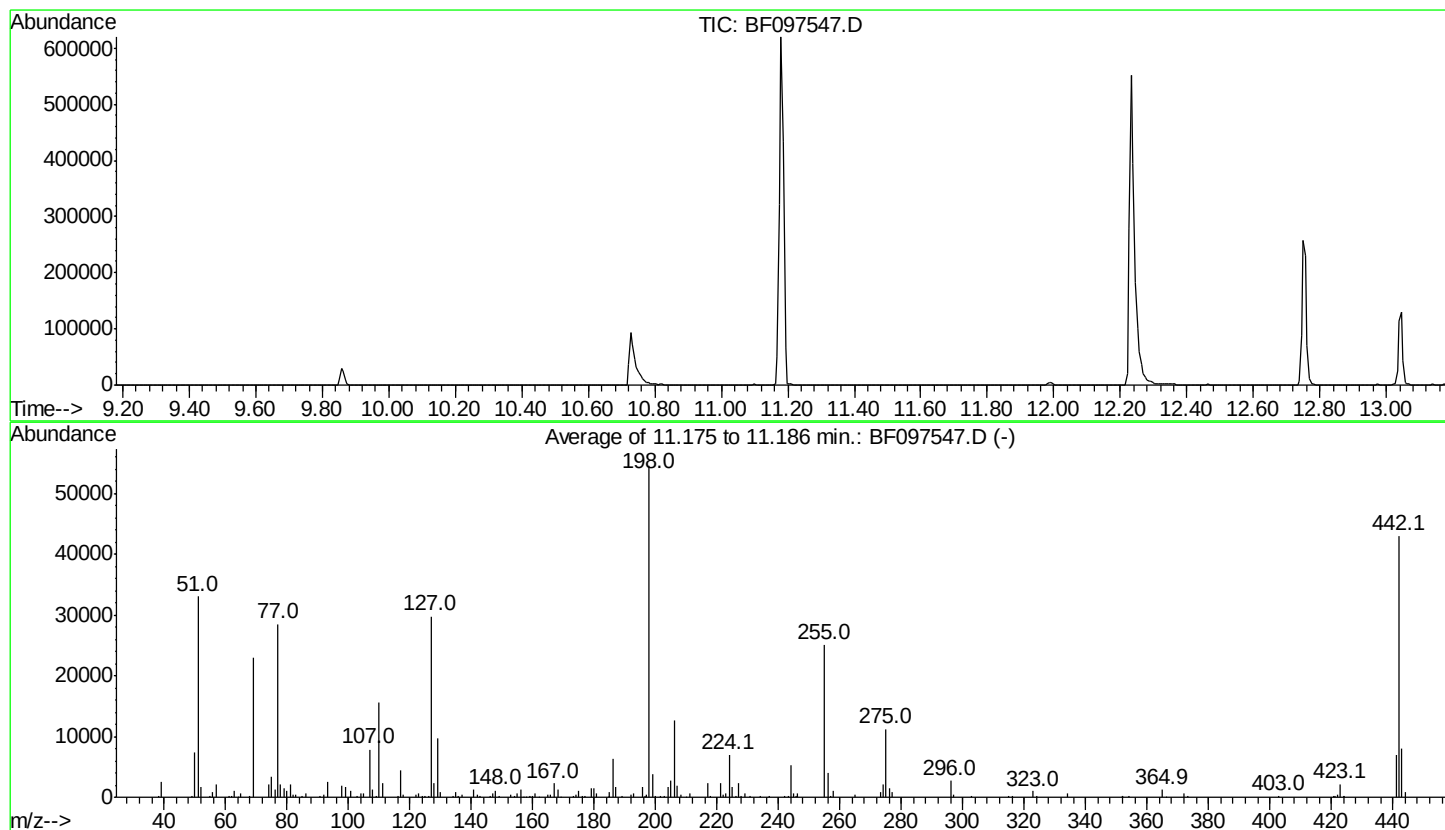

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.5	33050	PASS
68	69	0.00	2	1.1	249	PASS
69	198	0.00	100	42.0	22916	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.5	29760	PASS
197	198	0.00	2	0.8	422	PASS
198	198	100	100	100.0	54613	PASS
199	198	5	9	6.8	3733	PASS
275	198	10	60	20.5	11217	PASS
365	198	1	100	2.2	1183	PASS
441	442	0.01	24	16.4	7050	PASS
442	198	50	100	78.9	43063	PASS
443	442	15	24	18.8	8103	PASS