
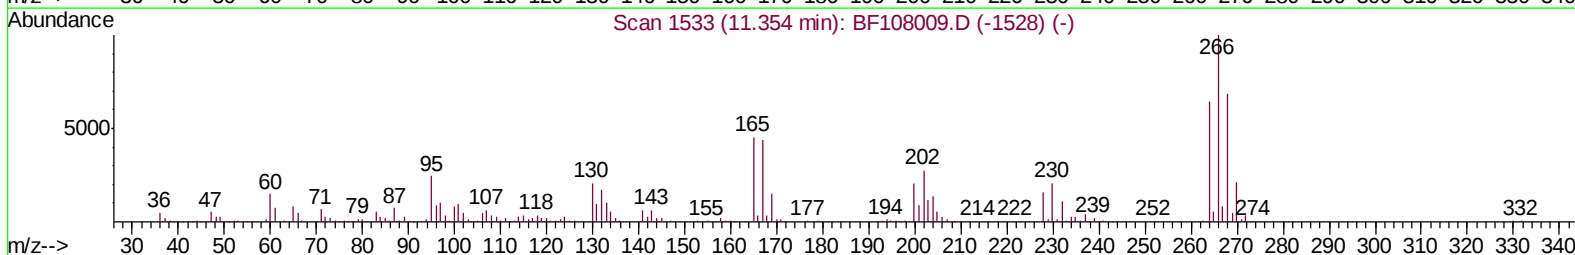
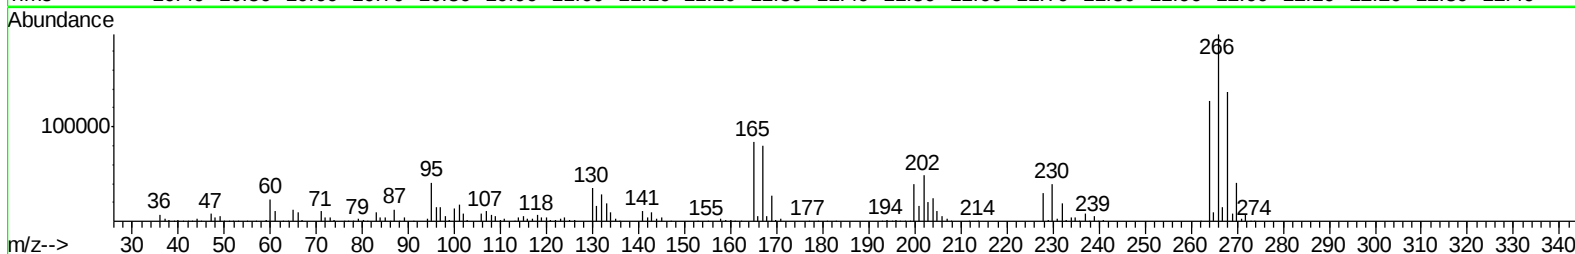


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080918\
Data File : BF108066.D
Acq On : 9 Aug 2018 22:23
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 04:27:06 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 12:24:24 2018
Response via : Initial Calibration

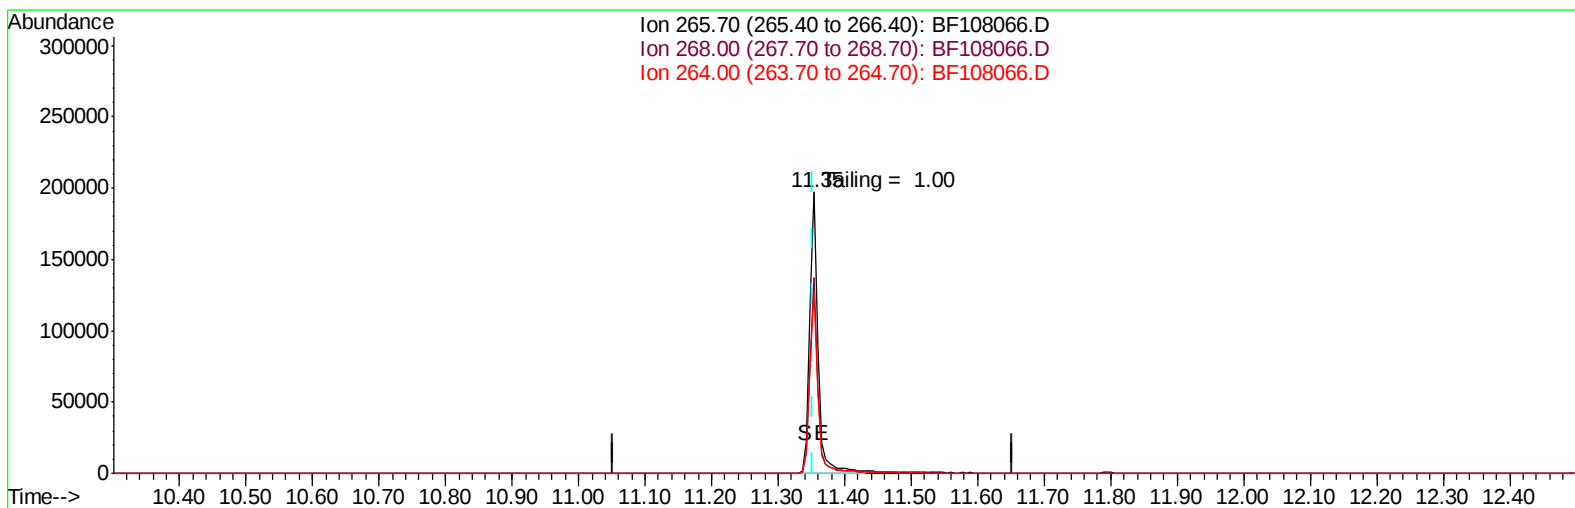

TIC: BF108066.D

(69) Pentachlorophenol (C)




11.354min (+0.000) 21423.46ng

response 180210

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	69.43
264.00	61.90	64.62
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080918\
 Data File : BF108066.D
 Acq On : 9 Aug 2018 22:23
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 04:27:06 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 12:24:24 2018
 Response via : Initial Calibration

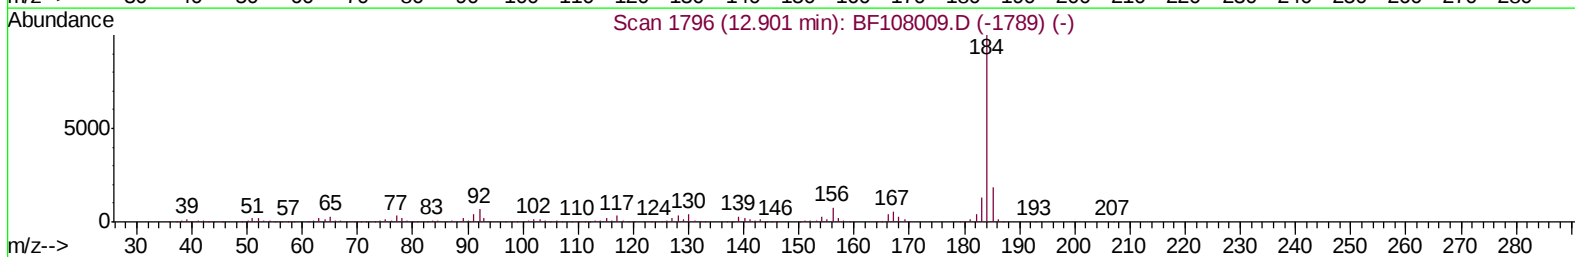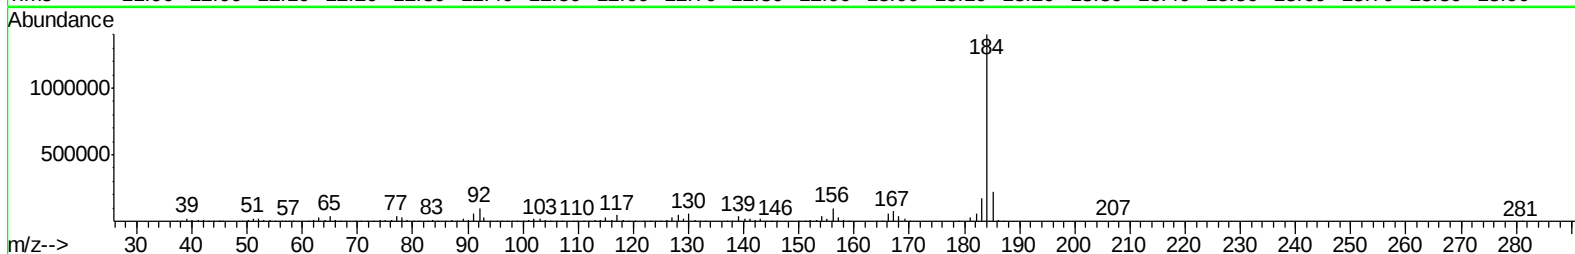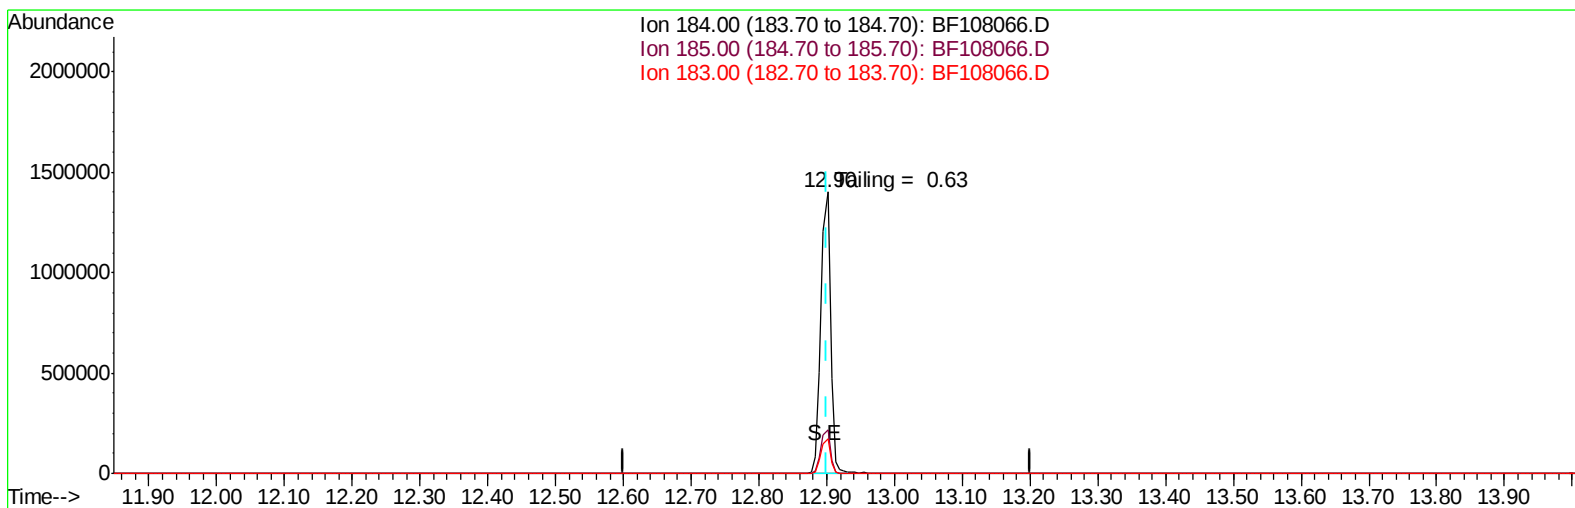

TIC: BF108066.D

(76) Benzidine

12.901min (+0.000) 17056.11ng

response 1340791

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.53
183.00	11.60	12.51
0.00	0.00	0.00