

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF080918\
 Data File : BF108059.D
 Acq On : 9 Aug 2018 18:17
 Operator : JU/SJ
 Sample : J4382-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 JTY-SB-03-04-05-1-11

Quant Time: Aug 10 01:40:47 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 12:24:24 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.02	152	289475	20.00	ng	0.00
21) Naphthalene-d8	8.30	136	1031194	20.00	ng	0.00
38) Acenaphthene-d10	10.06	164	435872	20.00	ng	0.00
63) Phenanthrene-d10	11.56	188	751247	20.00	ng	0.00
75) Chrysene-d12	14.21	240	713695	20.00	ng	0.00
86) Perylene-d12	15.78	264	539177	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	1583187	99.02	ng	0.01
7) Phenol-d6	6.63	99	2115253	99.55	ng	0.00
23) Nitrobenzene-d5	7.58	82	1342098	72.63	ng	0.00
41) 2,4,6-Tribromophenol	10.85	330	411647	94.68	ng	0.00
44) 2-Fluorobiphenyl	9.38	172	2004693	73.84	ng	0.00
78) Terphenyl-d14	13.15	244	1979795	70.53	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.77	163	410585	13.523	ng	Qvalue # 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF080918\
Data File : BF108059.D
Acq On : 9 Aug 2018 18:17
Operator : JU/SJ
Sample : J4382-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
JTY-SB-03-04-05-1-11

Quant Time: Aug 10 01:40:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 12:24:24 2018
Response via : Initial Calibration

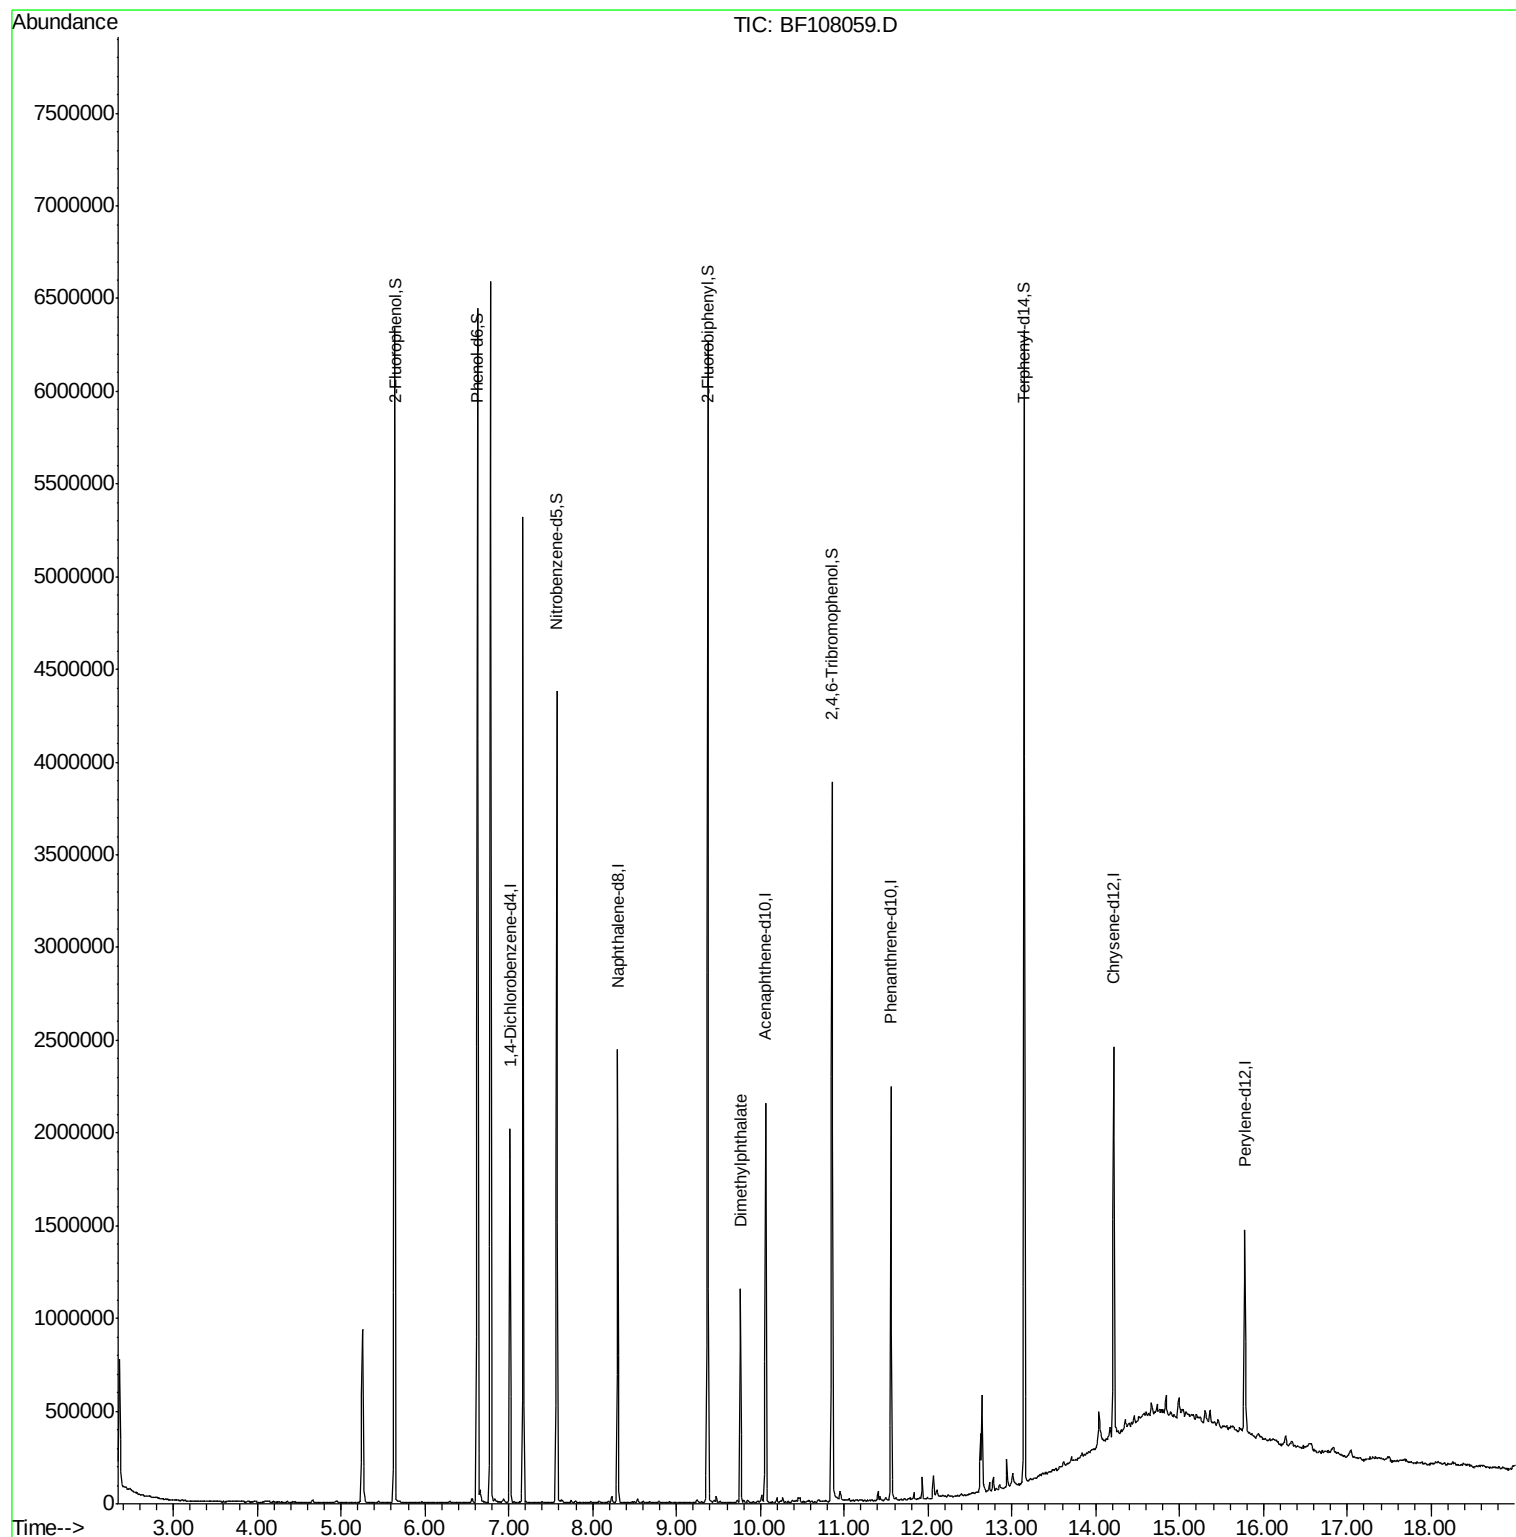




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.02 min Scan# 796
Delta R.T. 0.01 min
Lab File: BF108059.D
Acq: 9 Aug 2018 18:17

Instrument :
BNA_F
ClientSampleId :
JTY-SB-03-04-05-1-11

Tot Ion:152 Resp: 289475
Ion Ratio Lower Upper
152 100
150 152.7 124.6 186.8
115 57.7 50.1 75.1

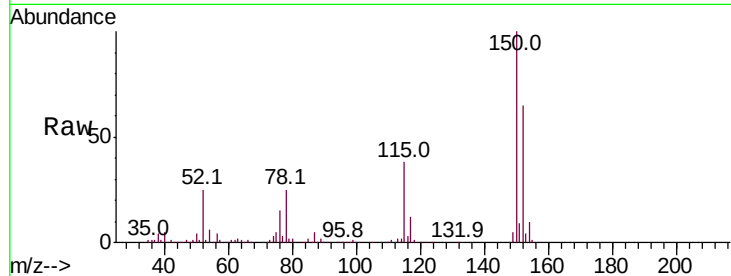


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

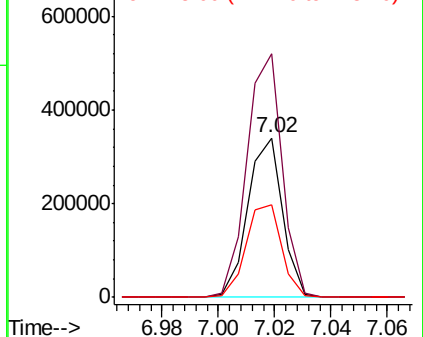



#5


2-Fluorophenol
Concen: 99.017 ng
RT: 5.64 min Scan# 562
Delta R.T. 0.01 min
Lab File: BF108059.D
Acq: 9 Aug 2018 18:17

Tgt Ion:112 Resp: 1583187
Ion Ratio Lower Upper
112 100
64 69.6 47.9 71.9
63 38.0 23.7 35.5#

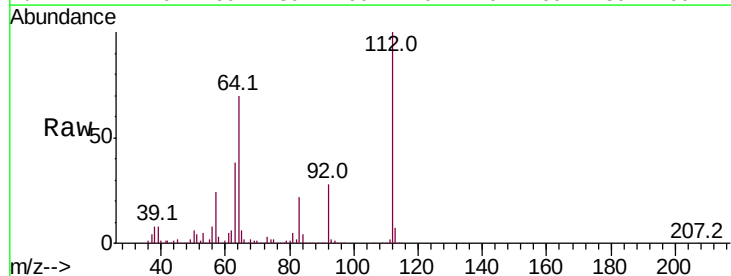

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

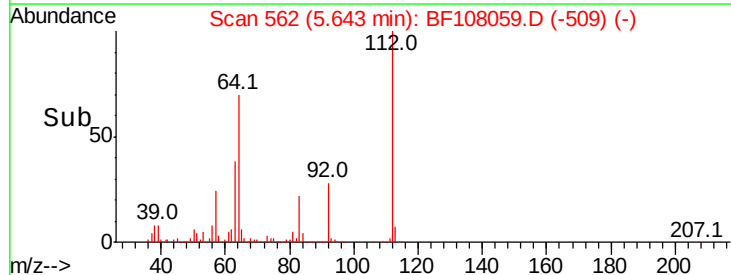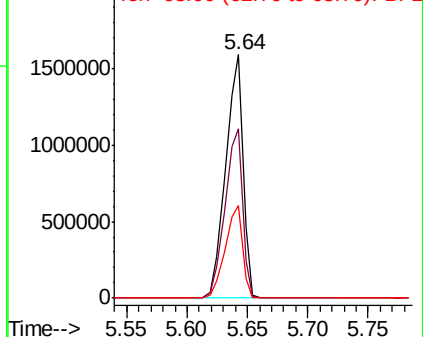



#7

Phenol-d6

Concen: 99.554 ng

RT: 6.63 min Scan# 730

Delta R.T. 0.00 min

Lab File: BF108059.D

Acq: 9 Aug 2018 18:17

Instrument :

BNA_F

ClientSampleId :

JTY-SB-03-04-05-1-11


Tot Ion: 99 Resp: 2115253

Ion Ratio Lower Upper




99 100

42 25.6 14.5 21.7#

71 39.5 25.4 38.0#

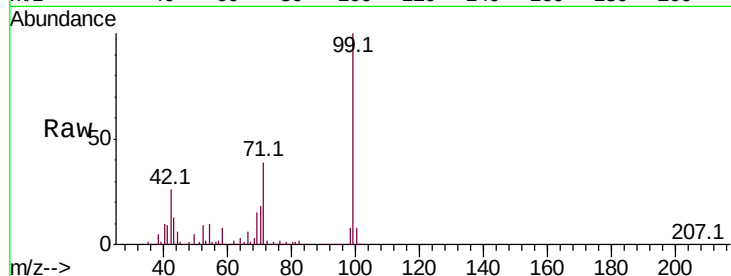

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

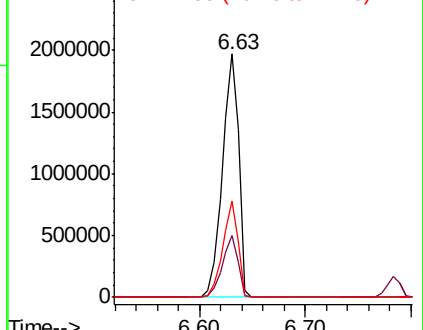

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.30 min Scan# 1014

Delta R.T. 0.00 min

Lab File: BF108059.D

Acq: 9 Aug 2018 18:17

Tgt Ion: 136 Resp: 1031194


Ion Ratio Lower Upper

136 100



137 10.8 8.9 13.3


54 9.7 6.6 9.8

68 6.2 5.0 7.4



Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

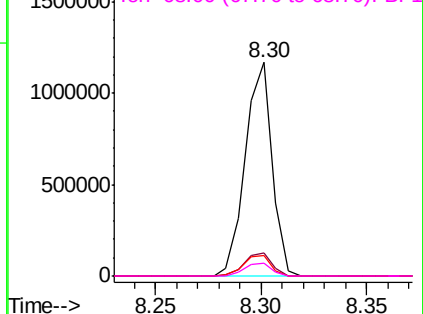







#23
 Nitrobenzene-d5
 Concen: 72.626 ng
 RT: 7.58 min Scan# 891
 Delta R.T. 0.00 min
 Lab File: BF108059.D
 Acq: 9 Aug 2018 18:17

Instrument :
 BNA_F
 ClientSampleId :
 JTY-SB-03-04-05-1-11

Tot Ion: 82 Resp: 1342098
 Ion Ratio Lower Upper
 82 100
 128 42.7 36.1 54.1
 54 60.8 41.4 62.2

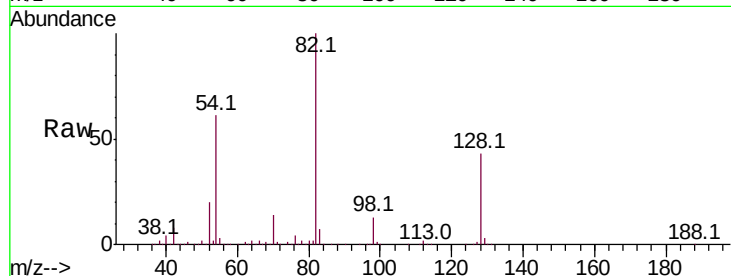


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1


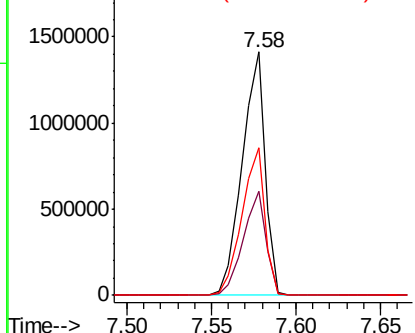



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 10.06 min Scan# 1313
 Delta R.T. -0.01 min
 Lab File: BF108059.D
 Acq: 9 Aug 2018 18:17

Tgt Ion: 164 Resp: 435872
 Ion Ratio Lower Upper
 164 100
 162 101.9 86.1 129.1
 160 46.0 38.3 57.5



Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

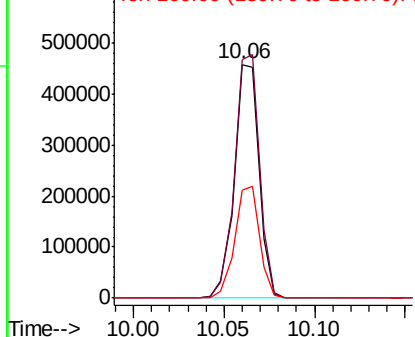


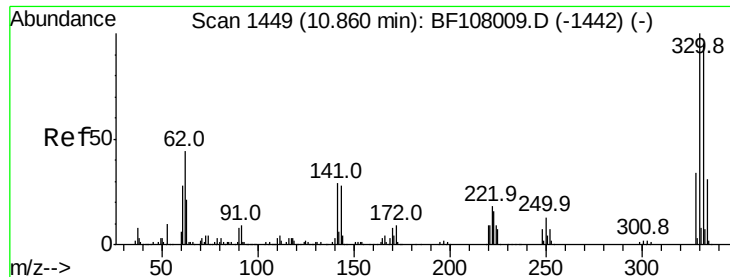




#41
 2,4,6-Tribromophenol
 Concen: 94.681 ng
 RT: 10.85 min Scan# 1448
 Delta R.T. -0.01 min
 Lab File: BF108059.D
 Acq: 9 Aug 2018 18:17

Instrument :
 BNA_F
 ClientSampleId :
 JTY-SB-03-04-05-1-11

Tot Ion:330 Resp: 411647
 Ion Ratio Lower Upper
 330 100
 332 97.2 77.0 115.6
 141 33.3 29.9 44.9

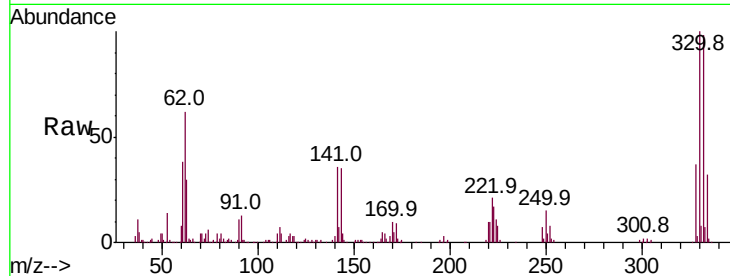


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

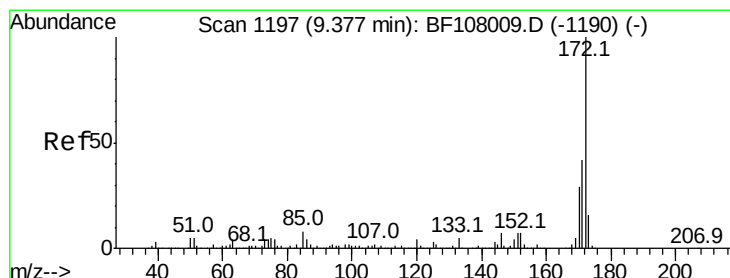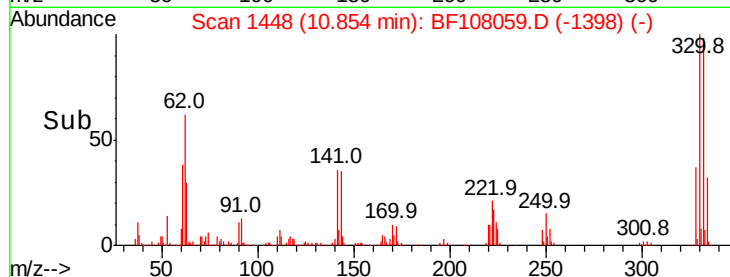
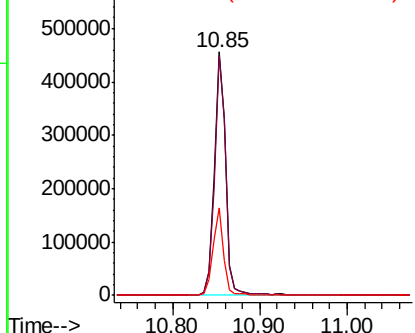



#44
 2-Fluorobiphenyl
 Concen: 73.840 ng
 RT: 9.38 min Scan# 1197
 Delta R.T. 0.00 min
 Lab File: BF108059.D
 Acq: 9 Aug 2018 18:17

Tgt Ion:172 Resp: 2004693
 Ion Ratio Lower Upper
 172 100
 171 38.5 29.7 44.5
 170 25.6 19.6 29.4

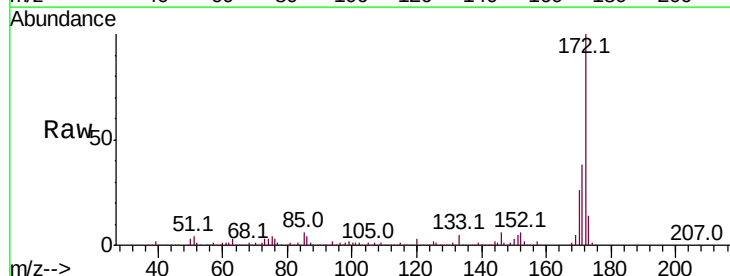

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

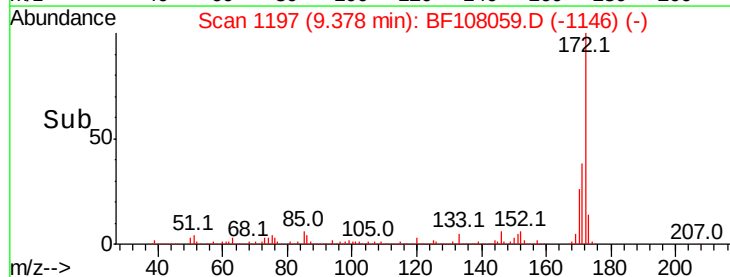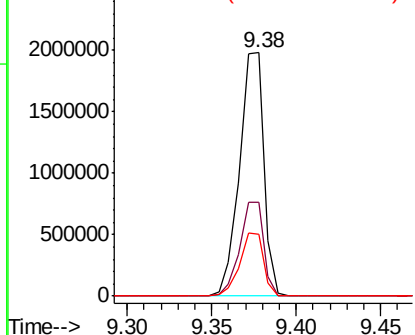



#49

Dimethylphthalate

Concen: 13.523 ng

RT: 9.77 min Scan# 1263

Delta R.T. -0.01 min

Lab File: BF108059.D

Acq: 9 Aug 2018 18:17

Instrument :

BNA_F

ClientSampleId :

JTY-SB-03-04-05-1-11


Tot Ion:163 Resp: 410585

Ion Ratio Lower Upper




163 100

194 4.2 2.7 4.1#

164 9.8 8.2 12.2



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

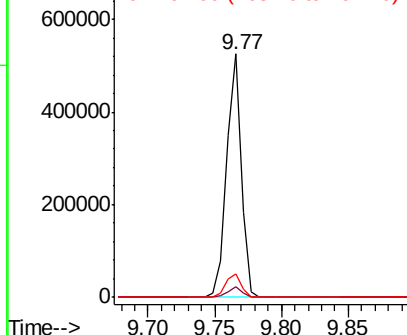

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.56 min Scan# 1568

Delta R.T. 0.00 min

Lab File: BF108059.D

Acq: 9 Aug 2018 18:17


Tgt Ion:188 Resp: 751247

Ion Ratio Lower Upper



188 100


94 8.5 8.5 12.7#

80 9.7 9.2 13.8



Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

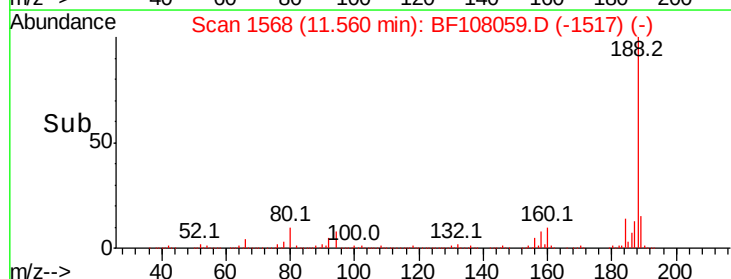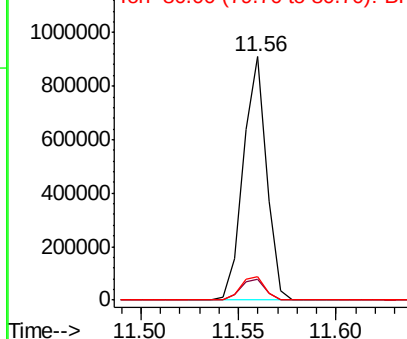

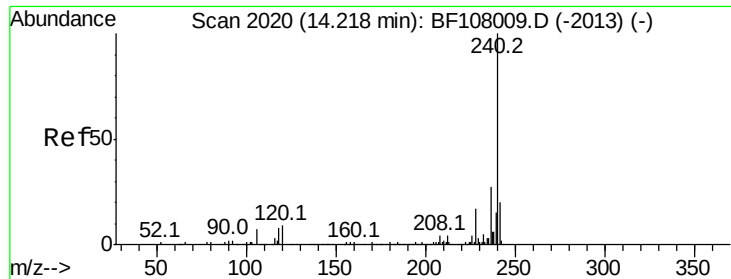

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.21 min Scan# 2019

Delta R.T. -0.01 min

Lab File: BF108059.D

Acq: 9 Aug 2018 18:17

Instrument :

BNA_F

ClientSampleId :

JTY-SB-03-04-05-1-11


Tot Ion:240 Resp: 713695

Ion Ratio Lower Upper

240 100

120 11.0 9.5 14.3




236 27.3 20.7 31.1

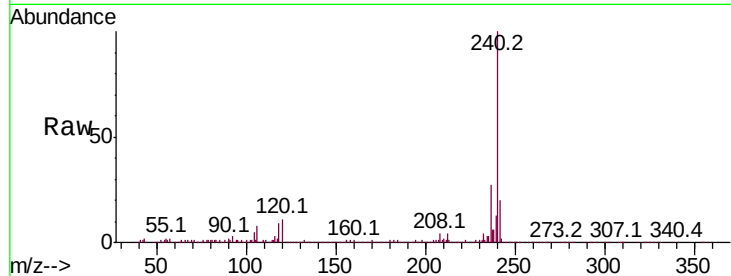

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

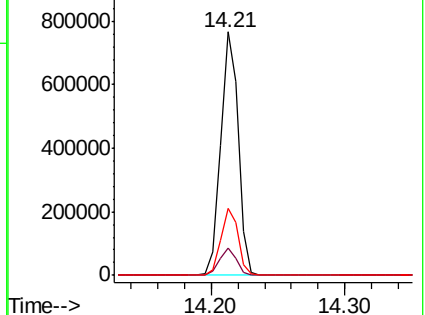

#78

Terphenyl-d14

Concen: 70.531 ng

RT: 13.15 min Scan# 1838

Delta R.T. 0.00 min

Lab File: BF108059.D

Acq: 9 Aug 2018 18:17


Tgt Ion:244 Resp: 1979795

Ion Ratio Lower Upper

244 100

212 8.1 5.4 8.0#



122 11.3 11.0 16.4




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

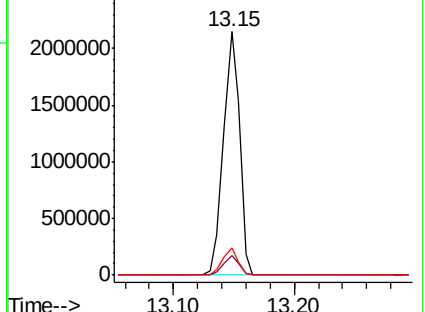

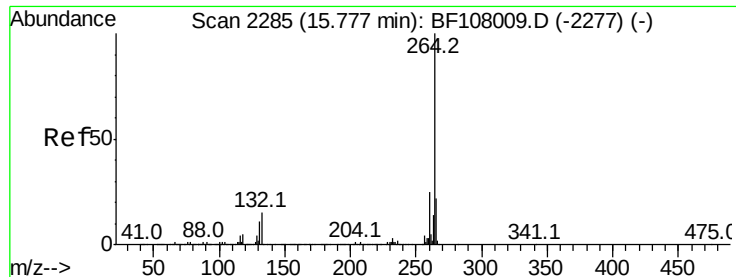

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.78 min Scan# 2285
 Delta R.T. 0.00 min
 Lab File: BF108059.D
 Acq: 9 Aug 2018 18:17

Instrument :
 BNA_F
 ClientSampleId :
 JTY-SB-03-04-05-1-11

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.8	19.2	28.8
265	21.6	17.5	26.3

