

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080918\
 Data File : BF108047.D
 Acq On : 9 Aug 2018 12:45
 Operator : JU/SJ
 Sample : J4275-05 2X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-02-080718-C

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.237	489	493	497	rBV	358080	356175	12.22%	1.080%
2	5.625	555	559	562	rBV	2154183	1852619	63.59%	5.617%
3	6.619	723	728	731	rBV	2512564	2124861	72.93%	6.443%
4	6.778	751	755	758	rBV	2425575	2074092	71.19%	6.289%
5	7.013	791	795	799	rBV	2343584	1881765	64.59%	5.706%
6	7.166	818	821	825	rVB	1737726	1551492	53.25%	4.704%
7	7.572	885	890	893	rBV	1468182	1325325	45.49%	4.018%
8	8.295	1009	1013	1017	rBV	3041560	2527865	86.76%	7.665%
9	9.372	1191	1196	1199	rBV	3194579	2636298	90.48%	7.993%
10	9.442	1205	1208	1212	rBV3	30011	40735	1.40%	0.124%
11	9.760	1259	1262	1266	rBV	225923	180137	6.18%	0.546%
12	9.925	1286	1290	1292	rBV4	37466	34757	1.19%	0.105%
13	9.972	1294	1298	1300	rVB2	63250	58490	2.01%	0.177%
14	10.060	1306	1313	1317	rBV2	3267824	2913547	100.00%	8.834%
15	10.089	1317	1318	1327	rVB4	36811	55556	1.91%	0.168%
16	10.378	1363	1367	1369	rBV4	38958	49498	1.70%	0.150%
17	10.472	1379	1383	1387	rVB4	54190	69580	2.39%	0.211%
18	10.695	1416	1421	1423	rBV6	35385	54135	1.86%	0.164%
19	10.748	1428	1430	1437	rVB8	21799	39178	1.34%	0.119%
20	10.848	1443	1447	1458	rBV	1594395	1448597	49.72%	4.392%
21	10.966	1462	1467	1474	rVB4	75831	125603	4.31%	0.381%
22	11.189	1503	1505	1510	rVB5	29310	36054	1.24%	0.109%
23	11.354	1530	1533	1536	rBV4	30228	34359	1.18%	0.104%
24	11.401	1538	1541	1543	rBV	51396	46984	1.61%	0.142%
25	11.430	1543	1546	1549	rBV	68007	70937	2.43%	0.215%
26	11.560	1563	1568	1570	rBV	2887051	2772840	95.17%	8.407%
27	11.578	1570	1571	1575	rVB	140870	99752	3.42%	0.302%
28	11.783	1603	1606	1609	rBV2	41433	37536	1.29%	0.114%
29	11.901	1622	1626	1629	rVB2	54446	75649	2.60%	0.229%
30	12.060	1650	1653	1656	rBV	145476	144726	4.97%	0.439%
31	12.613	1744	1747	1748	rBV2	30937	35786	1.23%	0.109%
32	12.772	1771	1774	1777	rBV	204581	188106	6.46%	0.570%
33	12.813	1778	1781	1783	rVB	106407	90452	3.10%	0.274%
34	13.007	1808	1814	1819	rBV2	240409	314005	10.78%	0.952%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080918\
Data File : BF108047.D
Acq On : 9 Aug 2018 12:45
Operator : JU/SJ
Sample : J4275-05 2X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-080718-C

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	13.142	1833	1837	1840	rBV	2907933	2379316	81.66%	7.214%
36	13.330	1867	1869	1871	rBV3	45160	36958	1.27%	0.112%
37	13.360	1871	1874	1876	rVV	94612	70905	2.43%	0.215%
38	13.701	1930	1932	1935	rBV	98990	90369	3.10%	0.274%
39	14.036	1986	1989	1996	rBV3	123102	231100	7.93%	0.701%
40	14.213	2014	2019	2022	rBV	2343885	2366239	81.22%	7.175%
41	14.354	2040	2043	2046	rBV2	121537	129450	4.44%	0.392%
42	14.660	2093	2095	2099	rVB	148301	118610	4.07%	0.360%
43	15.360	2212	2214	2220	rVB	179440	193208	6.63%	0.586%
44	15.777	2279	2285	2291	rVB	1408118	2017389	69.24%	6.117%


Sum of corrected areas: 32981035

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF080918\
Data File : BF108047.D
Acq On : 9 Aug 2018 12:45
Operator : JU/SJ
Sample : J4275-05 2X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-080718-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

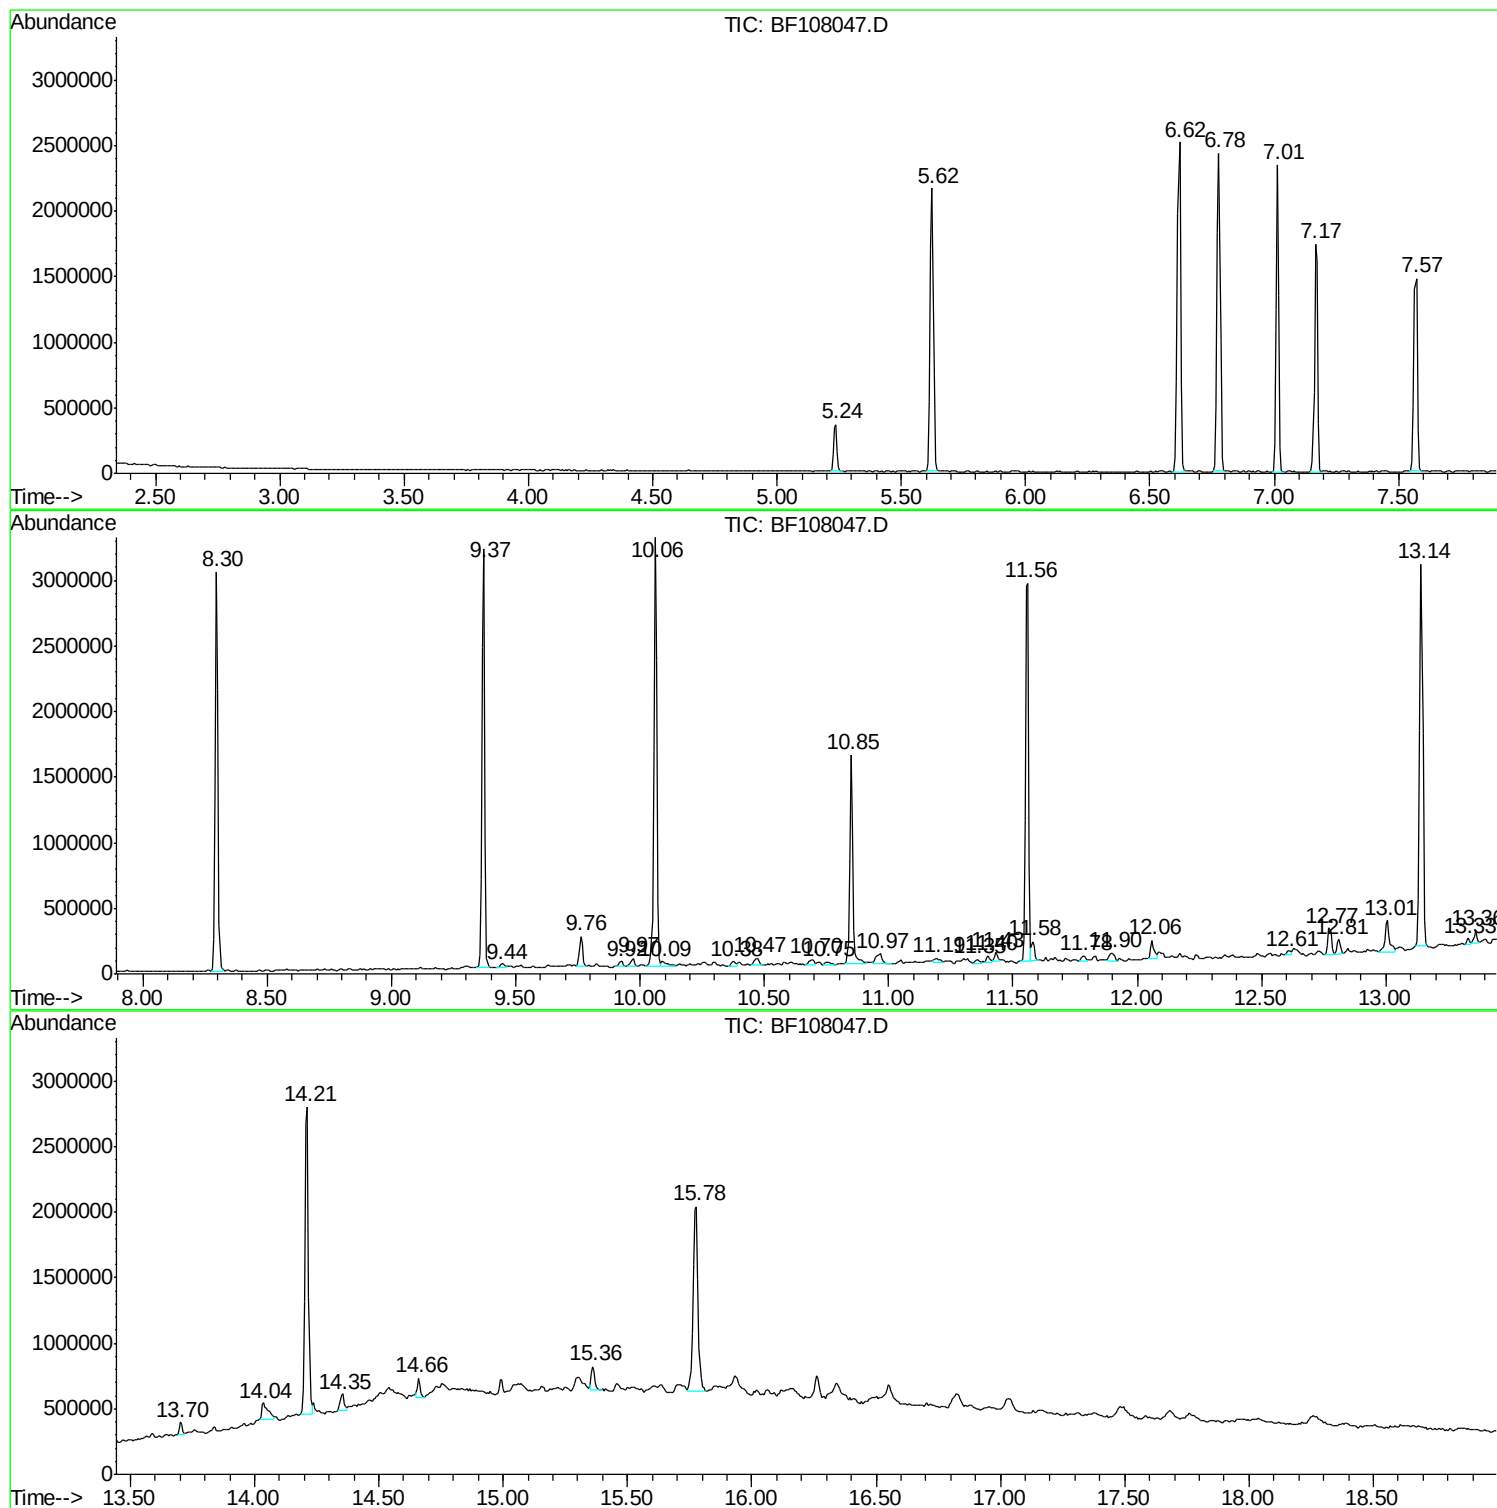

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF080918\
Data File : BF108047.D
Acq On : 9 Aug 2018 12:45
Operator : JU/SJ
Sample : J4275-05 2X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-080718-C










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.24	3.79 ng	356175	1,4-Dichlorobenzene-d4	7.01

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	16
3		1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
4		Butane	58	C4H10	000106-97-8	9
5		4-Penten-2-one, 4-methyl-	98	C6H10O	003744-02-3	9

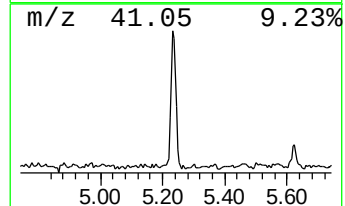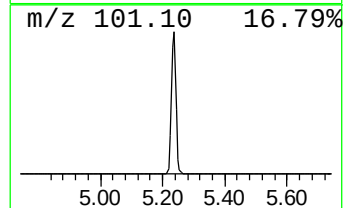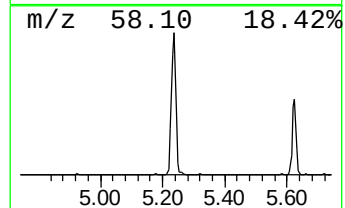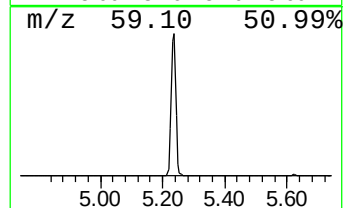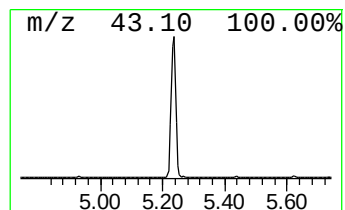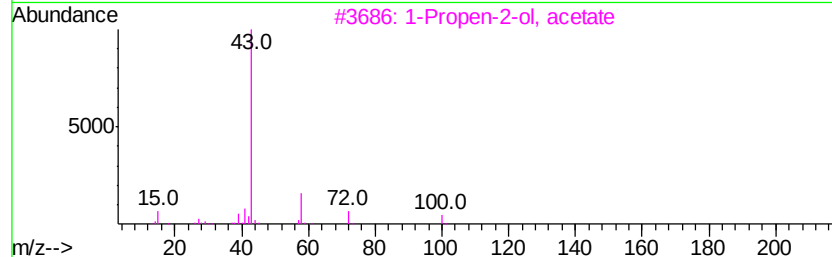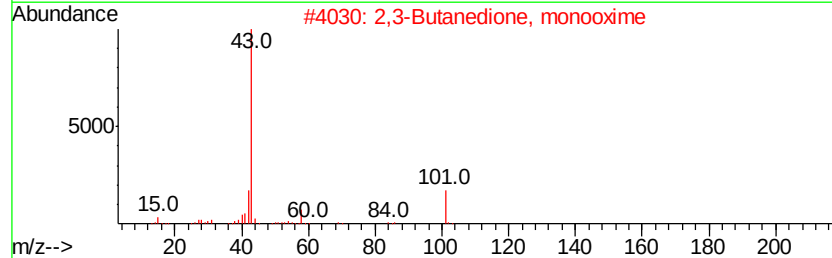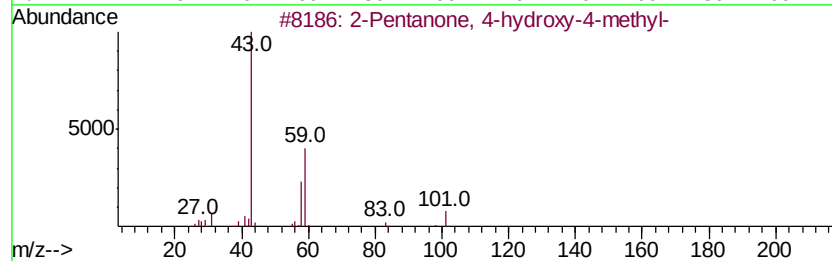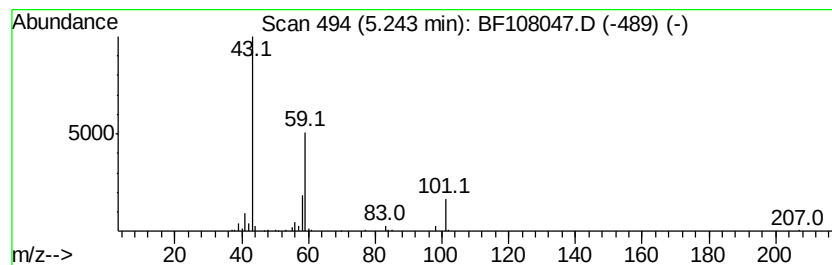

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF080918\
Data File : BF108047.D
Acq On : 9 Aug 2018 12:45
Operator : JU/SJ
Sample : J4275-05 2X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-080718-C










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.78 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.78	22.04 ng	2074090	1,4-Dichlorobenzene-d4	7.01

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10
4		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

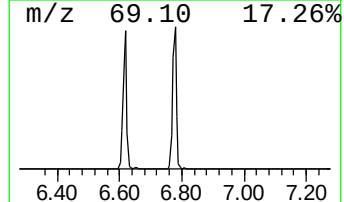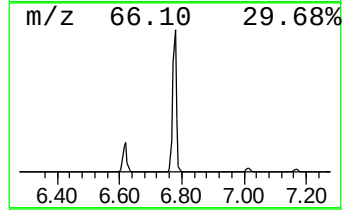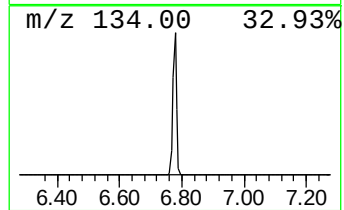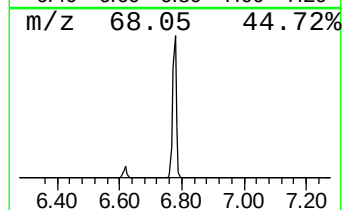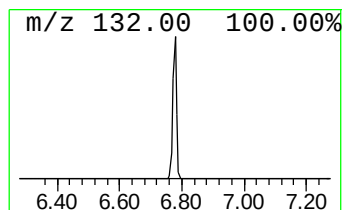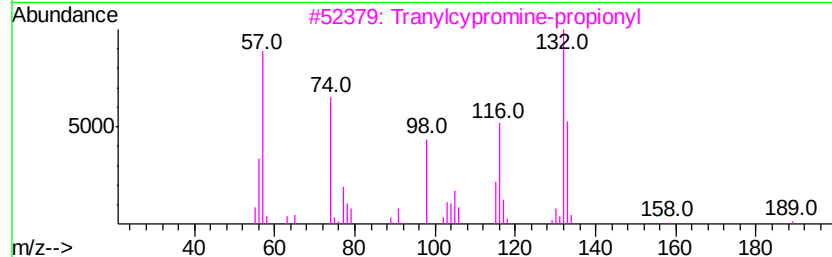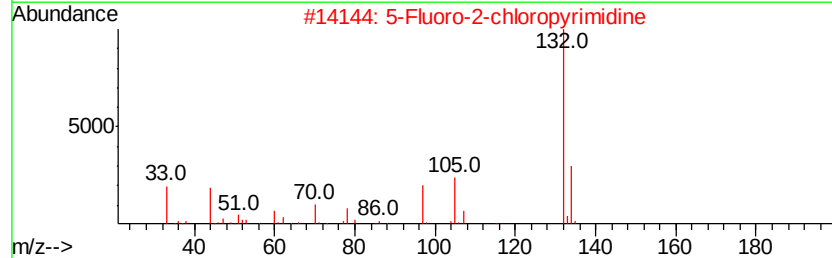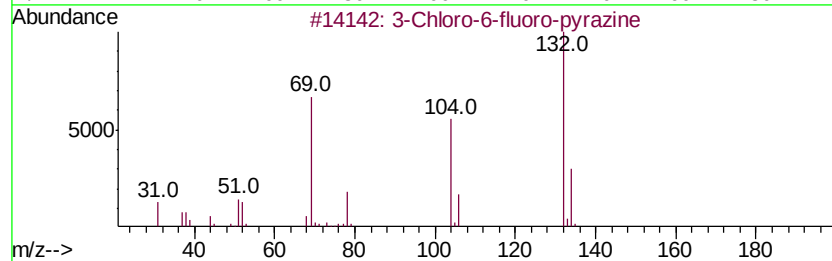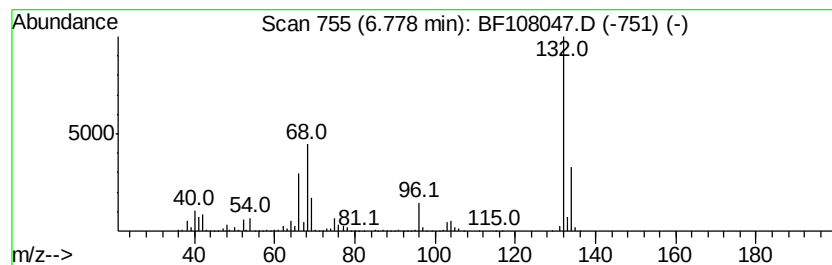

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080918\
Data File : BF108047.D
Acq On : 9 Aug 2018 12:45
Operator : JU/SJ
Sample : J4275-05 2X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-080718-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.24	3.8	ng	356175	1	7.01	1881770	20.0
unknown6.78	6.78	22.0	ng	2074090	1	7.01	1881770	20.0